

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026609.D
 Acq On : 30 Jun 2022 15:56
 Operator : SY/MD
 Sample : N3534-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AG7

Quant Time: Jul 01 00:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	380021	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	377697	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	164684	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	125083	40.378	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.760%
7) Chloroethane-d5	1.584	69	115838	43.602	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.200%
11) 1,1-Dichloroethene-d2	2.121	63	185185	31.734	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.460%
21) 2-Butanone-d5	3.915	46	134410	86.663	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.660%
24) Chloroform-d	4.362	84	264165	44.164	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.320%
26) 1,2-Dichloroethane-d4	5.040	65	153258	45.029	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.060%
32) Benzene-d6	5.060	84	508929	44.313	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.620%
36) 1,2-Dichloropropane-d6	6.076	67	168512	46.582	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.160%
41) Toluene-d8	7.320	98	415977	41.236	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.480%
43) trans-1,3-Dichloroprop...	7.625	79	58715	40.426	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.860%
47) 2-Hexanone-d5	8.092	63	107233	85.708	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.710%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	236467	45.273	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.540%
66) 1,2-Dichlorobenzene-d4	11.622	152	162363	50.376	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.760%
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.249	75	18550	6.290	ug/L	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026609.D
Acq On : 30 Jun 2022 15:56
Operator : SY/MD
Sample : N3534-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AG7


Quant Time: Jul 01 00:23:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 01 00:19:36 2022
Response via : Initial Calibration

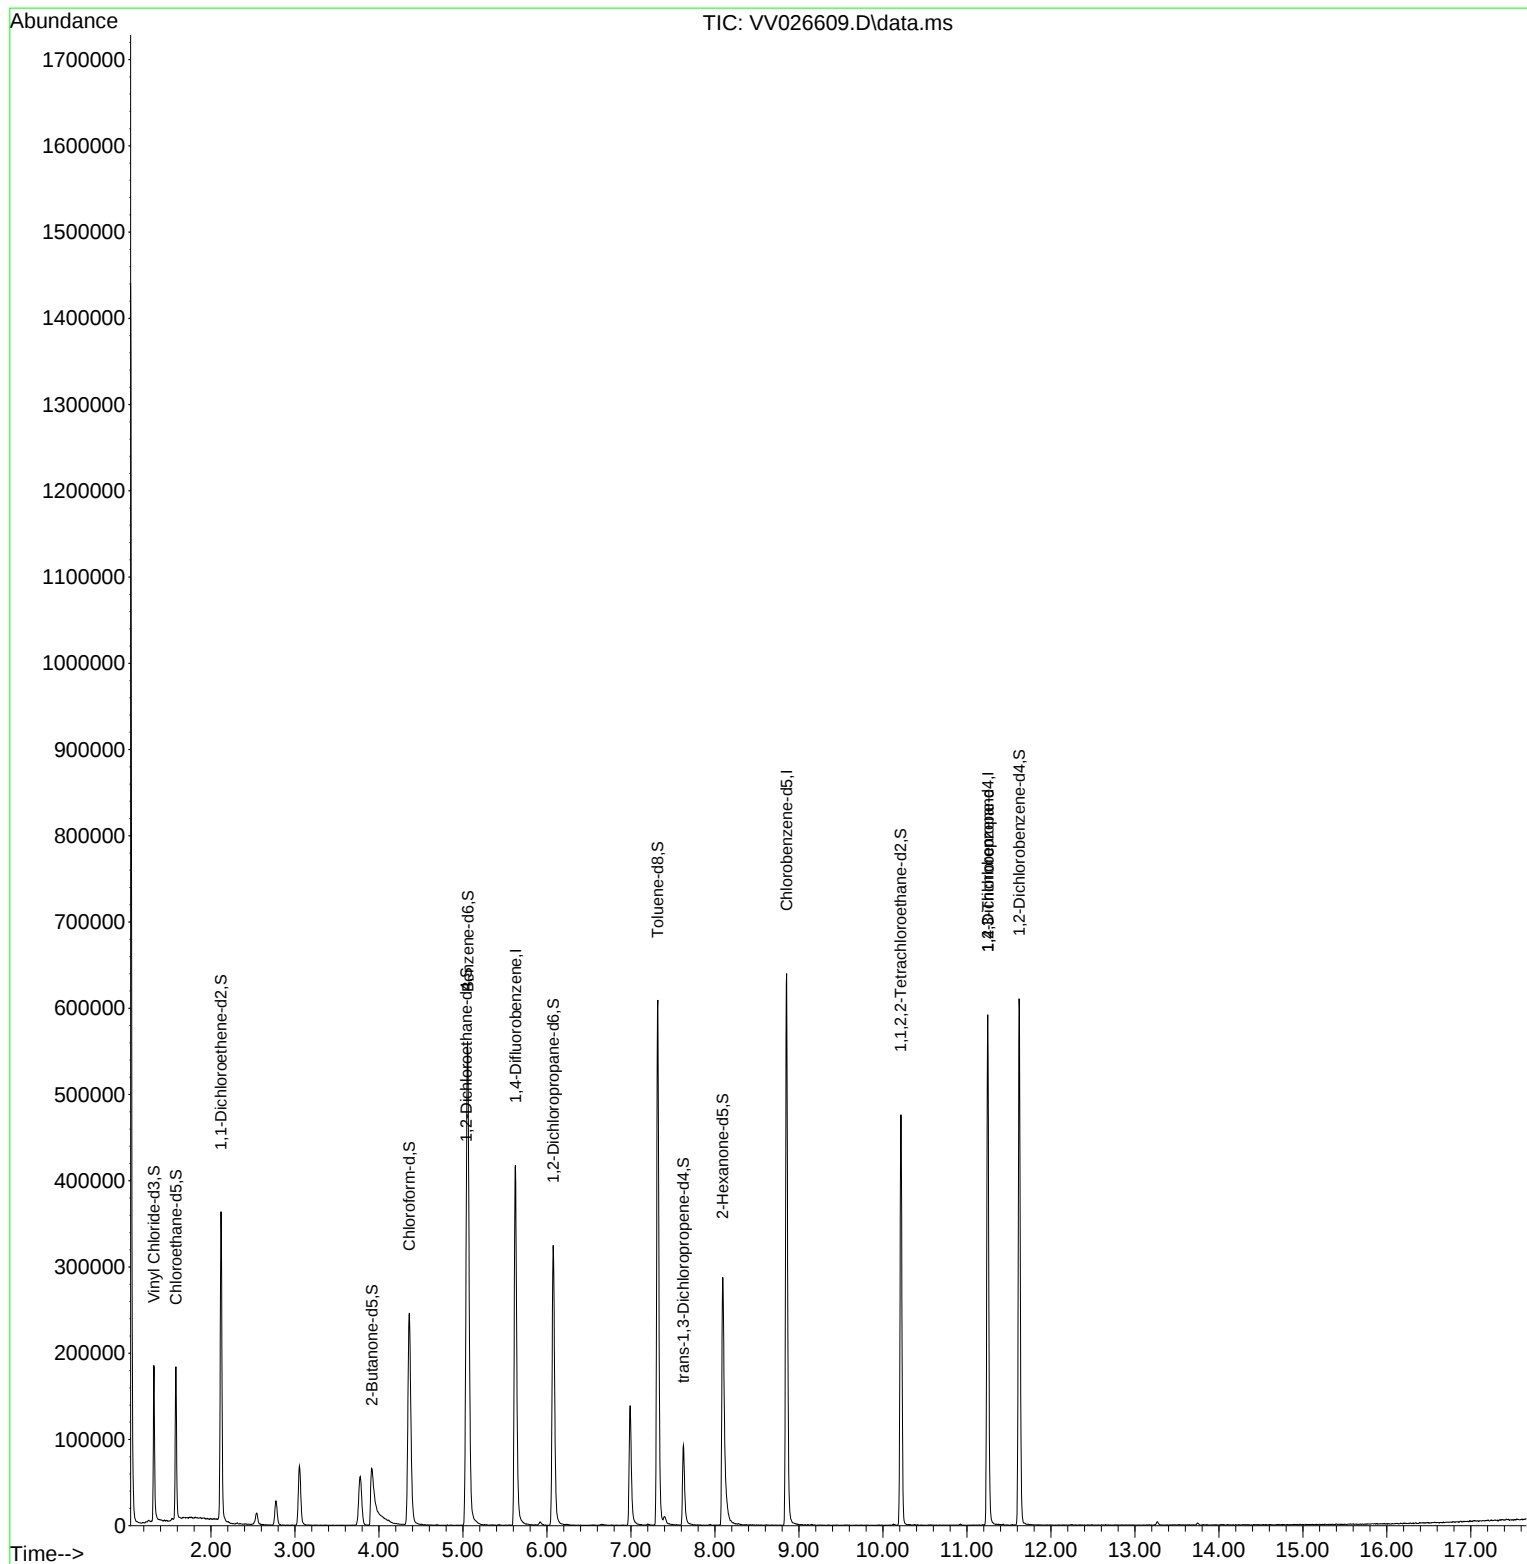

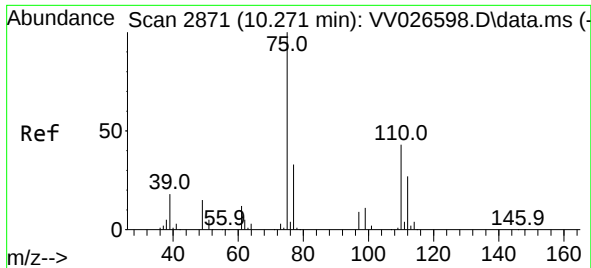

#61
 1,2,3-Trichloropropane
 Concen: 6.290 ug/L
 RT: 11.249 min Scan# 31
 Delta R.T. 0.978 min
 Lab File: VV026609.D
 Acq: 30 Jun 2022 15:56

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AG7

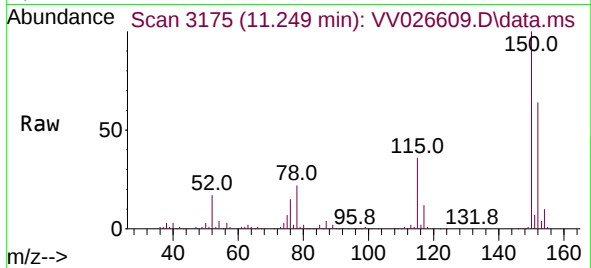

Tgt Ion: 75	Resp:	18550
Ion	Ratio	Lower Upper
75	100	
77	28.7	25.8 38.6
110	1.8	32.8 49.2#

