


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026601.D
Acq On : 30 Jun 2022 12:44
Operator : SY/MD
Sample : N3521-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JY3

Manual IntegrationsAPPROVED

Quant Time: Jul 01 00:21:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 01 00:19:36 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

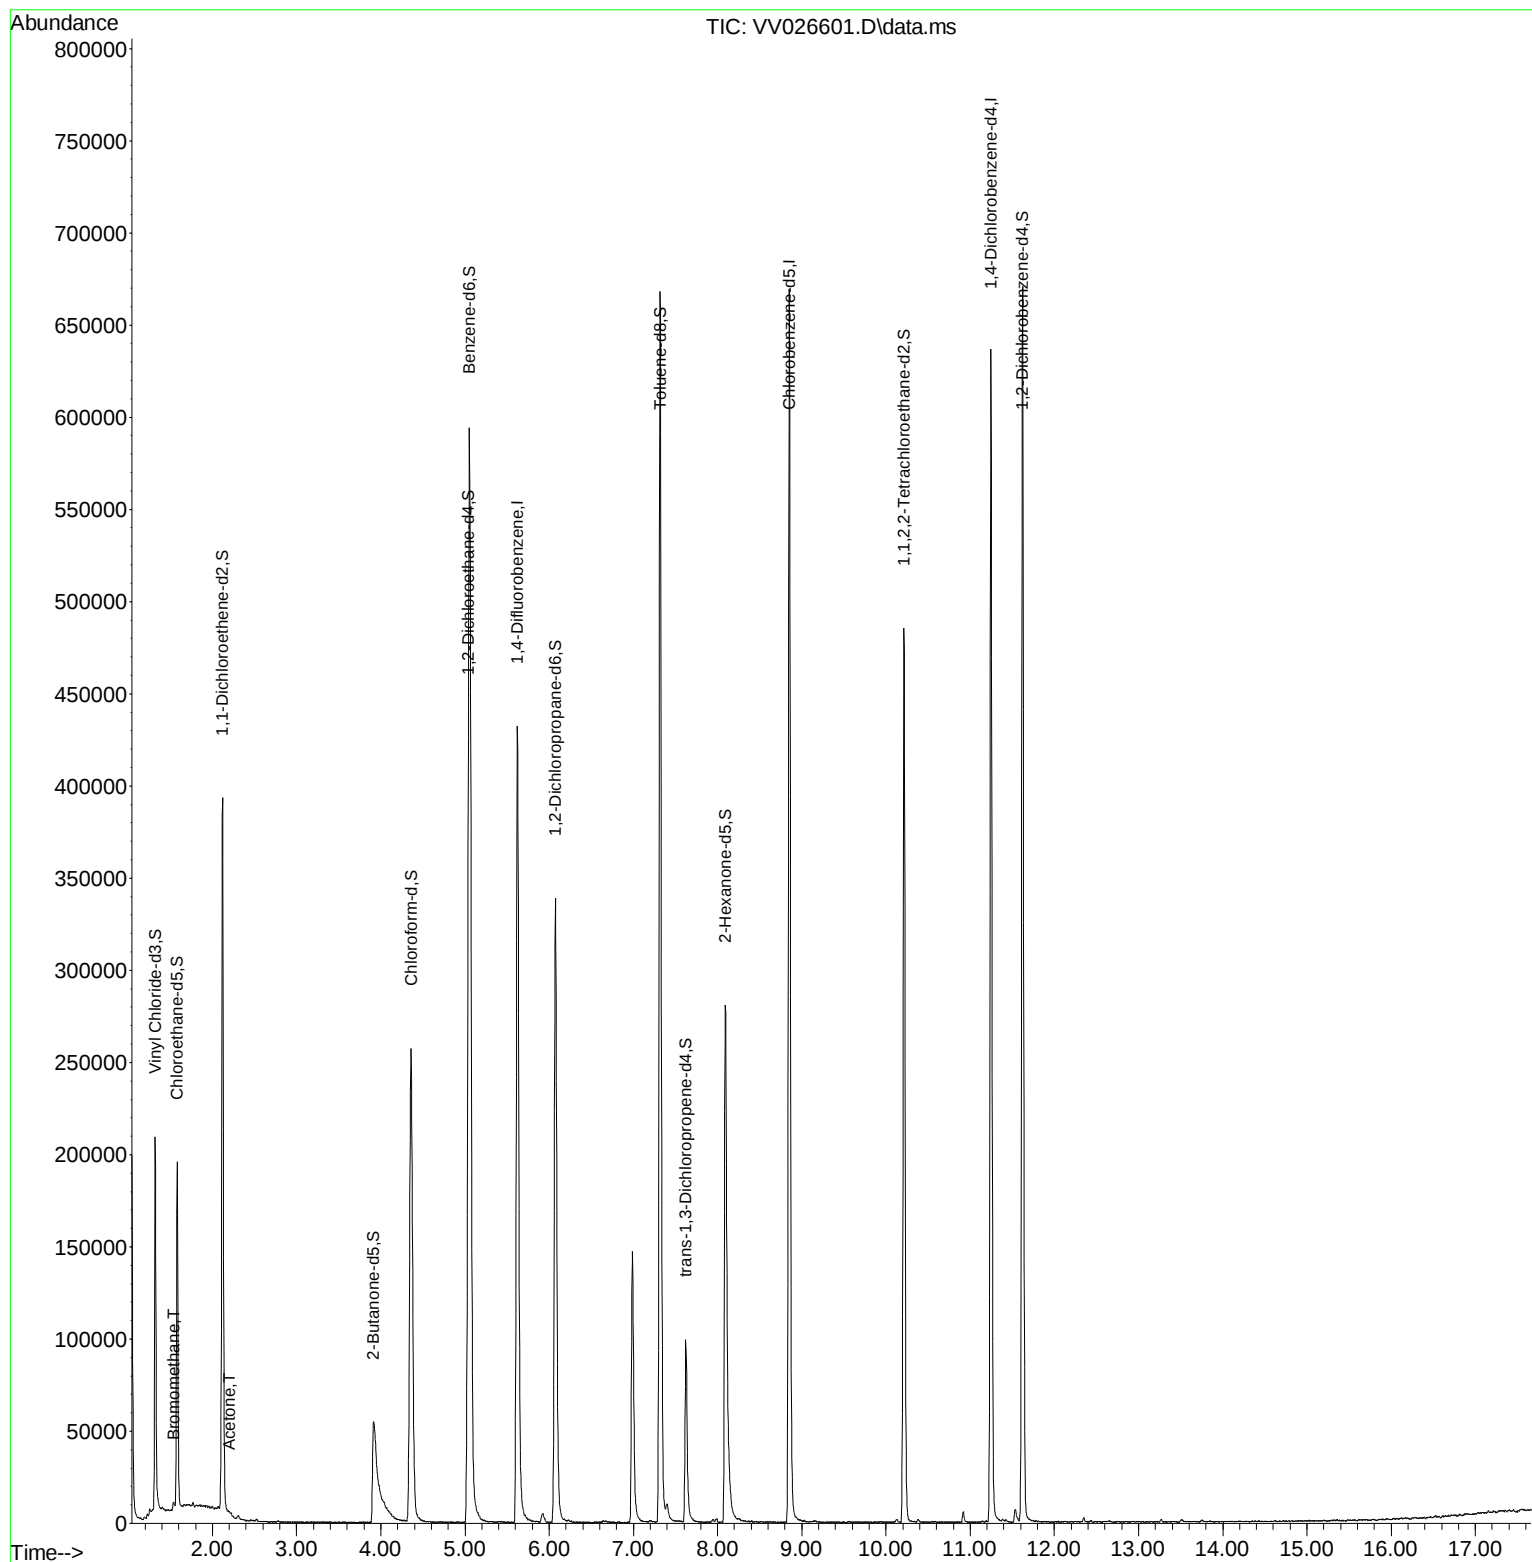




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026601.D
Acq On : 30 Jun 2022 12:44
Operator : SY/MD
Sample : N3521-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JY3

Manual IntegrationsAPPROVED

Quant Time: Jul 01 00:21:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 01 00:19:36 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

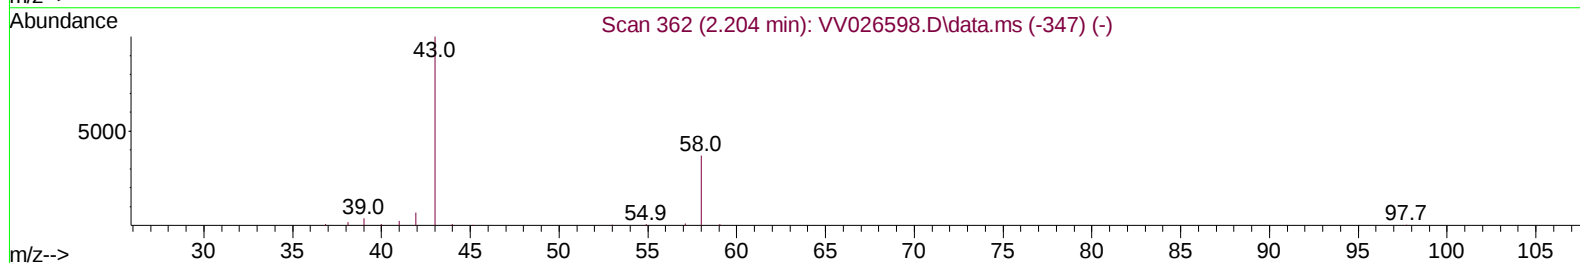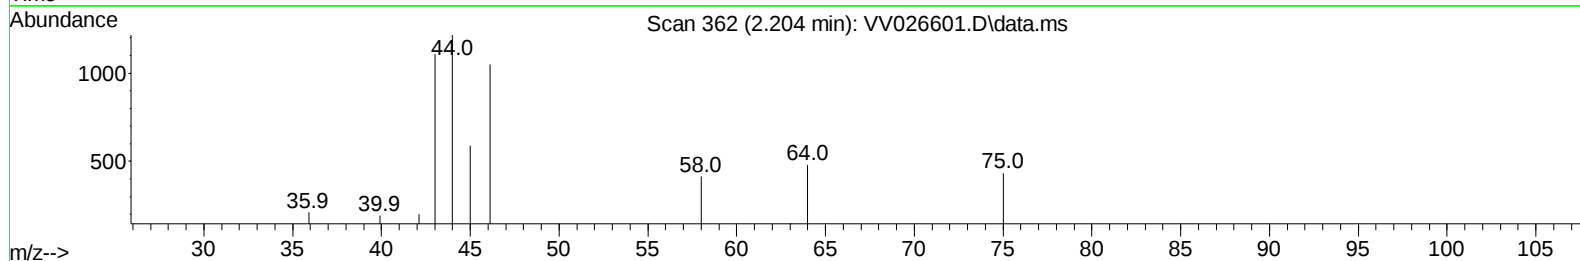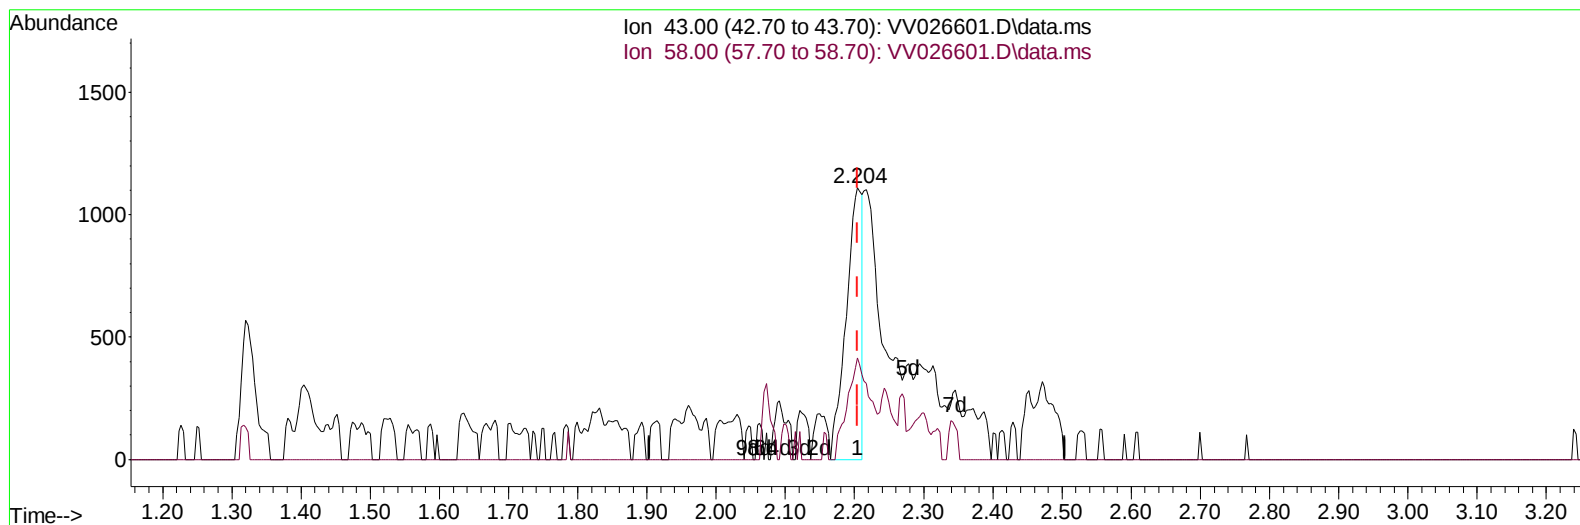

TIC: VV026601.D\data.ms

(13) Acetone (T)

2.204min (+ 0.000) 1.53 ug/L

response 1769

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	53.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026601.D
Acq On : 30 Jun 2022 12:44
Operator : SY/MD
Sample : N3521-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JY3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

Quant Time: Jul 01 00:21:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 01 00:19:36 2022
Response via : Initial Calibration

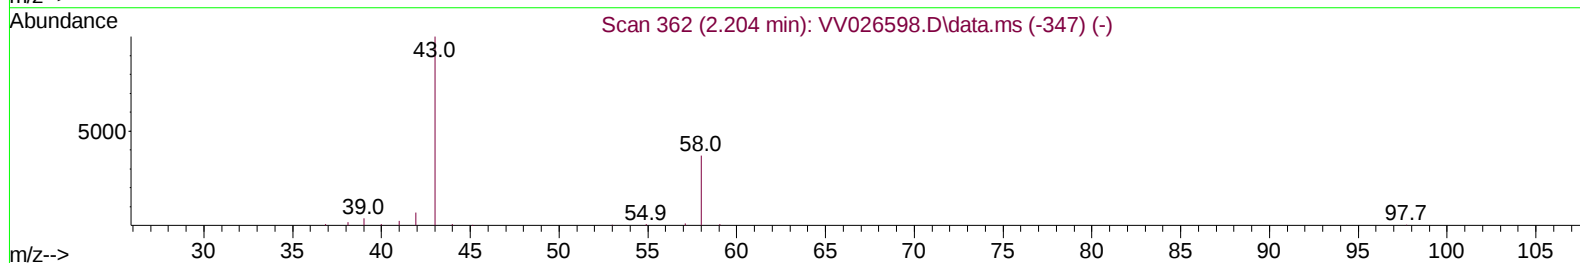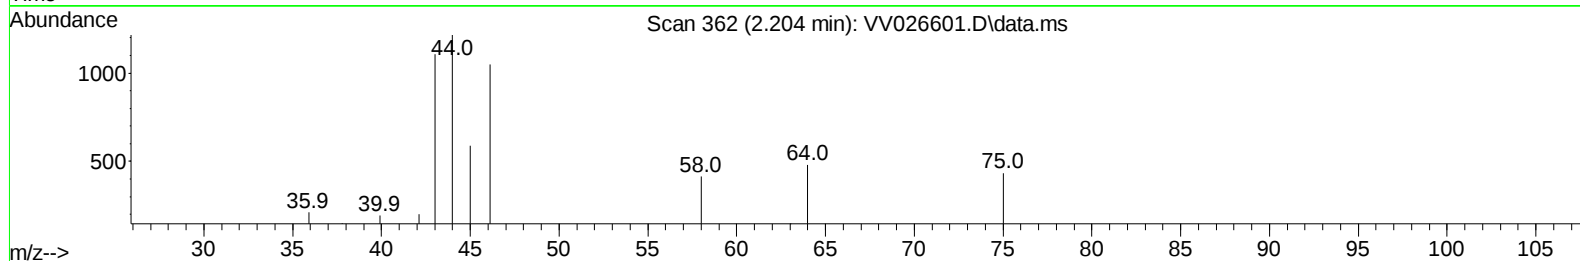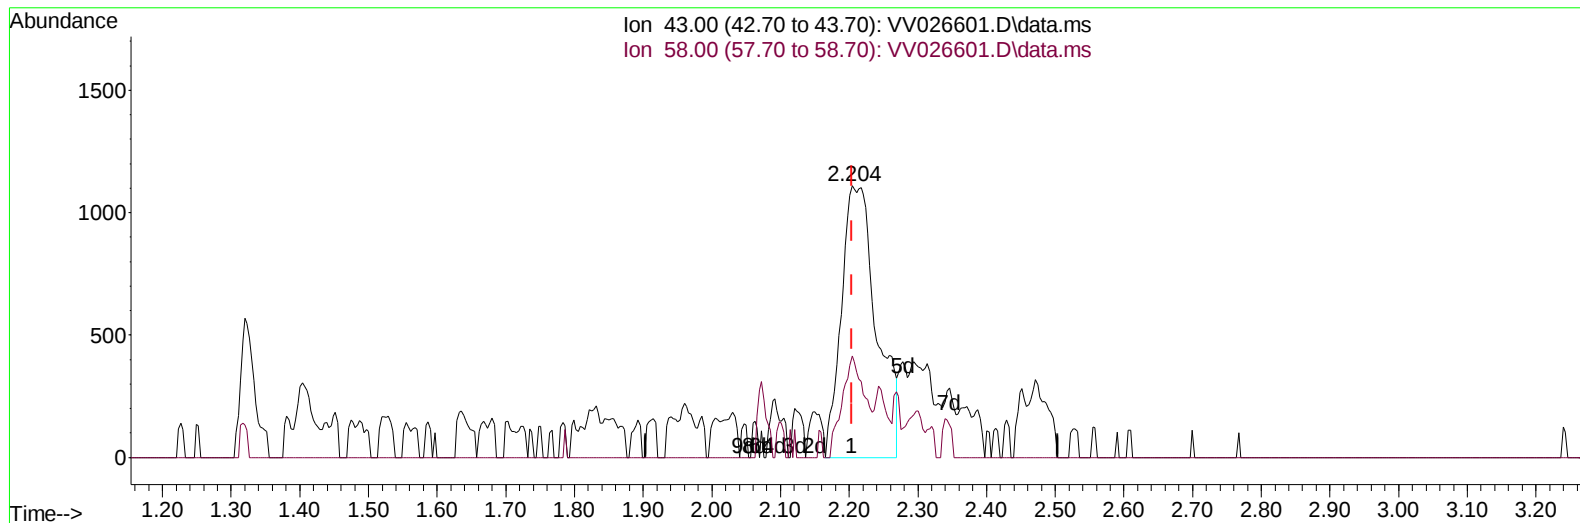

TIC: VV026601.D\data.ms

(13) Acetone (T)

2.204min (+ 0.000) 3.42 ug/L m

response 3946

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	23.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026601.D
 Acq On : 30 Jun 2022 12:44
 Operator : SY/MD
 Sample : N3521-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JY3

Manual IntegrationsAPPROVED

Quant Time: Jul 01 00:21:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.622	114		388174	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		386290	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		177149	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.320	65		136878	43.258	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	86.520%	
7) Chloroethane-d5	1.580	69		124208	45.770	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	91.540%	
11) 1,1-Dichloroethene-d2	2.121	63		204222	34.262	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	68.520%	
21) 2-Butanone-d5	3.915	46		134547	84.929	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	84.930%	
24) Chloroform-d	4.358	84		277484	45.416	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	90.840%	
26) 1,2-Dichloroethane-d4	5.040	65		162622	46.777	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	93.560%	
32) Benzene-d6	5.056	84		539520	45.931	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	91.860%	
36) 1,2-Dichloropropane-d6	6.075	67		173321	46.846	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	93.700%	
41) Toluene-d8	7.317	98		447687	43.392	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	86.780%	
43) trans-1,3-Dichloroprop...	7.622	79		60796	40.928	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	81.860%	
47) 2-Hexanone-d5	8.091	63		105654	82.568	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	82.570%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		235787	44.138	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	88.280%	
66) 1,2-Dichlorobenzene-d4	11.622	152		174103	50.217	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	100.440%	
Target Compounds							
6) Bromomethane	1.539	94		2405	1.045	ug/L	98
13) Acetone	2.204	43		3946m	3.421	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed