


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026611.D
Acq On : 30 Jun 2022 16:47
Operator : SY/MD
Sample : N3521-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0JT3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

Quant Time: Jul 01 00:23:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 01 00:19:36 2022
Response via : Initial Calibration

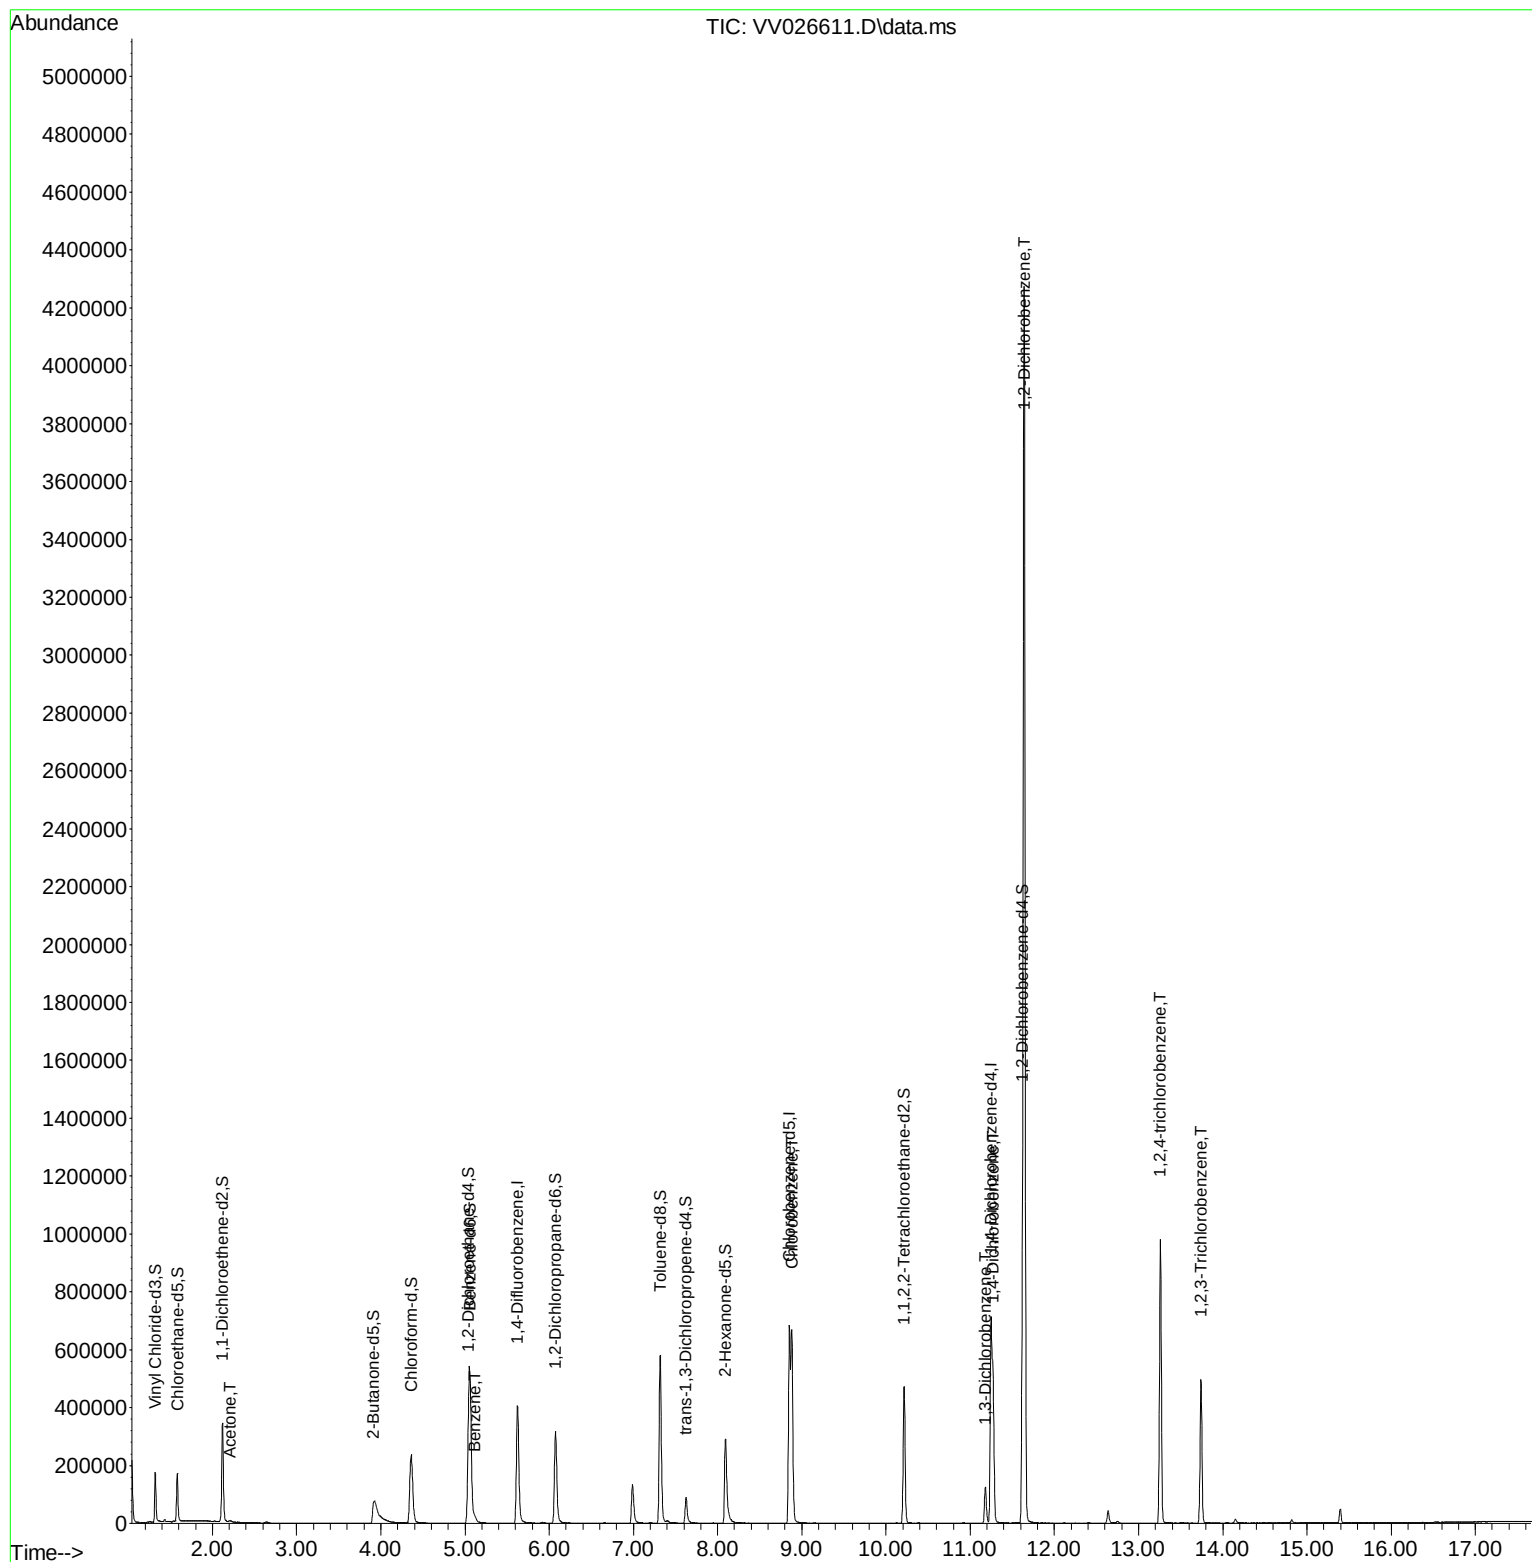




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026611.D
 Acq On : 30 Jun 2022 16:47
 Operator : SY/MD
 Sample : N3521-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JT3

Manual IntegrationsAPPROVED

Quant Time: Jul 01 00:23:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

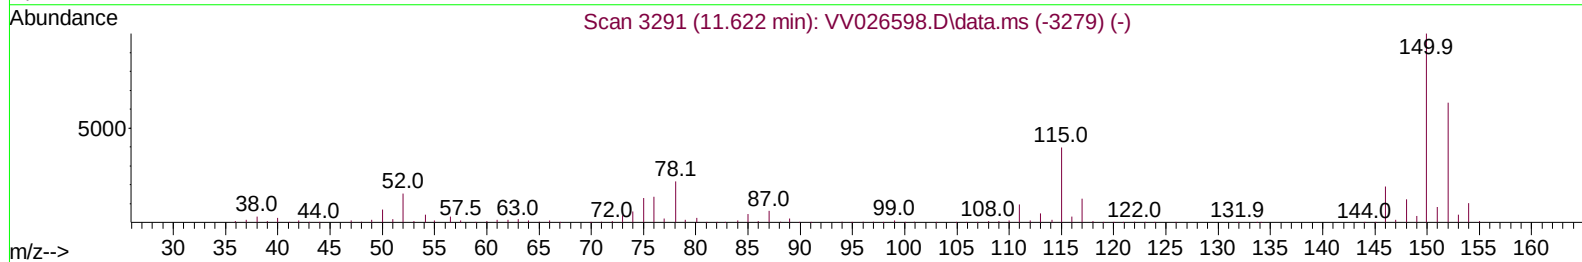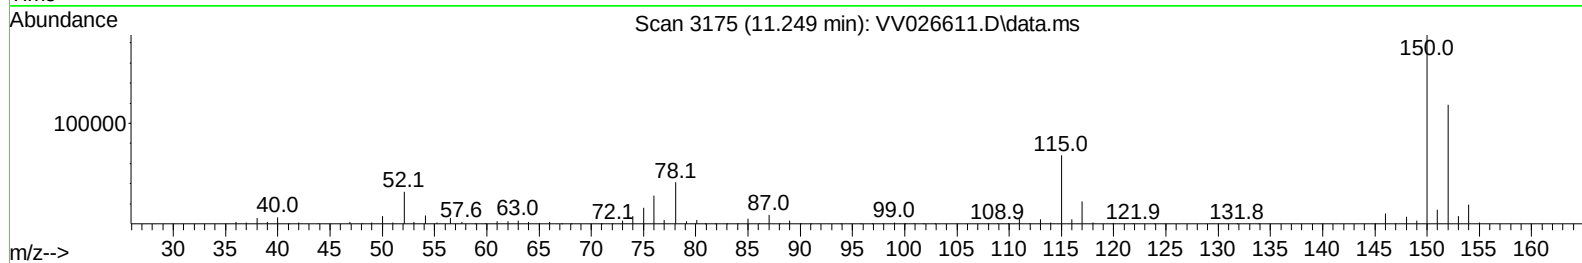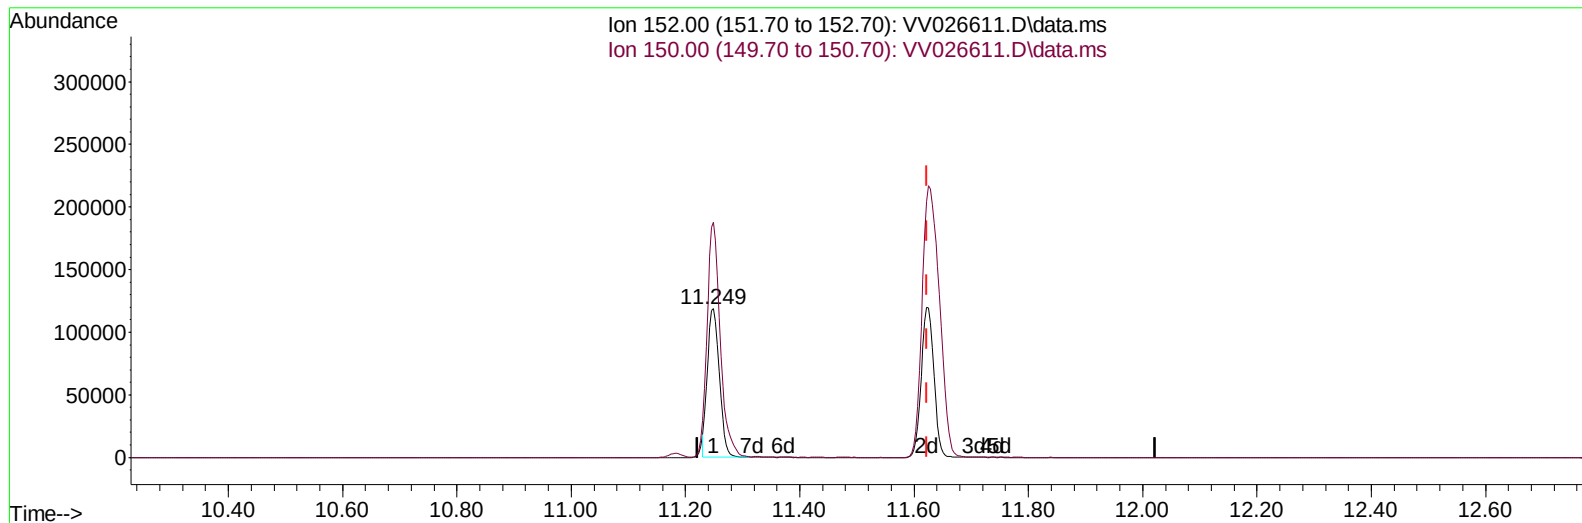

TIC: VV026611.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.249min (-0.373) 48.95 ug/L

response 172468

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	174.70	168.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026611.D
 Acq On : 30 Jun 2022 16:47
 Operator : SY/MD
 Sample : N3521-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JT3

Manual IntegrationsAPPROVED

Quant Time: Jul 01 00:23:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

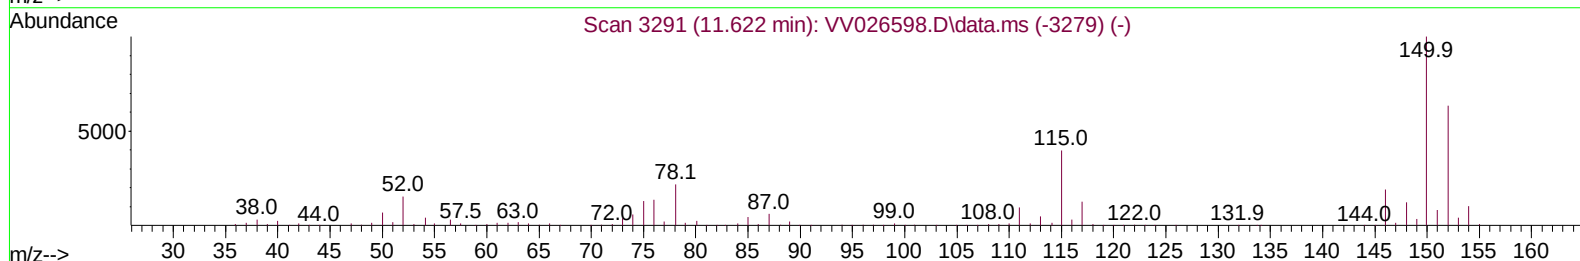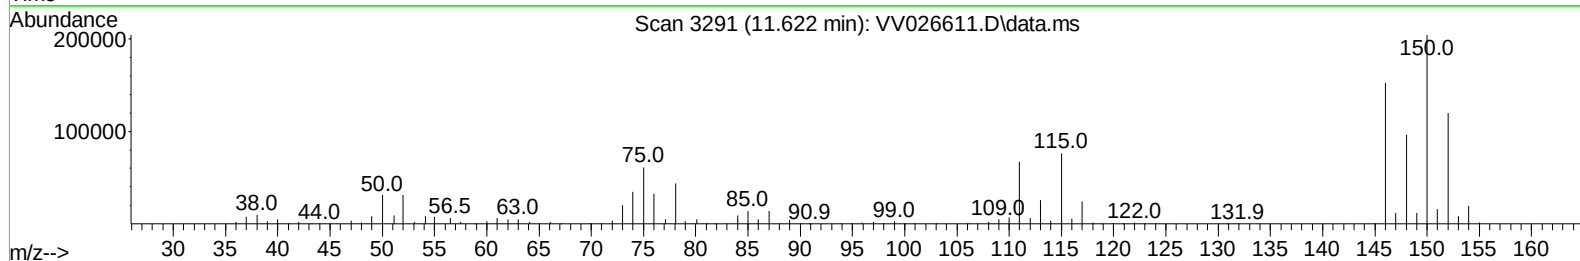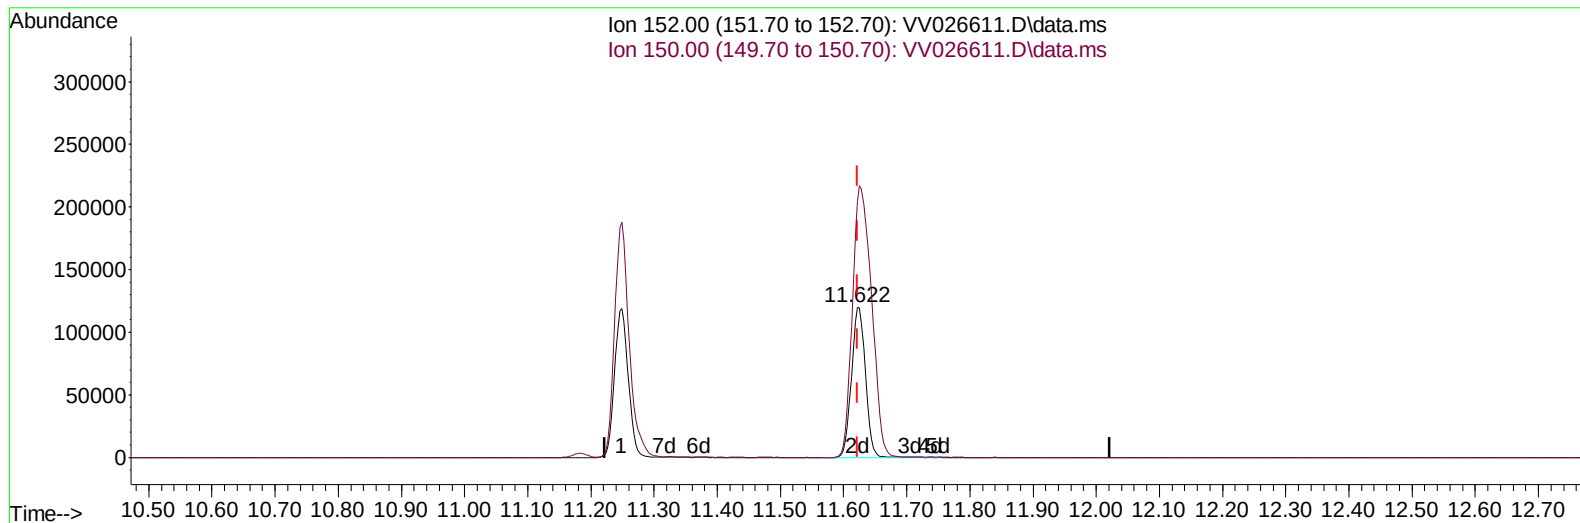

TIC: VV026611.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.622min (+ 0.000) 52.22 ug/L m

response 183994

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	174.70	158.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026611.D
 Acq On : 30 Jun 2022 16:47
 Operator : SY/MD
 Sample : N3521-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JT3

Manual IntegrationsAPPROVED

Quant Time: Jul 01 00:23:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	370168	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	368792	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	180040	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	119607	39.638	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	79.280%	
7) Chloroethane-d5	1.584	69	110702	42.777	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	85.560%	
11) 1,1-Dichloroethene-d2	2.121	63	178134	31.339	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	62.680%	
21) 2-Butanone-d5	3.915	46	154111	102.010	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	102.010%	
24) Chloroform-d	4.362	84	257944	44.271	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.540%	
26) 1,2-Dichloroethane-d4	5.040	65	153336	46.251	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.500%	
32) Benzene-d6	5.059	84	491284	43.809	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.620%	
36) 1,2-Dichloropropane-d6	6.076	67	161907	45.837	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	91.680%	
41) Toluene-d8	7.320	98	401094	40.720	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	81.440%	
43) trans-1,3-Dichloroprop...	7.625	79	56069	39.536	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.080%	
47) 2-Hexanone-d5	8.092	63	104025	85.152	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	85.150%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	235693	46.214	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	92.420%	
66) 1,2-Dichlorobenzene-d4	11.622	152	183994m	52.218	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	104.440%	
Target Compounds						
					Qvalue	
13) Acetone	2.208	43	11016	10.015	ug/L	97
33) Benzene	5.111	78	20407	1.707	ug/L	100
51) Chlorobenzene	8.882	112	374921	44.313	ug/L	99
64) 1,3-Dichlorobenzene	11.181	146	52732	9.496	ug/L	97
65) 1,4-Dichlorobenzene	11.271	146	210346	36.530	ug/L	99
67) 1,2-Dichlorobenzene	11.641	146	1647137	291.093	ug/L	100
70) 1,2,4-trichlorobenzene	13.259	180	296616	92.329	ug/L	99
72) 1,2,3-Trichlorobenzene	13.741	180	150117	46.028	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed