

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026600.D
 Acq On : 30 Jun 2022 12:18
 Operator : SY/MD
 Sample : N3534-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

Quant Time: Jul 01 00:20:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	421346	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	410997	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	212407	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	149594	43.554	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.100%		
7) Chloroethane-d5	1.580	69	128791	43.722	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.440%		
11) 1,1-Dichloroethene-d2	2.121	63	314331	48.583	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.160%		
21) 2-Butanone-d5	3.915	46	170025	98.874	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.870%		
24) Chloroform-d	4.355	84	310682m	46.846	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.700%		
26) 1,2-Dichloroethane-d4	5.037	65	173623	46.009	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.020%		
32) Benzene-d6	5.053	84	580594	46.457	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.920%		
36) 1,2-Dichloropropane-d6	6.072	67	189386	48.111	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.220%		
41) Toluene-d8	7.316	98	508838	46.354	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.700%		
43) trans-1,3-Dichloroprop...	7.622	79	75854	47.995	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.980%		
47) 2-Hexanone-d5	8.091	63	124645	91.553	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.550%		
56) 1,1,2,2-Tetrachloroeth...	10.213	84	259464	45.651	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.300%		
66) 1,2-Dichlorobenzene-d4	11.622	152	196214	47.201	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.400%		
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.146	85	111789	36.898	ug/L	100
3) Chloromethane	1.256	50	121955	32.465	ug/L	100
5) Vinyl chloride	1.326	62	239652	60.392	ug/L	100
6) Bromomethane	1.535	94	44833	17.947	ug/L	99
8) Chloroethane	1.600	64	77118	28.961	ug/L	99
9) Trichlorofluoromethane	1.764	101	290703	52.212	ug/L	99
10) 1,1,2-Trichloro-1,2,2-...	2.127	101	83325	25.493	ug/L	99
12) 1,1-Dichloroethene	2.127	96	185693	57.665	ug/L	95
16) Methylene chloride	2.519	84	169507	44.839	ug/L	99
17) trans-1,2-Dichloroethene	2.770	96	70405	21.192	ug/L	100
19) 1,1-Dichloroethane	3.201	63	416262	69.212	ug/L	100
20) cis-1,2-Dichloroethene	3.921	96	161651	45.541	ug/L	100
23) Bromochloromethane	4.259	128	83892	41.786	ug/L	98
25) Chloroform	4.381	83	388471	61.033	ug/L	100
27) 1,2-Dichloroethane	5.133	62	330453	76.821	ug/L	100
30) 1,1,1-Trichloroethane	4.616	97	120870	22.511	ug/L	99
31) Carbon tetrachloride	4.834	117	287358	63.738	ug/L	100
33) Benzene	5.104	78	672769	50.486	ug/L	100
34) Trichloroethene	5.915	95	299166	88.948	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026600.D
 Acq On : 30 Jun 2022 12:18
 Operator : SY/MD
 Sample : N3534-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

Quant Time: Jul 01 00:20:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

37) 1,2-Dichloropropane	6.175	63	144968	41.764	ug/L	99
38) Bromodichloromethane	6.513	83	91991	20.624	ug/L	99
39) cis-1,3-Dichloropropene	7.027	75	122447	26.197	ug/L	98
44) trans-1,3-Dichloropropene	7.651	75	197993	45.935	ug/L	99
45) 1,1,2-Trichloroethane	7.837	97	94583	26.845	ug/L	99
46) Tetrachloroethene	7.976	164	213010	78.367	ug/L	99
49) Dibromochloromethane	8.246	129	126077	37.175	ug/L	99
50) 1,2-Dibromoethane	8.352	107	111217	31.105	ug/L	96
57) 1,1,2,2-Tetrachloroethane	10.239	83	209054	38.124	ug/L	100
59) Bromoform	9.731	173	82348	44.044	ug/L	99
63) 1,2,4-Trimethylbenzene	10.914	105	522112	49.974	ug/L	100
68) 1,2-Dibromo-3-chloropr...	12.426	75	34201	40.261	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026600.D
 Acq On : 30 Jun 2022 12:18
 Operator : SY/MD
 Sample : N3534-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1


Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0

Manual Integrations APPROVED

Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

Quant Time: Jul 01 00:20:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

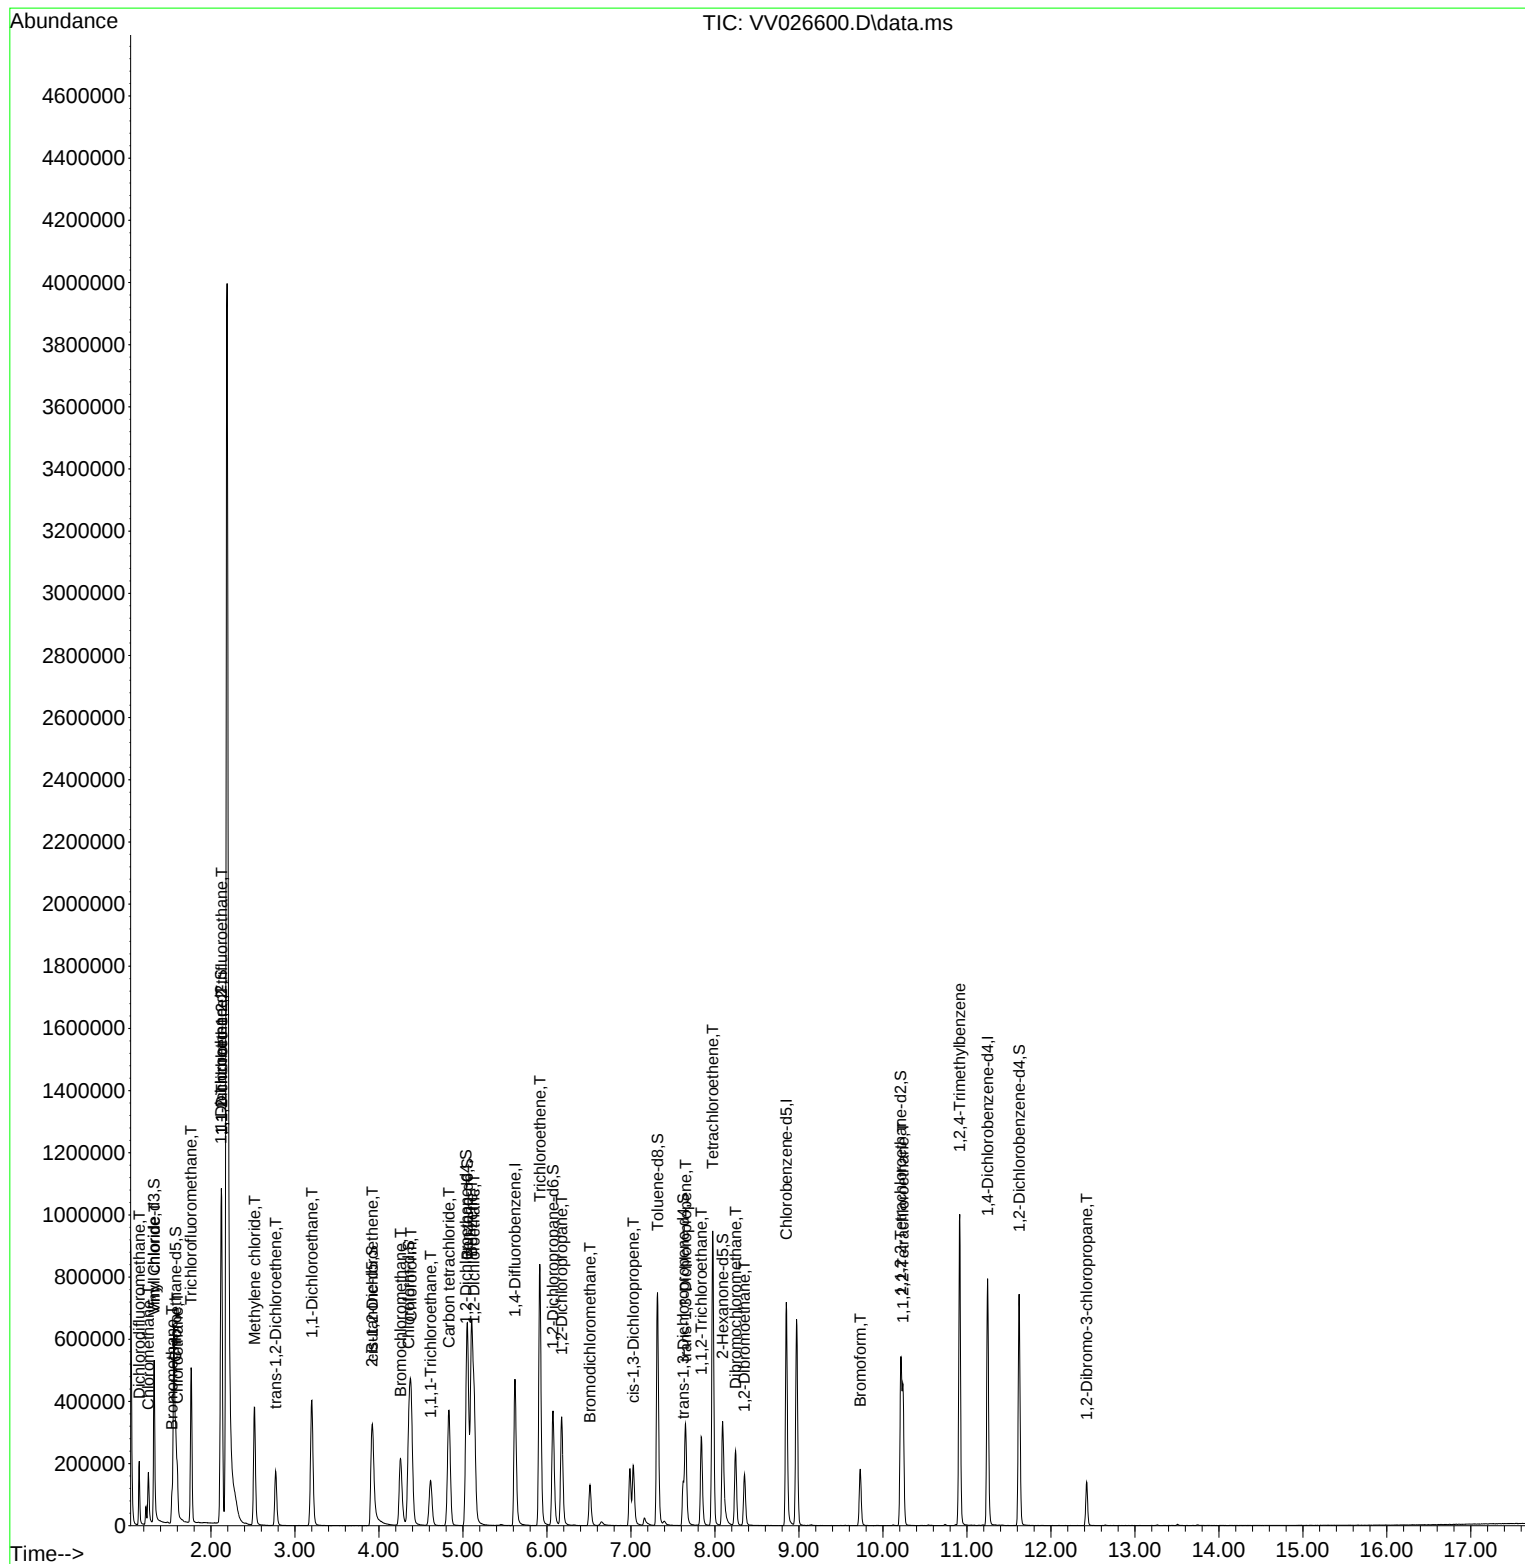

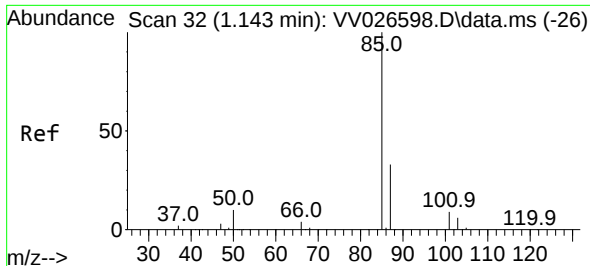





#2
 Dichlorodifluoromethane
 Concen: 36.898 ug/L
 RT: 1.146 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0

Tgt Ion: 85 Resp: 111789
 Ion Ratio Lower Upper
 85 100
 87 32.5 25.8 38.8




Manual Integrations
 APPROVED


Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

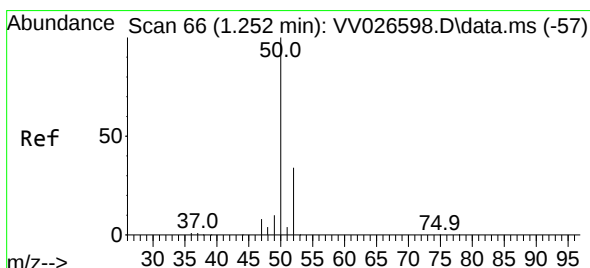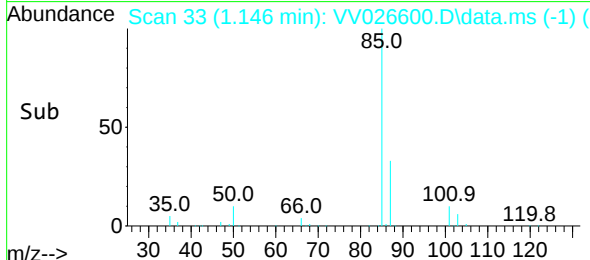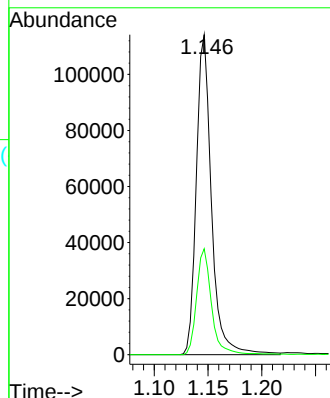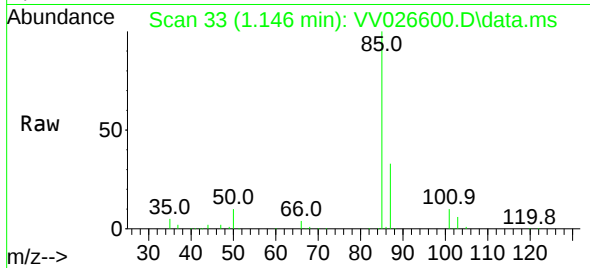

#3
 Chloromethane
 Concen: 32.465 ug/L
 RT: 1.256 min Scan# 67
 Delta R.T. 0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18


Tgt Ion: 50 Resp: 121955
 Ion Ratio Lower Upper
 50 100
 52 32.8 23.1 42.9

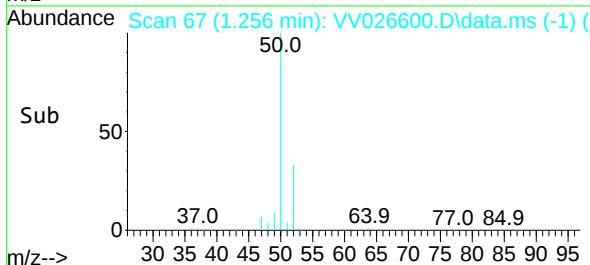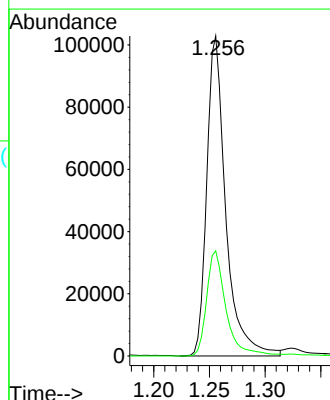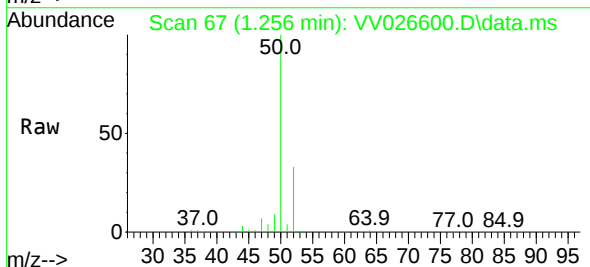

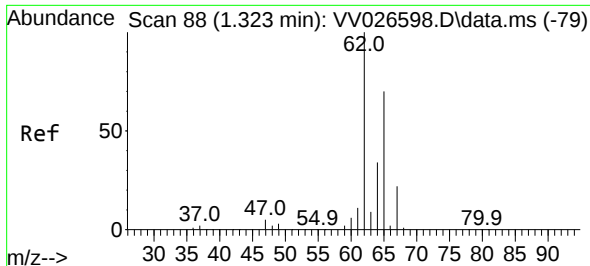

#5
 Vinyl chloride
 Concen: 60.392 ug/L
 RT: 1.326 min Scan# 89
 Delta R.T. 0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18




Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0

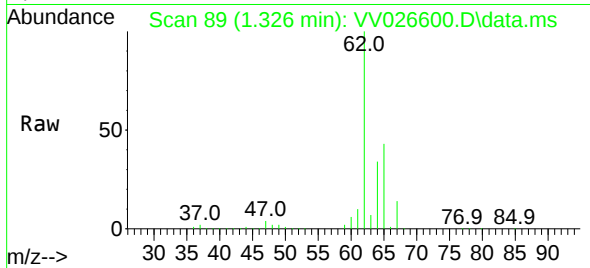

Tgt Ion: 62 Resp: 239652
 Ion Ratio Lower Upper
 62 100
 64 33.9 23.7 44.1




Manual Integrations
 APPROVED


Reviewed By :Krupa Patel 07/01/2022
 Supervised By :Mahesh Dadoda 07/01/2022

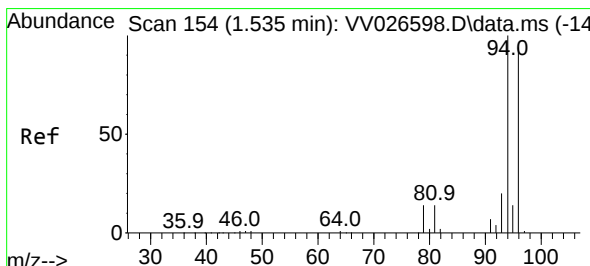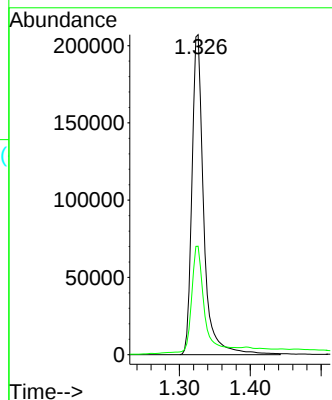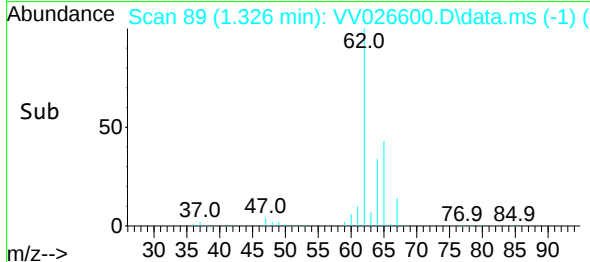

#6
 Bromomethane
 Concen: 17.947 ug/L
 RT: 1.535 min Scan# 154
 Delta R.T. -0.000 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18

Tgt Ion: 94 Resp: 44833
 Ion Ratio Lower Upper
 94 100
 96 94.2 65.6 121.8

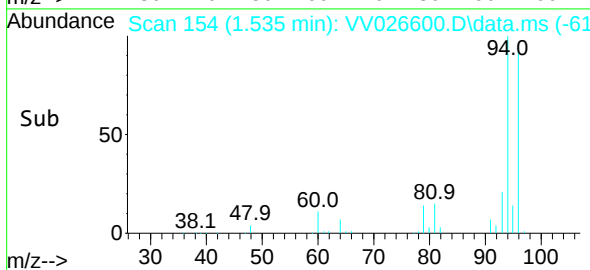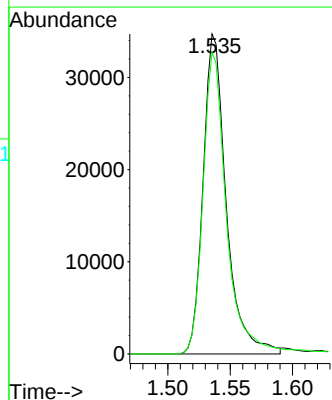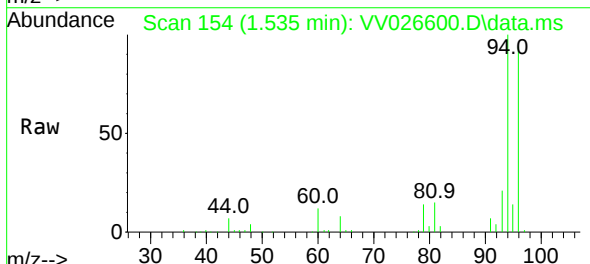

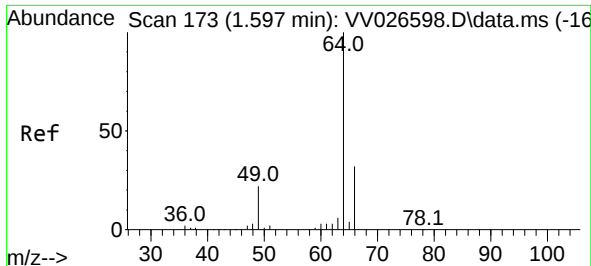





#8
Chloroethane
Concen: 28.961 ug/L
RT: 1.600 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
A0AH0

Tgt Ion: 64 Resp: 77118
Ion Ratio Lower Upper
64 100
66 31.4 21.6 40.0




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

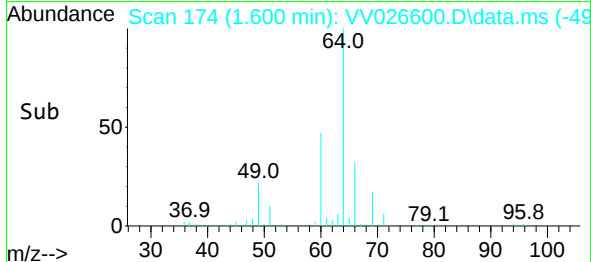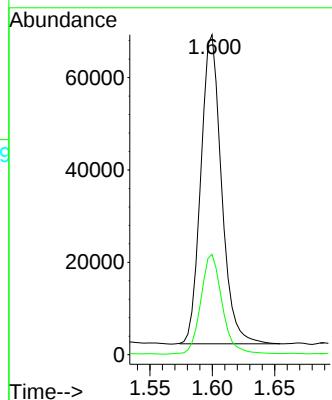

#9
Trichlorofluoromethane
Concen: 52.212 ug/L
RT: 1.764 min Scan# 225
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18


Tgt Ion:101 Resp: 290703
Ion Ratio Lower Upper
101 100
103 64.3 51.8 77.6

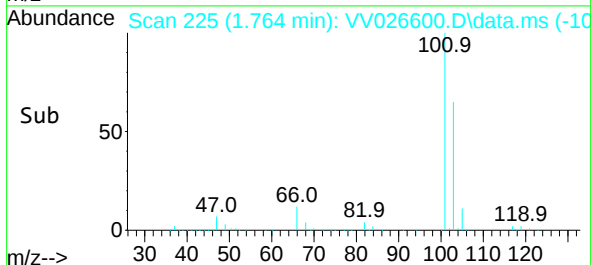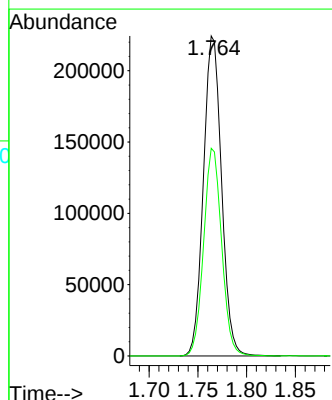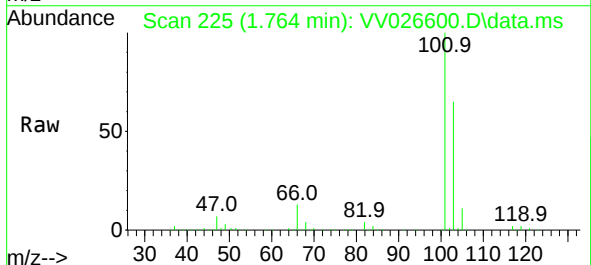

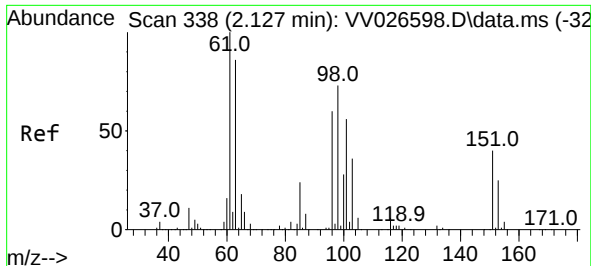

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 25.493 ug/L
RT: 2.127 min Scan# 338
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0




Tgt Ion:101 Resp: 8332
Ion Ratio Lower Upper
101 100
85 43.3 34.5 51.7
151 69.6 56.9 85.3

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

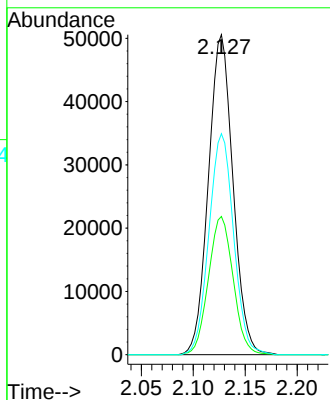


#12
1,1-Dichloroethene
Concen: 57.665 ug/L
RT: 2.127 min Scan# 338
Delta R.T. -0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Tgt Ion: 96 Resp: 185693
Ion Ratio Lower Upper
96 100
61 165.5 114.9 213.5
63 115.9 88.8 164.8

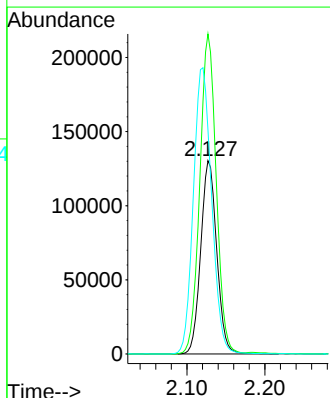



#16
Methylene chloride
Concen: 44.839 ug/L
RT: 2.519 min Scan# 460
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0




Tgt Ion: 84 Resp: 16950
Ion Ratio Lower Upper
84 100
86 64.5 45.4 84.2
49 107.9 76.5 142.1

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

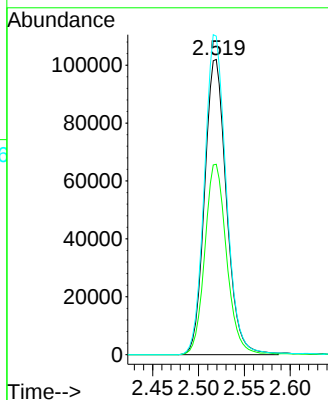


#17
trans-1,2-Dichloroethene
Concen: 21.192 ug/L
RT: 2.770 min Scan# 538
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18



Tgt Ion: 96 Resp: 70405
Ion Ratio Lower Upper
96 100
61 125.8 88.4 164.2
98 63.5 44.2 82.0

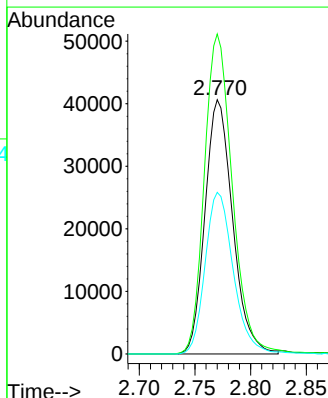



#19

1,1-Dichloroethane

Concen: 69.212 ug/L

RT: 3.201 min Scan# 61

Delta R.T. -0.000 min

Lab File: VV026600.D

Acq: 30 Jun 2022 12:18

Instrument :

MSVOA_V

ClientSampleId :

A0AH0

Tgt Ion: 63 Resp: 41626

Ion Ratio Lower Upper

63 100

65 31.7 22.2 41.2





83 13.4 9.5 17.7

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 07/01/2022

Supervised By :Mahesh Dadoda 07/01/2022

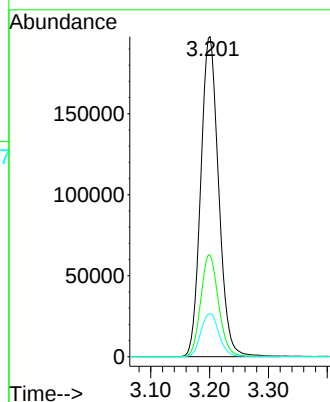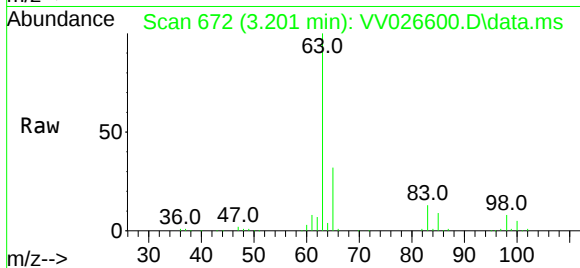

#20

cis-1,2-Dichloroethene

Concen: 45.541 ug/L

RT: 3.921 min Scan# 896

Delta R.T. -0.000 min

Lab File: VV026600.D

Acq: 30 Jun 2022 12:18




Tgt Ion: 96 Resp: 161651


Ion Ratio Lower Upper

96 100

61 117.5 82.6 153.4


68 0.0 0.0 0.0

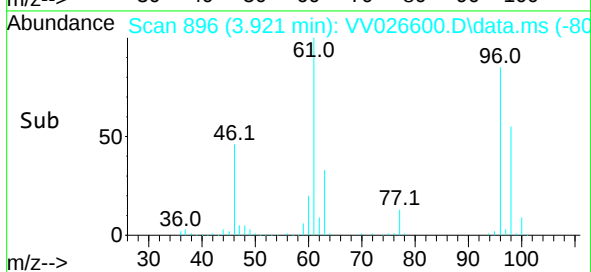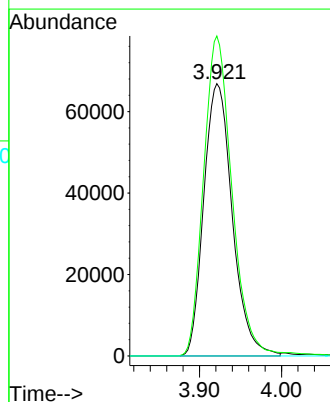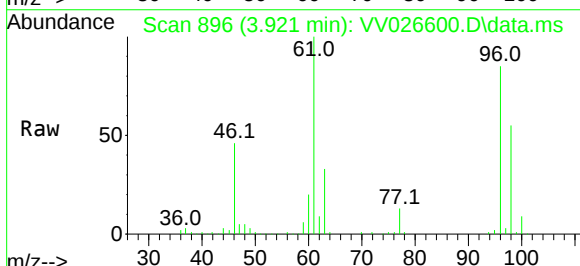



#23
Bromochloromethane
Concen: 41.786 ug/L
RT: 4.259 min Scan# 1000
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0

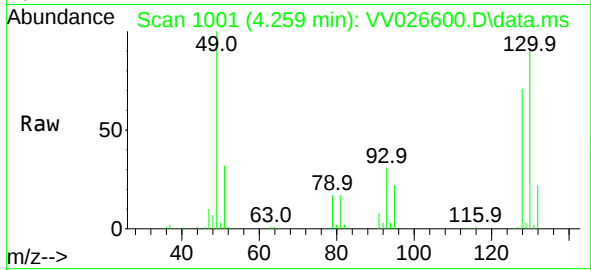


Tgt Ion:128 Resp: 83892
Ion Ratio Lower Upper
128 100
49 141.5 102.3 190.1
130 128.0 90.2 167.6
51 45.9 36.2 54.4

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

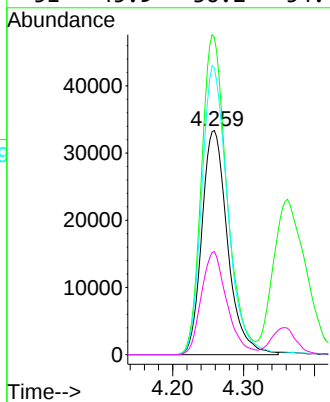


#25
Chloroform
Concen: 61.033 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. -0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

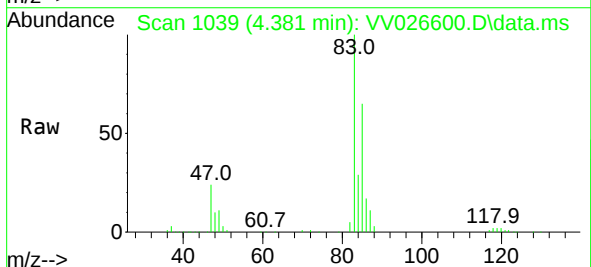

Tgt Ion: 83 Resp: 388471
Ion Ratio Lower Upper
83 100
85 65.1 45.4 84.4

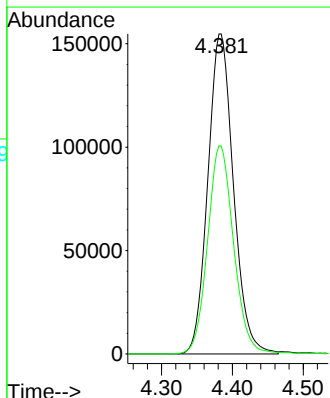







#27
1,2-Dichloroethane
Concen: 76.821 ug/L
RT: 5.133 min Scan# 11273
Delta R.T. -0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
A0AH0

Tgt Ion: 62 Resp: 33045
Ion Ratio Lower Upper
62 100
98 10.9 8.8 13.2




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

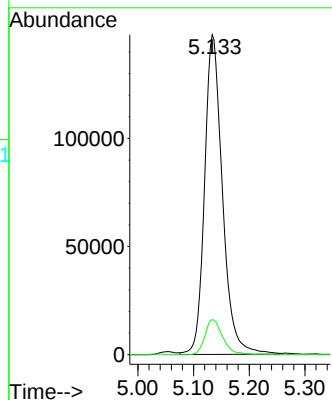

#30
1,1,1-Trichloroethane
Concen: 22.511 ug/L
RT: 4.616 min Scan# 1112
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18


Tgt Ion: 97 Resp: 120870
Ion Ratio Lower Upper
97 100
99 63.9 52.1 78.1
61 40.1 31.8 47.6

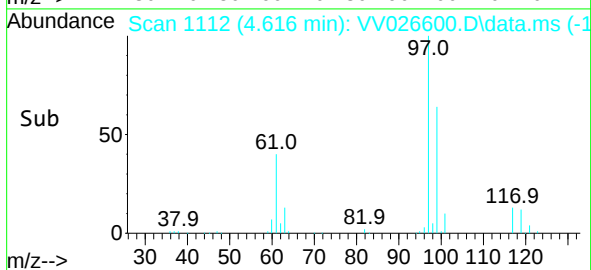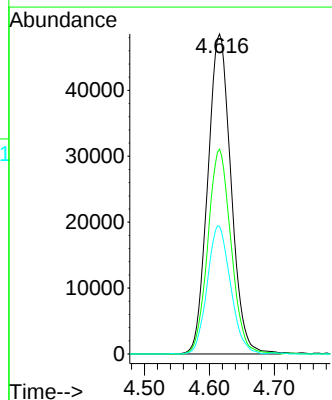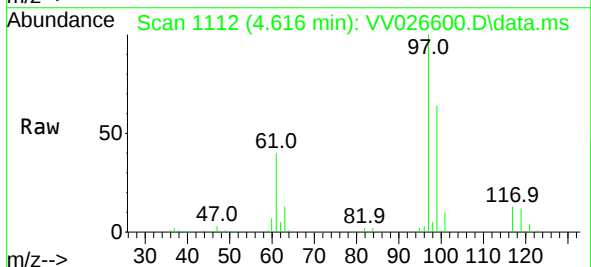



#31
Carbon tetrachloride
Concen: 63.738 ug/L
RT: 4.834 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0

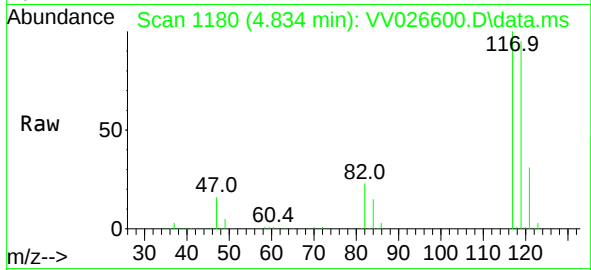

Tgt Ion:117 Resp: 287358
Ion Ratio Lower Upper
117 100
119 95.9 77.0 115.4




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

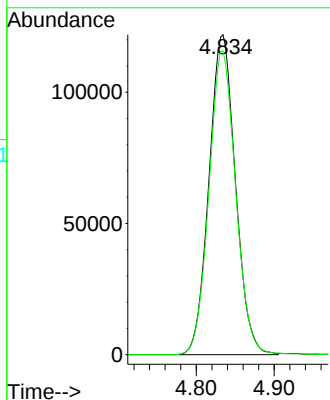

#33
Benzene
Concen: 50.486 ug/L
RT: 5.104 min Scan# 1264
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18


Tgt Ion: 78 Resp: 672769

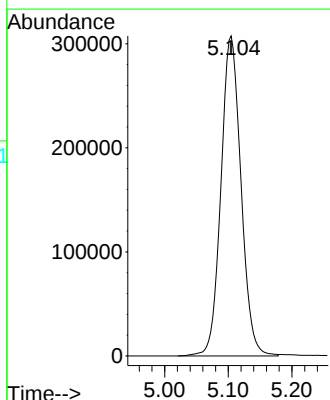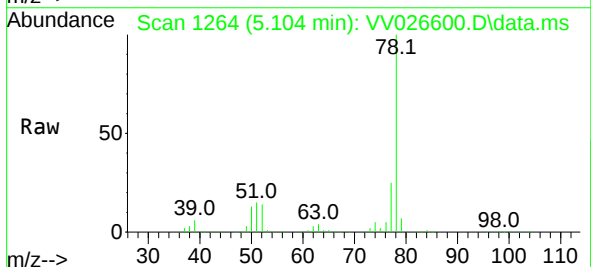



#34
Trichloroethene
Concen: 88.948 ug/L
RT: 5.915 min Scan# 1516
Delta R.T. -0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0




Tgt Ion: 95 Resp: 299160
Ion Ratio Lower Upper
95 100
97 63.7 45.0 83.6
132 99.5 69.0 128.2
130 105.0 73.1 135.8

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

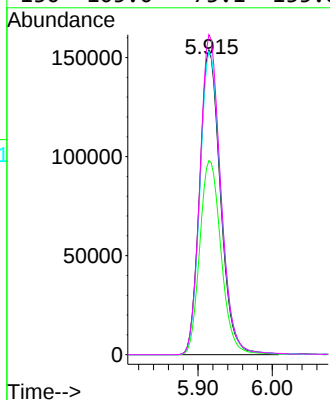


#37
1,2-Dichloropropane
Concen: 41.764 ug/L
RT: 6.175 min Scan# 1597
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

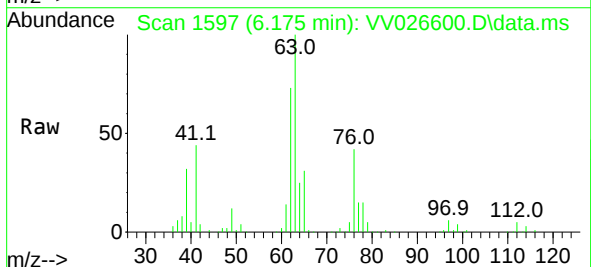

Tgt Ion: 63 Resp: 144968
Ion Ratio Lower Upper
63 100
112 4.9 4.2 6.2

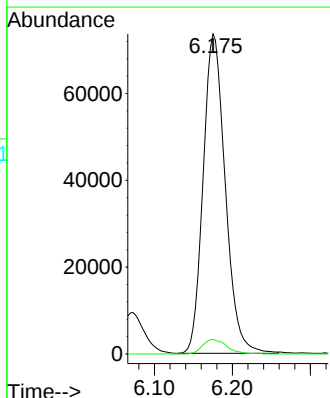







#38
Bromodichloromethane
Concen: 20.624 ug/L
RT: 6.513 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
A0AH0

Tgt Ion: 83 Resp: 9199
Ion Ratio Lower Upper
83 100
85 64.2 44.6 82.8
127 8.3 7.3 10.9




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

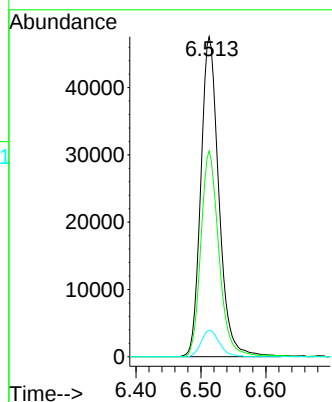

#39
cis-1,3-Dichloropropene
Concen: 26.197 ug/L
RT: 7.027 min Scan# 1862
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18


Tgt Ion: 75 Resp: 122447
Ion Ratio Lower Upper
75 100
77 30.7 22.4 41.6

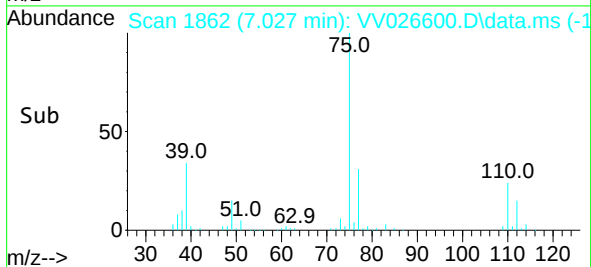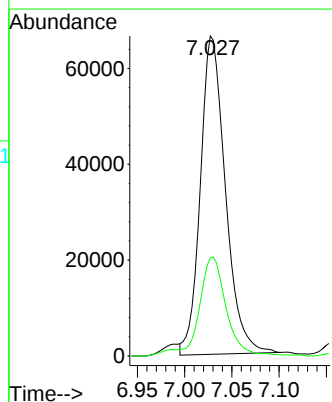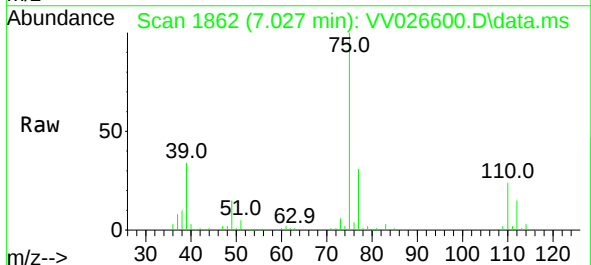



#44
trans-1,3-Dichloropropene
Concen: 45.935 ug/L
RT: 7.651 min Scan# 2056
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0



Tgt Ion: 75 Resp: 197993
Ion Ratio Lower Upper
75 100
77 31.7 22.6 42.0




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

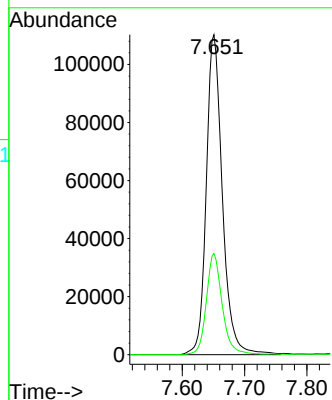

#45
1,1,2-Trichloroethane
Concen: 26.845 ug/L
RT: 7.837 min Scan# 2114
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18


Tgt Ion: 97 Resp: 94583
Ion Ratio Lower Upper
97 100
99 63.2 42.8 79.6
83 84.1 59.1 109.7
85 54.5 37.7 70.1

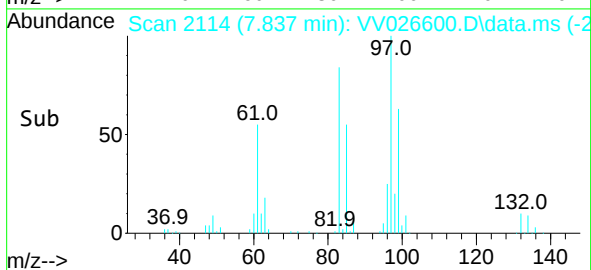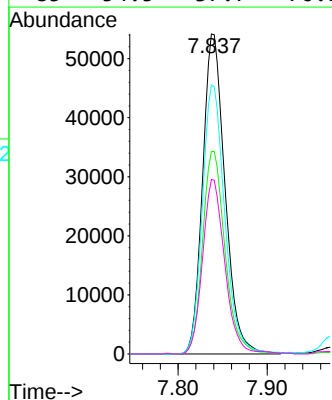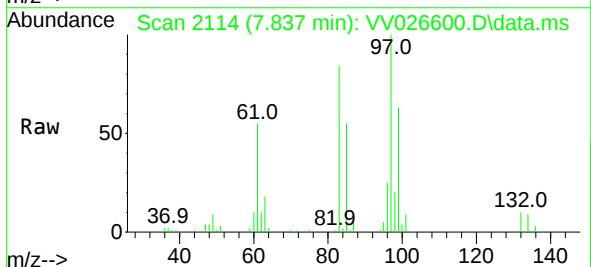



#46
Tetrachloroethene
Concen: 78.367 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0




Tgt Ion:164 Resp: 213010
Ion Ratio Lower Upper
164 100
129 95.9 66.1 122.8
131 91.9 64.2 119.2
166 126.9 88.1 163.7

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

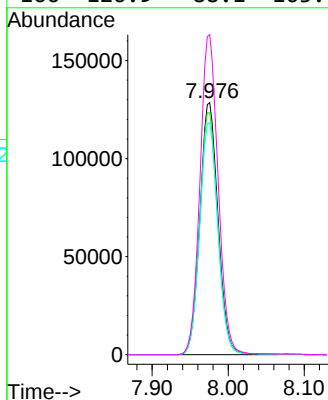


#49
Dibromochloromethane
Concen: 37.175 ug/L
RT: 8.246 min Scan# 2241
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

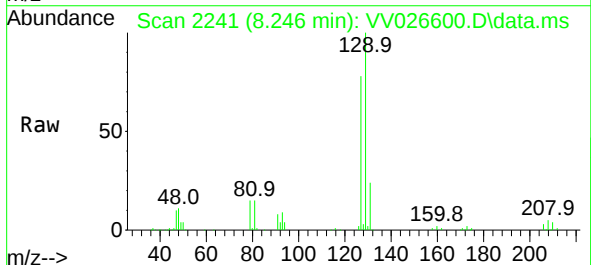


Tgt Ion:129 Resp: 126077
Ion Ratio Lower Upper
129 100
127 77.9 54.1 100.5

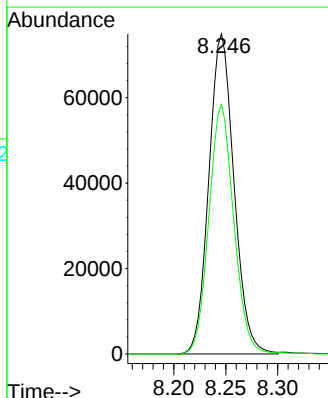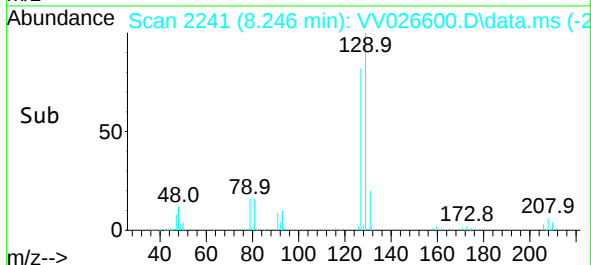



#50
1,2-Dibromoethane
Concen: 31.105 ug/L
RT: 8.352 min Scan# 211
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0




Tgt Ion:107 Resp: 11121
Ion Ratio Lower Upper
107 100
109 92.0 67.3 125.1
188 3.4 2.7 4.1

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

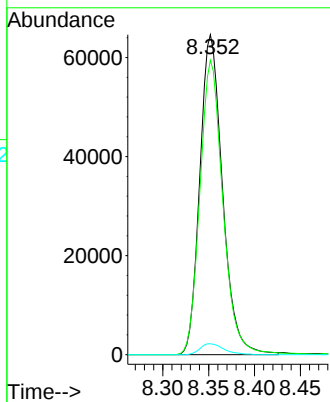


#57
1,1,2,2-Tetrachloroethane
Concen: 38.124 ug/L
RT: 10.239 min Scan# 2861
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

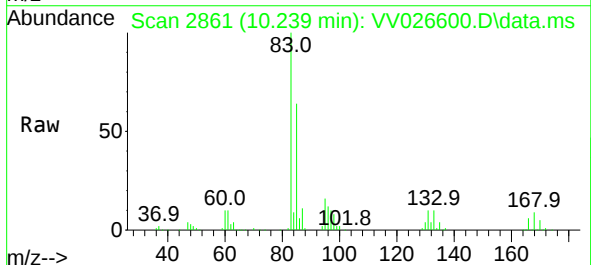


Tgt Ion: 83 Resp: 209054
Ion Ratio Lower Upper
83 100
85 63.9 44.6 82.8
131 9.9 7.6 11.4

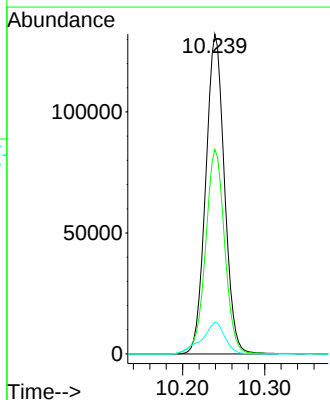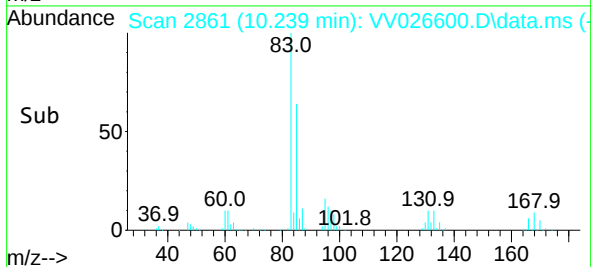



#59
Bromoform
Concen: 44.044 ug/L
RT: 9.731 min Scan# 2702
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0




Tgt Ion:173 Resp: 82348
Ion Ratio Lower Upper
173 100
175 49.5 39.1 58.7
254 8.8 7.1 10.7

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

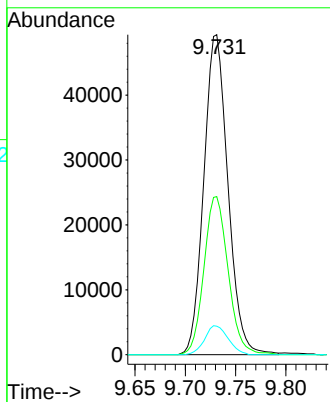


#63
1,2,4-Trimethylbenzene
Concen: 49.974 ug/L
RT: 10.914 min Scan# 3071
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

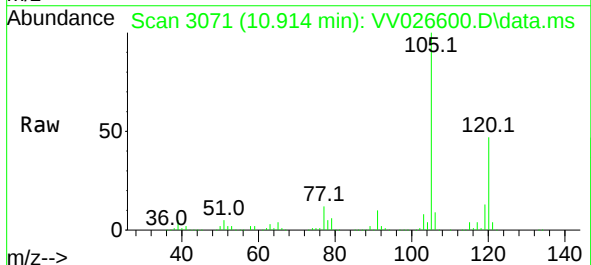


Tgt Ion:105 Resp: 522112
Ion Ratio Lower Upper
105 100
120 47.1 37.5 56.3

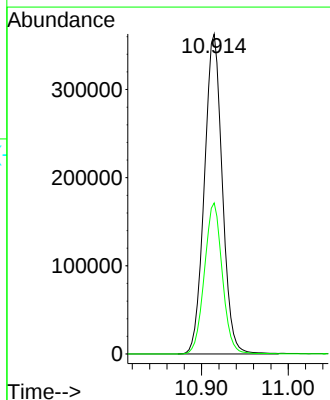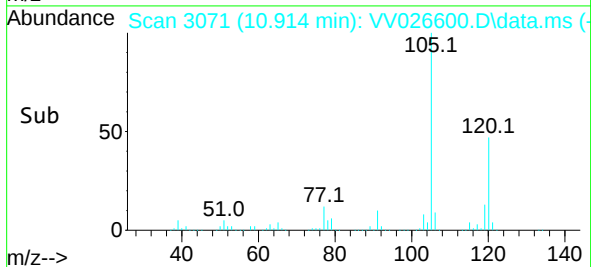



#68
1,2-Dibromo-3-chloropropane
Concen: 40.261 ug/L
RT: 12.426 min Scan# 3541
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
A0AH0



Tgt Ion: 75 Resp: 3420
Ion Ratio Lower Upper
75 100
155 92.8 71.0 106.4
157 119.8 91.3 136.9

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 07/01/2022
Supervised By :Mahesh Dadoda 07/01/2022

