

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026599.D
 Acq On : 30 Jun 2022 11:47
 Operator : SY/MD
 Sample : VV0630WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	104	rBV	212835	230350	15.12%	2.053%
2	1.581	161	168	181	rVB	191797	215090	14.12%	1.917%
3	2.118	325	335	365	rVB	402226	583659	38.31%	5.202%
4	2.391	418	420	424	rVB2	495	327	0.02%	0.003%
5	2.436	431	434	436	rBV2	479	404	0.03%	0.004%
6	2.474	443	446	447	rBV	386	219	0.01%	0.002%
7	2.520	454	460	468	rBV4	2088	3114	0.20%	0.028%
8	2.606	484	487	489	rBV2	379	251	0.02%	0.002%
9	2.661	501	504	510	rVB3	347	341	0.02%	0.003%
10	2.693	510	514	516	rBV2	333	251	0.02%	0.002%
11	2.764	530	536	538	rBV5	738	633	0.04%	0.006%
12	2.838	557	559	564	rVB5	334	222	0.01%	0.002%
13	2.905	573	580	586	rVB3	351	474	0.03%	0.004%
14	2.979	601	603	609	rVB2	375	306	0.02%	0.003%
15	3.069	625	631	634	rBV2	384	357	0.02%	0.003%
16	3.118	640	646	649	rBV2	411	392	0.03%	0.003%
17	3.458	749	752	757	rBV2	253	263	0.02%	0.002%
18	3.709	827	830	833	rBV3	322	206	0.01%	0.002%
19	3.915	884	894	936	rBV2	58647	264006	17.33%	2.353%
20	4.355	1014	1031	1054	rBV	258444	634656	41.65%	5.656%
21	4.790	1163	1166	1168	rBV2	353	251	0.02%	0.002%
22	5.050	1230	1247	1277	rBV2	598607	1523693	100.00%	13.579%
23	5.243	1304	1307	1311	rVB3	538	457	0.03%	0.004%
24	5.355	1339	1342	1344	rBV	275	208	0.01%	0.002%
25	5.426	1362	1364	1370	rVB3	283	246	0.02%	0.002%
26	5.462	1373	1375	1379	rBV2	331	212	0.01%	0.002%
27	5.548	1398	1402	1405	rBV	409	311	0.02%	0.003%
28	5.619	1412	1424	1454	rBV	429401	865419	56.80%	7.713%
29	5.915	1506	1516	1526	rBV4	5097	9712	0.64%	0.087%
30	5.970	1530	1533	1535	rBV3	394	250	0.02%	0.002%
31	6.072	1550	1565	1594	rBV	339736	700639	45.98%	6.244%
32	6.275	1624	1628	1631	rVB3	543	360	0.02%	0.003%
33	6.391	1655	1664	1666	rBV4	306	324	0.02%	0.003%
34	6.552	1710	1714	1716	rBV2	559	316	0.02%	0.003%
35	6.654	1738	1746	1753	rBV5	1210	1805	0.12%	0.016%
36	6.799	1786	1791	1794	rVB2	253	235	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026599.D
 Acq On : 30 Jun 2022 11:47
 Operator : SY/MD
 Sample : VV0630WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	6.886	1816	1818	1824	rVB2	281	215	0.01%	0.002%
38	6.944	1829	1836	1838	rVB2	295	216	0.01%	0.002%
39	6.986	1838	1849	1878	rBV	147480	280506	18.41%	2.500%
40	7.182	1907	1910	1911	rBV	396	245	0.02%	0.002%
41	7.317	1940	1952	1970	rBV	667591	1151666	75.58%	10.264%
42	7.542	2017	2022	2024	rBV3	364	315	0.02%	0.003%
43	7.622	2037	2047	2072	rBV	101209	182712	11.99%	1.628%
44	7.822	2106	2109	2111	rVV	567	349	0.02%	0.003%
45	7.976	2154	2157	2158	rBV	476	254	0.02%	0.002%
46	7.986	2158	2160	2165	rVB2	658	402	0.03%	0.004%
47	8.011	2165	2168	2171	rVB	376	224	0.01%	0.002%
48	8.034	2172	2175	2178	rVB2	298	214	0.01%	0.002%
49	8.092	2182	2193	2228	rBV2	294878	621150	40.77%	5.536%
50	8.362	2275	2277	2281	rVB2	683	357	0.02%	0.003%
51	8.500	2316	2320	2325	rBV4	742	681	0.04%	0.006%
52	8.603	2348	2352	2357	rBV3	352	340	0.02%	0.003%
53	8.754	2393	2399	2404	rBV2	260	229	0.02%	0.002%
54	8.850	2417	2429	2459	rBV	667511	1081262	70.96%	9.636%
55	8.992	2470	2473	2475	rVB2	486	239	0.02%	0.002%
56	9.066	2494	2496	2504	rVB4	497	550	0.04%	0.005%
57	9.156	2517	2524	2529	rVV3	1189	1530	0.10%	0.014%
58	9.285	2561	2564	2568	rVB	350	229	0.02%	0.002%
59	9.551	2639	2647	2652	rBV3	1049	1304	0.09%	0.012%
60	9.616	2665	2667	2673	rVB2	274	234	0.02%	0.002%
61	9.931	2760	2765	2774	rVV3	1170	1642	0.11%	0.015%
62	10.124	2817	2825	2832	rBV3	1790	2787	0.18%	0.025%
63	10.214	2838	2853	2869	rBV	494748	762472	50.04%	6.795%
64	10.465	2928	2931	2936	rVB2	348	318	0.02%	0.003%
65	10.548	2949	2957	2962	rBV3	1275	1524	0.10%	0.014%
66	10.577	2962	2966	2968	rBV	584	402	0.03%	0.004%
67	10.667	2990	2994	2998	rVB2	293	234	0.02%	0.002%
68	10.915	3061	3071	3082	rBV8	2390	4389	0.29%	0.039%
69	10.960	3082	3085	3089	rVB3	441	316	0.02%	0.003%
70	11.037	3106	3109	3112	rBV	306	232	0.02%	0.002%
71	11.143	3136	3142	3148	rVB4	812	1035	0.07%	0.009%
72	11.188	3148	3156	3163	rBV5	3866	6049	0.40%	0.054%
73	11.246	3163	3174	3196	rBV	635433	984174	64.59%	8.771%
74	11.622	3279	3291	3319	rBV	676516	1041594	68.36%	9.283%
75	11.783	3339	3341	3347	rVB4	606	589	0.04%	0.005%
76	11.815	3348	3351	3353	rBV	336	249	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026599.D
 Acq On : 30 Jun 2022 11:47
 Operator : SY/MD
 Sample : VV0630WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	12.027	3413	3417	3419	rBV	319	273	0.02%	0.002%
78	12.063	3423	3428	3431	rBV2	305	291	0.02%	0.003%
79	12.104	3438	3441	3445	rBV2	440	345	0.02%	0.003%
80	12.130	3446	3449	3452	rBV2	248	204	0.01%	0.002%
81	12.448	3541	3548	3552	rBV3	528	676	0.04%	0.006%
82	12.503	3559	3565	3571	rVB3	381	562	0.04%	0.005%
83	12.564	3579	3584	3587	rVB2	243	219	0.01%	0.002%
84	12.596	3590	3594	3598	rVB4	368	327	0.02%	0.003%
85	12.648	3603	3610	3621	rVB3	4279	6189	0.41%	0.055%
86	12.825	3660	3665	3667	rBV2	381	327	0.02%	0.003%
87	13.046	3730	3734	3737	rBV	301	227	0.01%	0.002%
88	13.069	3738	3741	3744	rVB	376	245	0.02%	0.002%
89	13.262	3793	3801	3802	rBV3	5184	4759	0.31%	0.042%
90	13.345	3825	3827	3831	rBV2	359	268	0.02%	0.002%
91	13.365	3831	3833	3838	rVB2	409	294	0.02%	0.003%
92	13.426	3846	3852	3853	rBV2	316	307	0.02%	0.003%
93	13.503	3868	3876	3892	rBV2	12671	19740	1.30%	0.176%
94	13.747	3944	3952	3963	rVB4	5694	9025	0.59%	0.080%
95	14.043	4042	4044	4050	rVB2	466	434	0.03%	0.004%
96	14.075	4051	4054	4061	rVB3	491	556	0.04%	0.005%
97	14.368	4142	4145	4147	rBV2	380	259	0.02%	0.002%
98	14.464	4170	4175	4178	rBV3	469	461	0.03%	0.004%
99	14.628	4224	4226	4233	rVB4	487	573	0.04%	0.005%
100	15.728	4565	4568	4571	rBV2	923	720	0.05%	0.006%




Sum of corrected areas: 11220669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026599.D
Acq On : 30 Jun 2022 11:47
Operator : SY/MD
Sample : VV0630WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

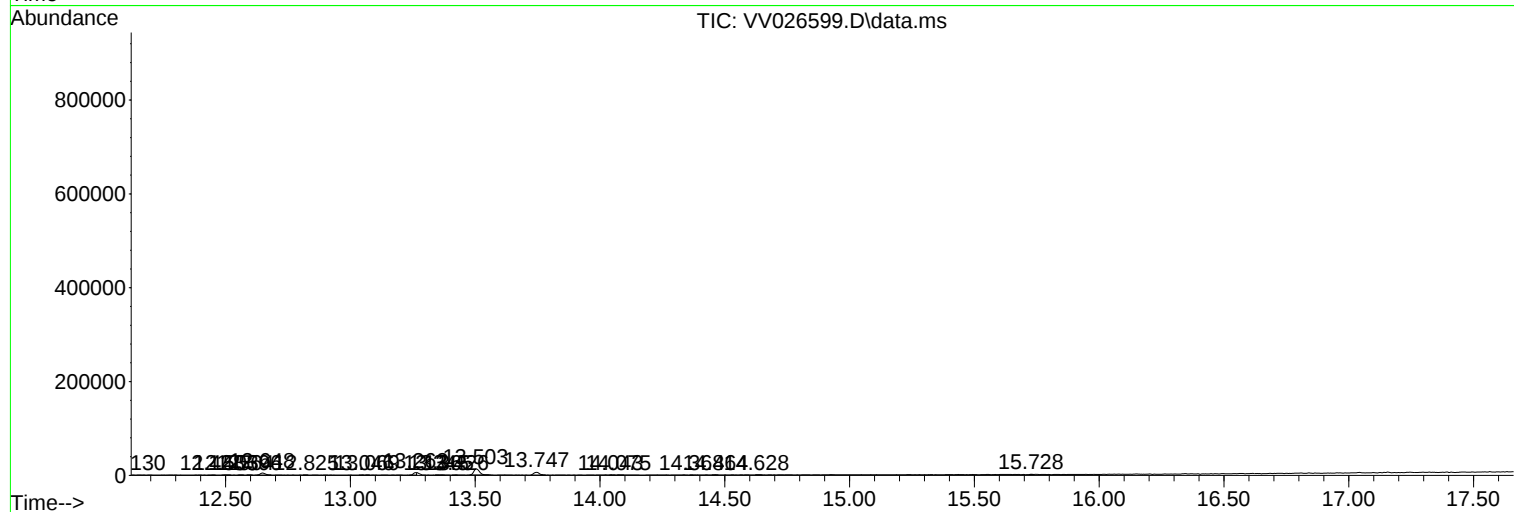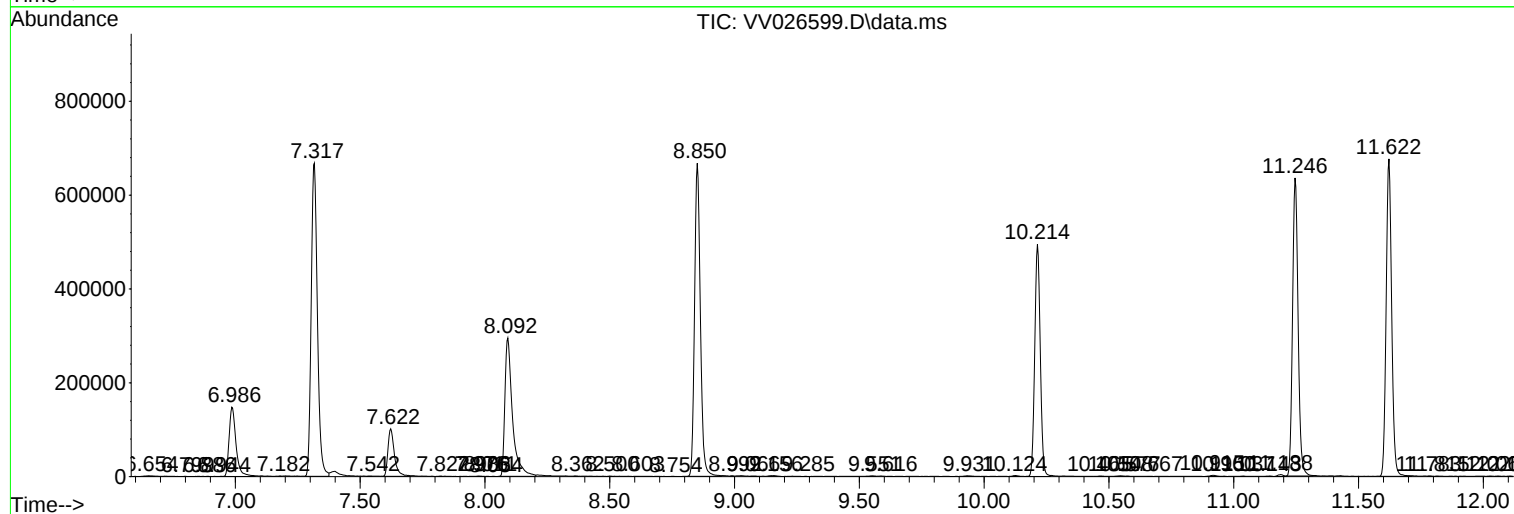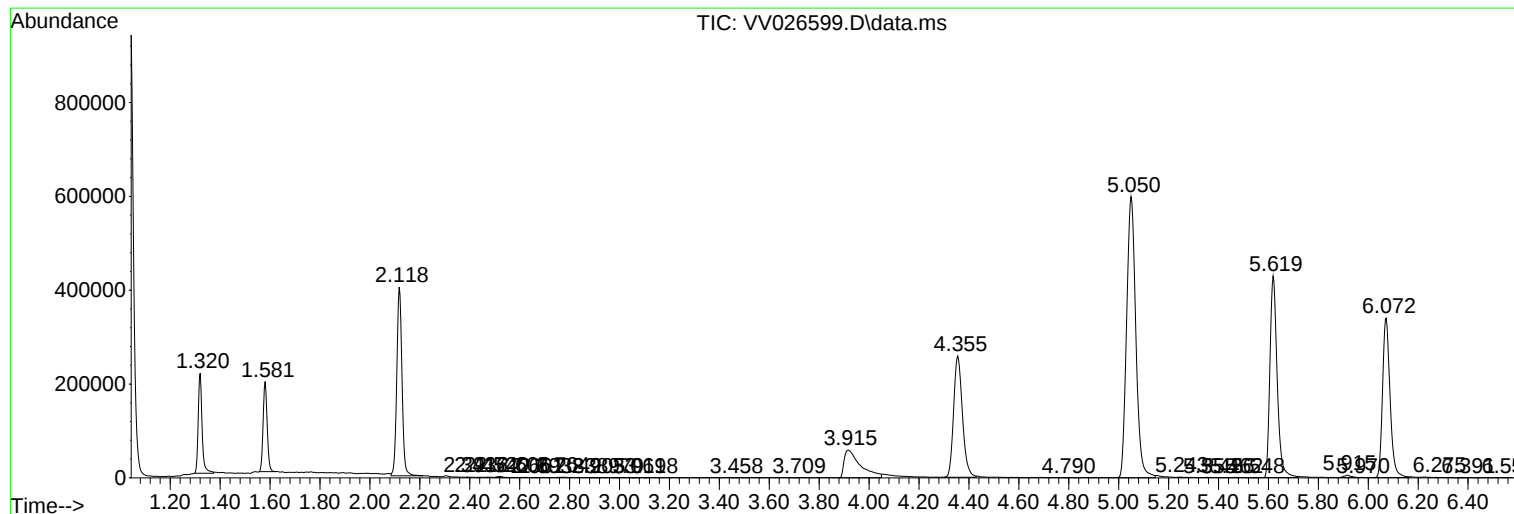

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026599.D
Acq On : 30 Jun 2022 11:47
Operator : SY/MD
Sample : VV0630WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026599.D
Acq On : 30 Jun 2022 11:47
Operator : SY/MD
Sample : VV0630WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc