

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026601.D
 Acq On : 30 Jun 2022 12:44
 Operator : SY/MD
 Sample : N3521-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	109	rVB	201897	215157	14.14%	1.941%
2	1.580	162	168	183	rVB	186774	213832	14.06%	1.929%
3	2.121	327	336	354	rVB	386983	551887	36.28%	4.979%
4	2.767	532	537	538	rBV4	463	382	0.03%	0.003%
5	2.889	572	575	576	rBV	290	170	0.01%	0.002%
6	3.105	640	642	643	rBV	198	95	0.01%	0.001%
7	3.156	654	658	660	rBV	387	310	0.02%	0.003%
8	3.262	688	691	696	rVB2	362	228	0.01%	0.002%
9	3.285	696	698	702	rBV3	359	271	0.02%	0.002%
10	3.355	717	720	725	rBV2	245	195	0.01%	0.002%
11	3.381	725	728	730	rBV	204	168	0.01%	0.002%
12	3.426	739	742	744	rBV	158	99	0.01%	0.001%
13	3.452	746	750	754	rVV3	229	197	0.01%	0.002%
14	3.555	779	782	785	rBV	322	213	0.01%	0.002%
15	3.641	807	809	812	rVB2	205	116	0.01%	0.001%
16	3.693	822	825	828	rVB	170	85	0.01%	0.001%
17	3.744	837	841	844	rBV2	258	195	0.01%	0.002%
18	3.783	850	853	855	rBV	233	116	0.01%	0.001%
19	3.838	866	870	875	rVB3	300	279	0.02%	0.003%
20	3.870	875	880	882	rBV2	237	196	0.01%	0.002%
21	3.915	885	894	940	rBV2	54472	252701	16.61%	2.280%
22	4.358	1016	1032	1068	rBV	256176	629643	41.39%	5.681%
23	4.616	1110	1112	1114	rBV	334	213	0.01%	0.002%
24	4.651	1122	1123	1126	rVB2	393	182	0.01%	0.002%
25	4.670	1126	1129	1131	rBV	272	182	0.01%	0.002%
26	4.709	1139	1141	1143	rVB2	448	183	0.01%	0.002%
27	4.728	1144	1147	1149	rVV	244	154	0.01%	0.001%
28	4.760	1154	1157	1160	rVB	343	234	0.02%	0.002%
29	4.773	1160	1161	1164	rBV2	191	91	0.01%	0.001%
30	4.802	1169	1170	1172	rBV2	201	91	0.01%	0.001%
31	4.838	1178	1181	1185	rVB3	251	197	0.01%	0.002%
32	4.860	1185	1188	1190	rVB	300	189	0.01%	0.002%
33	4.876	1190	1193	1195	rBV	197	114	0.01%	0.001%
34	4.892	1195	1198	1200	rBV	249	153	0.01%	0.001%
35	4.928	1208	1209	1213	rVB	443	190	0.01%	0.002%
36	4.950	1213	1216	1219	rVB	198	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026601.D
 Acq On : 30 Jun 2022 12:44
 Operator : SY/MD
 Sample : N3521-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	4.973	1221	1223	1226	rVB2	310	131	0.01%	0.001%
38	4.989	1226	1228	1231	rBV2	128	87	0.01%	0.001%
39	5.053	1231	1248	1289	rBV2	593643	1521380	100.00%	13.727%
40	5.394	1352	1354	1357	rBV3	271	147	0.01%	0.001%
41	5.503	1384	1388	1389	rBV	330	206	0.01%	0.002%
42	5.567	1407	1408	1410	rBV	319	150	0.01%	0.001%
43	5.622	1413	1425	1451	rBV	431615	868269	57.07%	7.834%
44	5.918	1509	1517	1533	rVV7	4446	10218	0.67%	0.092%
45	5.992	1537	1540	1542	rBV	375	276	0.02%	0.002%
46	6.075	1552	1566	1595	rBV	338373	692688	45.53%	6.250%
47	6.291	1631	1633	1635	rVB	404	184	0.01%	0.002%
48	6.317	1638	1641	1642	rBV	212	143	0.01%	0.001%
49	6.352	1649	1652	1655	rBV3	371	294	0.02%	0.003%
50	6.381	1659	1661	1665	rVB2	330	156	0.01%	0.001%
51	6.410	1665	1670	1674	rBV3	288	240	0.02%	0.002%
52	6.471	1686	1689	1693	rVB3	316	220	0.01%	0.002%
53	6.538	1703	1710	1712	rBV4	343	333	0.02%	0.003%
54	6.590	1723	1726	1731	rBV4	358	371	0.02%	0.003%
55	6.635	1737	1740	1742	rBV2	732	563	0.04%	0.005%
56	6.757	1775	1778	1782	rBV3	276	257	0.02%	0.002%
57	6.812	1790	1795	1796	rBV2	318	221	0.01%	0.002%
58	6.911	1823	1826	1828	rBV2	145	83	0.01%	0.001%
59	6.989	1838	1850	1882	rBV	147061	278095	18.28%	2.509%
60	7.275	1936	1939	1940	rBV	559	239	0.02%	0.002%
61	7.317	1940	1952	1972	rBV	667494	1139534	74.90%	10.281%
62	7.622	2038	2047	2078	rBV	98825	181238	11.91%	1.635%
63	7.860	2118	2121	2122	rBV2	260	142	0.01%	0.001%
64	7.979	2154	2158	2159	rBV3	1138	846	0.06%	0.008%
65	8.037	2172	2176	2180	rBV3	317	338	0.02%	0.003%
66	8.091	2183	2193	2229	rBV2	280508	604858	39.76%	5.457%
67	8.590	2345	2348	2354	rVB4	323	280	0.02%	0.003%
68	8.664	2370	2371	2373	rBV2	357	145	0.01%	0.001%
69	8.712	2383	2386	2388	rBV	275	195	0.01%	0.002%
70	8.783	2402	2408	2411	rBV3	339	343	0.02%	0.003%
71	8.850	2418	2429	2464	rBV	668822	1093675	71.89%	9.868%
72	9.243	2549	2551	2553	rBV	229	126	0.01%	0.001%
73	9.268	2558	2559	2561	rBV	165	73	0.00%	0.001%
74	9.339	2578	2581	2582	rBV	297	147	0.01%	0.001%
75	9.403	2598	2601	2604	rVB	331	220	0.01%	0.002%
76	9.419	2604	2606	2607	rBV	187	84	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026601.D
 Acq On : 30 Jun 2022 12:44
 Operator : SY/MD
 Sample : N3521-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	9.474	2620	2623	2625	rBV2	190	133	0.01%	0.001%
78	9.551	2639	2647	2650	rBV3	659	683	0.04%	0.006%
79	9.583	2655	2657	2664	rBV2	245	239	0.02%	0.002%
80	9.612	2664	2666	2667	rBV2	220	91	0.01%	0.001%
81	9.850	2737	2740	2742	rBV2	153	130	0.01%	0.001%
82	9.937	2762	2767	2769	rBV2	464	429	0.03%	0.004%
83	9.963	2773	2775	2778	rVB2	180	85	0.01%	0.001%
84	10.214	2841	2853	2871	rBV	485008	754407	49.59%	6.807%
85	10.384	2898	2906	2913	rBV3	1549	2347	0.15%	0.021%
86	10.538	2949	2954	2955	rBV2	649	424	0.03%	0.004%
87	10.660	2990	2992	2993	rBV	365	131	0.01%	0.001%
88	10.828	3040	3044	3049	rBV2	311	336	0.02%	0.003%
89	10.918	3065	3072	3081	rBV4	5606	7499	0.49%	0.068%
90	11.143	3137	3142	3144	rBV3	614	532	0.03%	0.005%
91	11.191	3151	3157	3159	rBV3	1019	882	0.06%	0.008%
92	11.246	3163	3174	3197	rBV	636361	997512	65.57%	9.000%
93	11.535	3255	3264	3278	rBV4	7015	13683	0.90%	0.123%
94	11.622	3280	3291	3315	rVV	669400	1030553	67.74%	9.298%
95	11.921	3380	3384	3387	rBV2	361	367	0.02%	0.003%
96	12.049	3422	3424	3426	rVB	610	231	0.02%	0.002%
97	12.349	3511	3517	3523	rBV7	2227	2648	0.17%	0.024%
98	13.268	3797	3803	3809	rVB2	1341	1615	0.11%	0.015%
99	13.747	3944	3952	3961	rBV5	1159	2122	0.14%	0.019%
100	13.902	3998	4000	4004	rBV	435	339	0.02%	0.003%




Sum of corrected areas: 11083431

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026601.D
Acq On : 30 Jun 2022 12:44
Operator : SY/MD
Sample : N3521-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

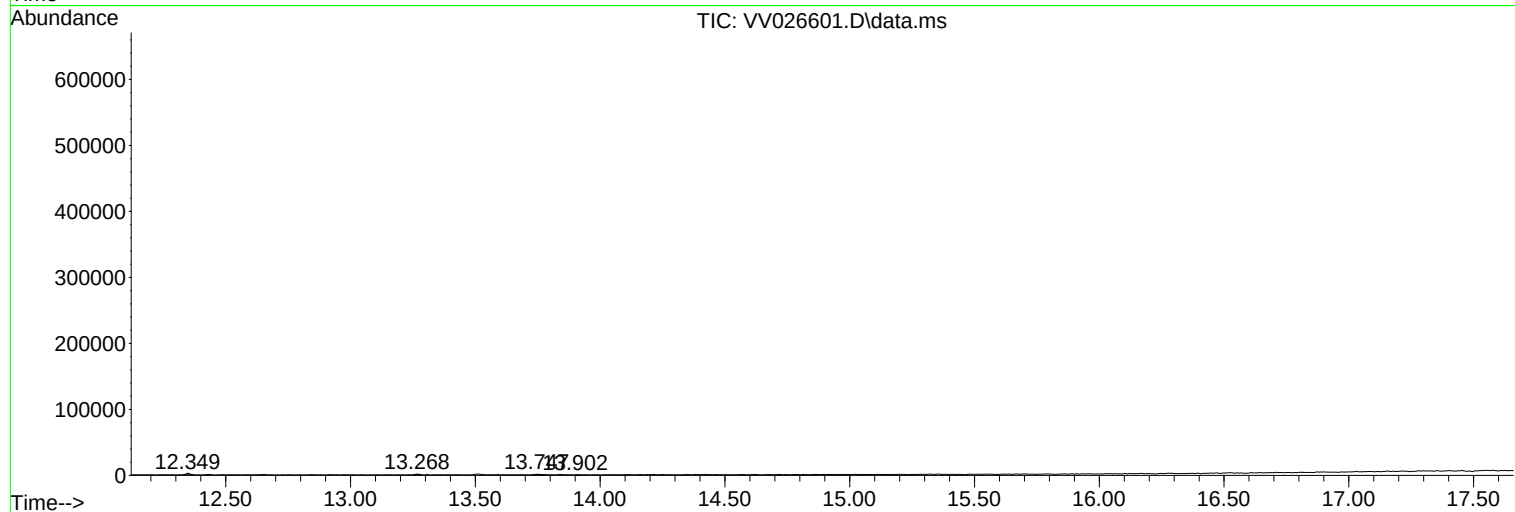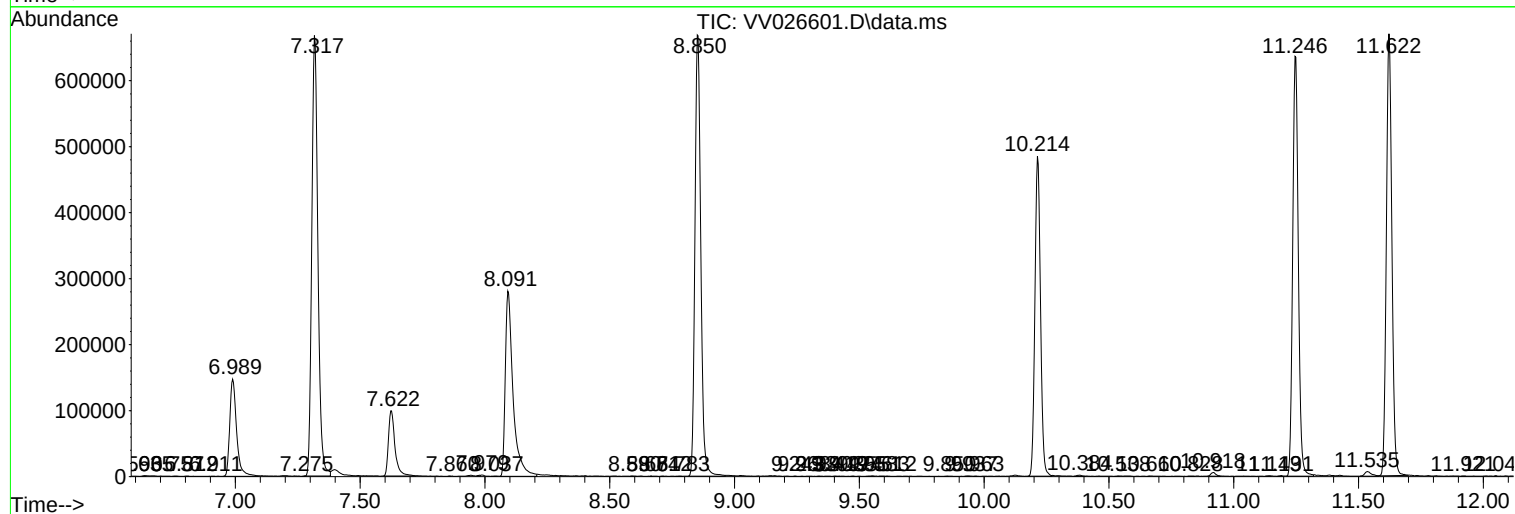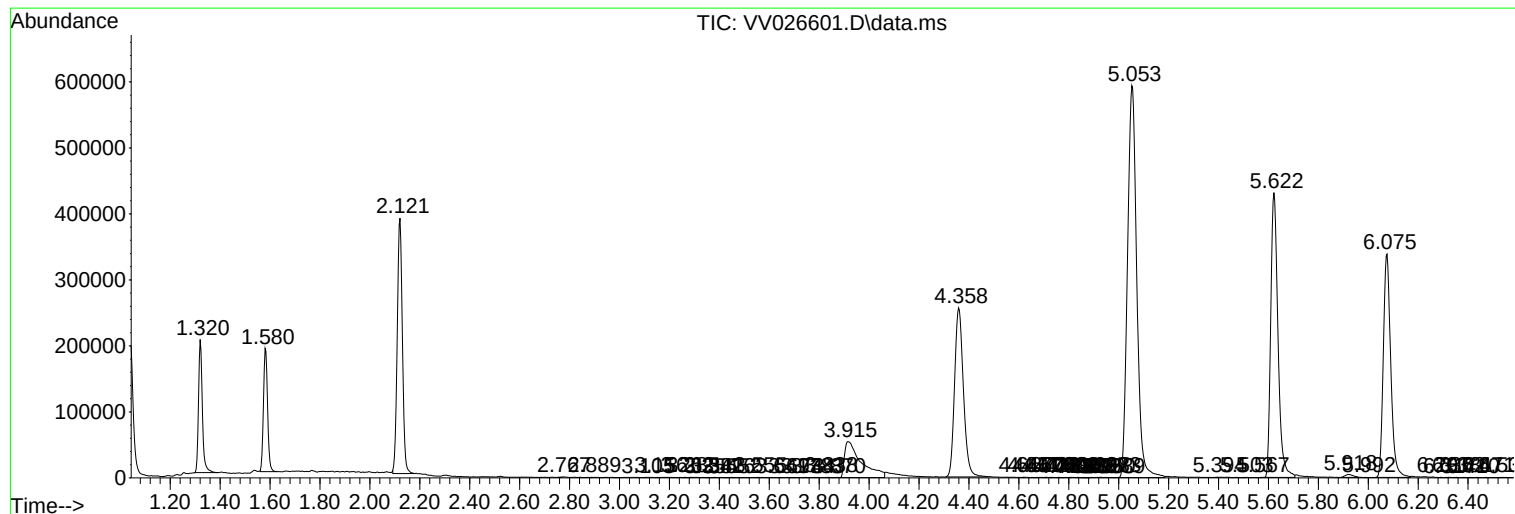

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026601.D
Acq On : 30 Jun 2022 12:44
Operator : SY/MD
Sample : N3521-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026601.D
Acq On : 30 Jun 2022 12:44
Operator : SY/MD
Sample : N3521-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------