

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026602.D
 Acq On : 30 Jun 2022 13:08
 Operator : SY/MD
 Sample : N3521-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M

Title : VOC Analysis

Signal : TIC: VV026602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	100	rBV	197798	205460	13.91%	1.884%
2	1.580	162	168	186	rVB	184856	210470	14.25%	1.930%
3	2.117	327	335	358	rVB	372859	543359	36.78%	4.983%
4	2.558	469	472	476	rBV3	434	308	0.02%	0.003%
5	2.635	485	496	509	rBV	5165	11007	0.75%	0.101%
6	2.719	520	522	524	rBV2	302	100	0.01%	0.001%
7	2.870	566	569	571	rVB2	316	181	0.01%	0.002%
8	2.889	571	575	578	rBV2	436	377	0.03%	0.003%
9	3.076	630	633	634	rBV	153	77	0.01%	0.001%
10	3.085	634	636	638	rBV2	259	135	0.01%	0.001%
11	3.178	662	665	667	rBV3	266	200	0.01%	0.002%
12	3.243	680	685	687	rBV2	229	210	0.01%	0.002%
13	3.304	702	704	707	rBV	179	120	0.01%	0.001%
14	3.420	737	740	742	rBV	271	166	0.01%	0.002%
15	3.506	765	767	771	rBV2	200	129	0.01%	0.001%
16	3.706	827	829	832	rVB2	232	103	0.01%	0.001%
17	3.921	884	896	942	rBV2	70588	347118	23.50%	3.183%
18	4.358	1018	1032	1061	rBV	248520	618419	41.86%	5.671%
19	4.632	1115	1117	1123	rBV2	404	330	0.02%	0.003%
20	4.693	1133	1136	1138	rBV2	274	213	0.01%	0.002%
21	4.764	1153	1158	1159	rBV2	350	300	0.02%	0.003%
22	4.793	1165	1167	1170	rBV2	418	291	0.02%	0.003%
23	4.844	1181	1183	1184	rBV	193	53	0.00%	0.000%
24	4.860	1184	1188	1191	rVB2	264	197	0.01%	0.002%
25	4.924	1205	1208	1210	rBV2	299	169	0.01%	0.002%
26	4.937	1210	1212	1213	rVB	201	55	0.00%	0.001%
27	4.953	1215	1217	1220	rBV3	200	124	0.01%	0.001%
28	4.973	1220	1223	1227	rVB2	330	183	0.01%	0.002%
29	5.053	1231	1248	1288	rBV2	576360	1477186	100.00%	13.547%
30	5.317	1328	1330	1338	rVB2	509	470	0.03%	0.004%
31	5.487	1381	1383	1385	rBV2	311	191	0.01%	0.002%
32	5.538	1393	1399	1405	rBV3	547	598	0.04%	0.005%
33	5.577	1406	1411	1413	rBV2	440	363	0.02%	0.003%
34	5.622	1413	1425	1457	rBV	424250	863146	58.43%	7.916%
35	5.918	1509	1517	1530	rVB6	3780	7304	0.49%	0.067%
36	6.075	1553	1566	1602	rBV	331418	681584	46.14%	6.251%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026602.D
 Acq On : 30 Jun 2022 13:08
 Operator : SY/MD
 Sample : N3521-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	6.288	1631	1632	1635	rBV	311	157	0.01%	0.001%
38	6.365	1651	1656	1659	rBV2	519	430	0.03%	0.004%
39	6.426	1670	1675	1676	rBV2	190	146	0.01%	0.001%
40	6.490	1692	1695	1699	rBV	338	273	0.02%	0.003%
41	6.538	1706	1710	1716	rBV3	349	357	0.02%	0.003%
42	6.606	1729	1731	1736	rVB2	205	144	0.01%	0.001%
43	6.648	1736	1744	1747	rBV3	1061	1450	0.10%	0.013%
44	6.744	1772	1774	1777	rBV2	354	205	0.01%	0.002%
45	6.780	1781	1785	1788	rVB2	309	257	0.02%	0.002%
46	6.799	1788	1791	1795	rVB2	152	103	0.01%	0.001%
47	6.831	1795	1801	1803	rBV2	203	168	0.01%	0.002%
48	6.847	1803	1806	1809	rBV2	166	116	0.01%	0.001%
49	6.895	1818	1821	1822	rBV2	126	71	0.00%	0.001%
50	6.924	1828	1830	1835	rBV	138	122	0.01%	0.001%
51	6.989	1839	1850	1872	rBV	143462	265090	17.95%	2.431%
52	7.185	1908	1911	1912	rBV2	728	430	0.03%	0.004%
53	7.255	1932	1933	1937	rBV	341	202	0.01%	0.002%
54	7.320	1941	1953	1972	rBV	635431	1104738	74.79%	10.131%
55	7.625	2038	2048	2073	rBV	94278	174265	11.80%	1.598%
56	7.850	2116	2118	2123	rVB2	501	384	0.03%	0.004%
57	7.886	2123	2129	2132	rBV3	270	318	0.02%	0.003%
58	7.979	2155	2158	2163	rBV3	826	650	0.04%	0.006%
59	7.998	2163	2164	2172	rVB	487	349	0.02%	0.003%
60	8.030	2172	2174	2177	rBV2	199	89	0.01%	0.001%
61	8.091	2181	2193	2236	rBV2	278889	605435	40.99%	5.552%
62	8.487	2313	2316	2318	rBV2	219	148	0.01%	0.001%
63	8.677	2373	2375	2378	rVB2	363	143	0.01%	0.001%
64	8.699	2380	2382	2385	rVV2	188	97	0.01%	0.001%
65	8.757	2398	2400	2401	rBV	216	78	0.01%	0.001%
66	8.805	2409	2415	2418	rBV2	333	375	0.03%	0.003%
67	8.853	2418	2430	2459	rBV	660136	1078633	73.02%	9.892%
68	9.194	2533	2536	2543	rVB2	394	335	0.02%	0.003%
69	9.320	2571	2575	2579	rBV	219	207	0.01%	0.002%
70	9.355	2583	2586	2588	rBV2	186	125	0.01%	0.001%
71	9.390	2596	2597	2600	rVB	136	54	0.00%	0.000%
72	9.432	2607	2610	2613	rBV2	234	174	0.01%	0.002%
73	9.538	2638	2643	2644	rBV3	245	226	0.02%	0.002%
74	9.879	2747	2749	2752	rVB	262	92	0.01%	0.001%
75	9.895	2752	2754	2759	rBV	323	279	0.02%	0.003%
76	9.992	2780	2784	2788	rBV2	396	423	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026602.D
 Acq On : 30 Jun 2022 13:08
 Operator : SY/MD
 Sample : N3521-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	10.127	2820	2826	2834	rVB5	1573	2120	0.14%	0.019%
78	10.217	2841	2854	2877	rBV	475529	744238	50.38%	6.825%
79	10.355	2894	2897	2900	rBV3	435	281	0.02%	0.003%
80	10.378	2900	2904	2906	rBV3	956	752	0.05%	0.007%
81	10.451	2924	2927	2934	rVB3	361	253	0.02%	0.002%
82	10.670	2994	2995	2996	rBV	359	89	0.01%	0.001%
83	10.705	3004	3006	3008	rBV	189	58	0.00%	0.001%
84	10.728	3008	3013	3016	rBV2	347	253	0.02%	0.002%
85	10.786	3028	3031	3034	rBV	325	207	0.01%	0.002%
86	10.853	3049	3052	3055	rBV2	534	313	0.02%	0.003%
87	10.918	3065	3072	3079	rBV5	1766	2489	0.17%	0.023%
88	11.030	3105	3107	3108	rVB5	258	94	0.01%	0.001%
89	11.043	3108	3111	3114	rBV2	282	203	0.01%	0.002%
90	11.088	3121	3125	3127	rBV2	318	234	0.02%	0.002%
91	11.123	3133	3136	3139	rBV	246	169	0.01%	0.002%
92	11.143	3139	3142	3143	rBV	503	284	0.02%	0.003%
93	11.249	3163	3175	3196	rBV	609480	944971	63.97%	8.666%
94	11.419	3226	3228	3233	rVB3	914	616	0.04%	0.006%
95	11.535	3257	3264	3279	rBV4	4428	8575	0.58%	0.079%
96	11.622	3280	3291	3312	rBV	638253	987152	66.83%	9.053%
97	11.953	3387	3394	3396	rBV3	552	612	0.04%	0.006%
98	12.654	3606	3612	3616	rBV3	801	904	0.06%	0.008%
99	13.390	3837	3841	3846	rBV3	359	462	0.03%	0.004%
100	13.583	3895	3901	3904	rBV3	577	685	0.05%	0.006%




Sum of corrected areas: 10904048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026602.D
Acq On : 30 Jun 2022 13:08
Operator : SY/MD
Sample : N3521-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COJW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

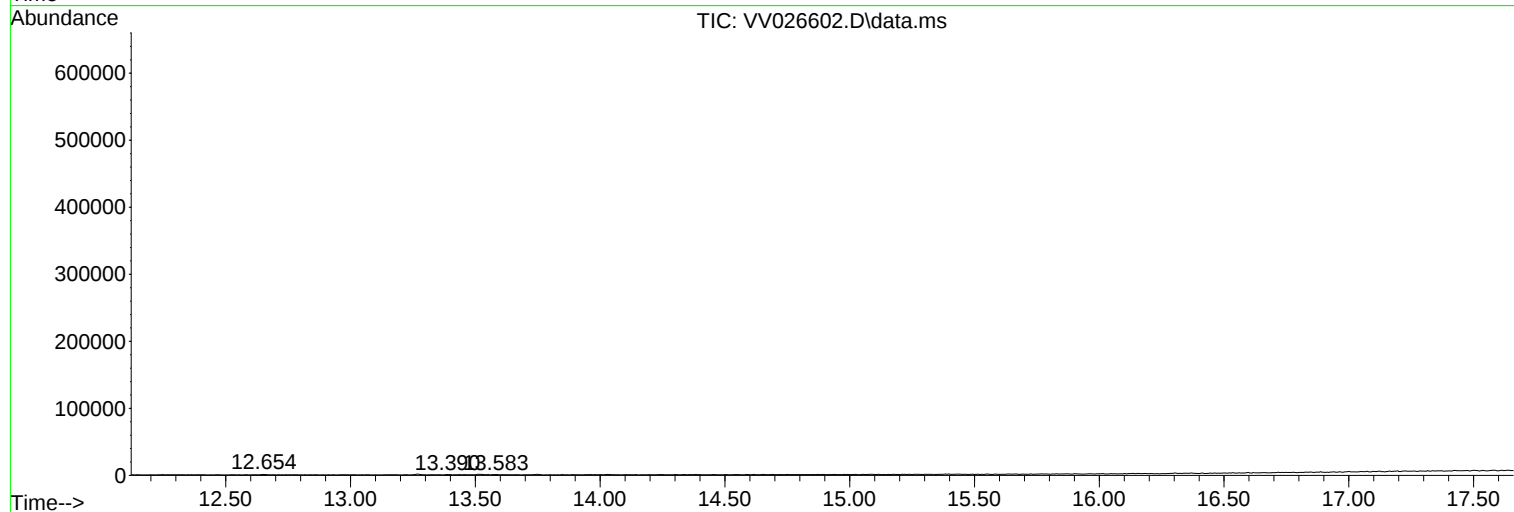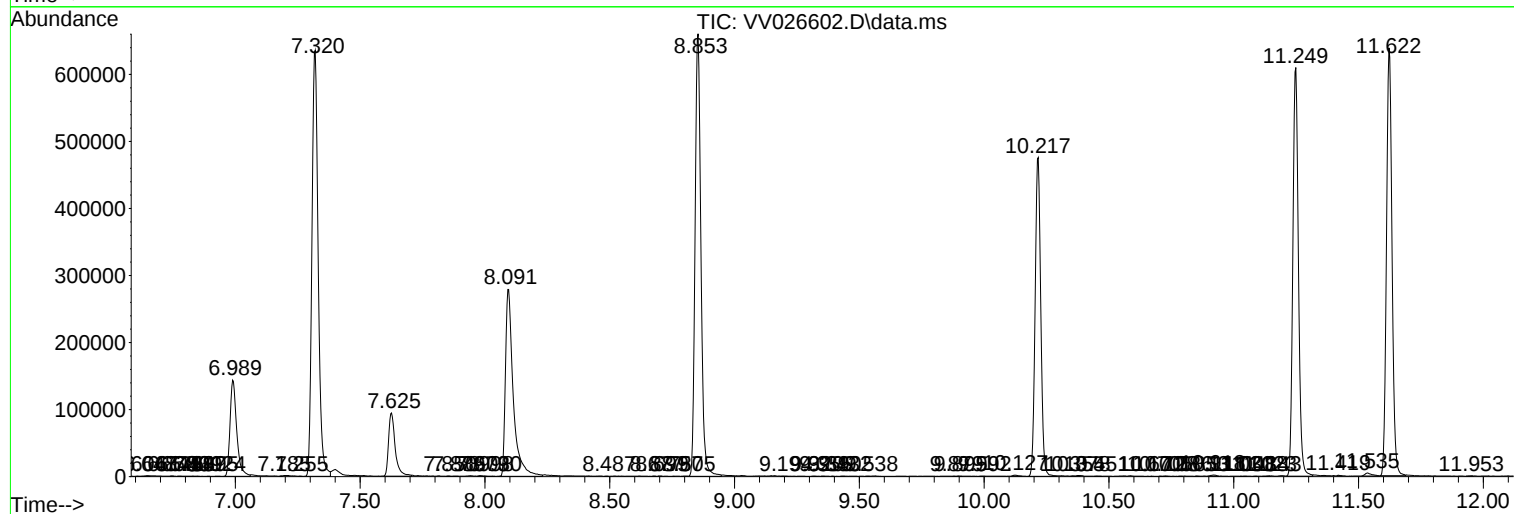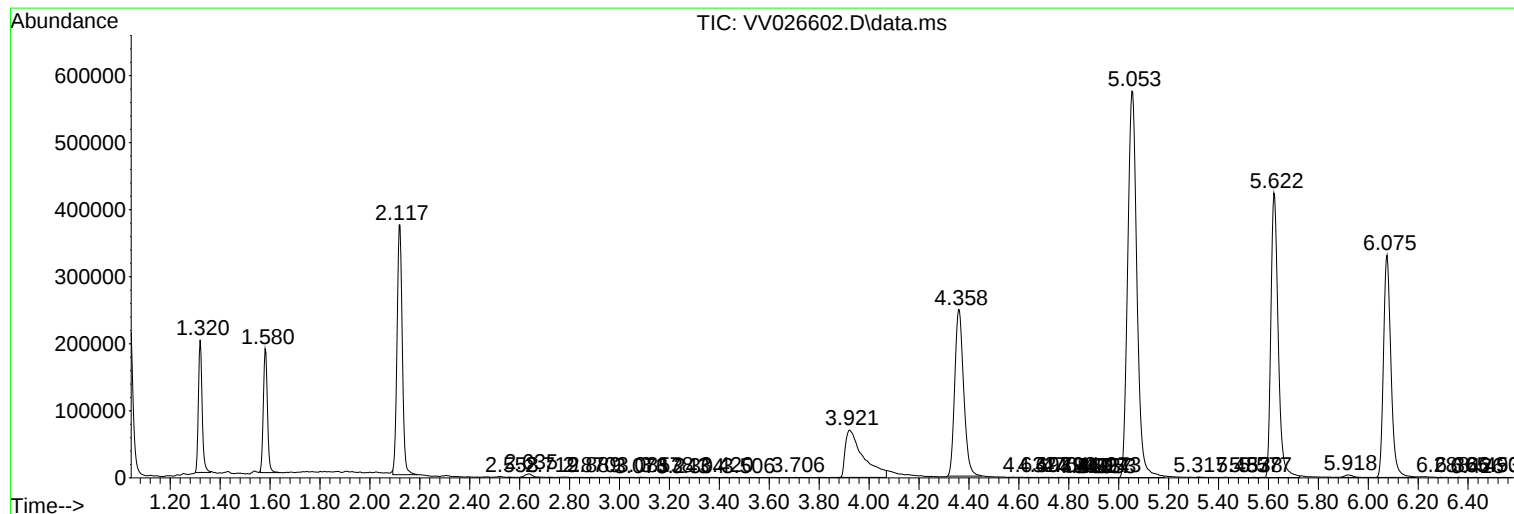

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026602.D
Acq On : 30 Jun 2022 13:08
Operator : SY/MD
Sample : N3521-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026602.D
Acq On : 30 Jun 2022 13:08
Operator : SY/MD
Sample : N3521-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc