

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026603.D
 Acq On : 30 Jun 2022 13:32
 Operator : SY/MD
 Sample : N3521-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	103	rBV	199999	213766	14.16%	1.932%
2	1.581	162	168	184	rVB	188138	216189	14.32%	1.954%
3	2.121	327	336	355	rVB	378827	543965	36.02%	4.916%
4	2.722	521	523	526	rVB2	216	85	0.01%	0.001%
5	2.999	606	609	611	rBV2	225	174	0.01%	0.002%
6	3.217	671	677	680	rBV2	224	289	0.02%	0.003%
7	3.346	714	717	718	rBV2	181	101	0.01%	0.001%
8	3.439	743	746	750	rVB	217	147	0.01%	0.001%
9	3.590	790	793	794	rBV	278	112	0.01%	0.001%
10	3.716	830	832	835	rBV2	161	95	0.01%	0.001%
11	3.780	850	852	854	rBV3	173	103	0.01%	0.001%
12	3.867	876	879	882	rBV	225	168	0.01%	0.002%
13	3.925	882	897	955	rBV2	77367	396863	26.28%	3.587%
14	4.362	1018	1033	1061	rBV	253132	618543	40.96%	5.590%
15	4.671	1125	1129	1132	rBV4	592	496	0.03%	0.004%
16	4.796	1166	1168	1169	rBV4	201	93	0.01%	0.001%
17	4.834	1177	1180	1182	rBV	209	94	0.01%	0.001%
18	4.854	1182	1186	1188	rVV2	249	202	0.01%	0.002%
19	4.873	1190	1192	1194	rVB	183	75	0.00%	0.001%
20	4.889	1195	1197	1198	rBV	204	72	0.00%	0.001%
21	4.963	1217	1220	1224	rBV3	328	273	0.02%	0.002%
22	4.995	1228	1230	1232	rBV	139	47	0.00%	0.000%
23	5.056	1232	1249	1289	rBV2	591181	1509987	100.00%	13.646%
24	5.413	1356	1360	1361	rBV2	579	280	0.02%	0.003%
25	5.487	1381	1383	1385	rVB	261	102	0.01%	0.001%
26	5.539	1397	1399	1400	rBV	193	92	0.01%	0.001%
27	5.564	1404	1407	1409	rBV	381	285	0.02%	0.003%
28	5.625	1413	1426	1457	rBV	420819	857355	56.78%	7.748%
29	5.982	1534	1537	1542	rBV2	472	347	0.02%	0.003%
30	6.076	1552	1566	1593	rBV	342139	693699	45.94%	6.269%
31	6.272	1625	1627	1629	rBV2	309	160	0.01%	0.001%
32	6.326	1642	1644	1649	rBV4	406	398	0.03%	0.004%
33	6.381	1658	1661	1663	rBV	240	136	0.01%	0.001%
34	6.400	1665	1667	1670	rVV	360	164	0.01%	0.001%
35	6.413	1670	1671	1676	rVB2	258	166	0.01%	0.002%
36	6.449	1681	1682	1683	rVB2	107	21	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026603.D
 Acq On : 30 Jun 2022 13:32
 Operator : SY/MD
 Sample : N3521-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	6.481	1690	1692	1694	rBV	148	88	0.01%	0.001%
38	6.510	1698	1701	1704	rBV2	404	299	0.02%	0.003%
39	6.561	1712	1717	1718	rBV2	413	283	0.02%	0.003%
40	6.641	1737	1742	1746	rBV4	866	1020	0.07%	0.009%
41	6.805	1792	1793	1794	rVB4	86	17	0.00%	0.000%
42	6.886	1815	1818	1822	rVB2	186	114	0.01%	0.001%
43	6.989	1839	1850	1872	rBV2	146560	271790	18.00%	2.456%
44	7.262	1933	1935	1937	rBV	265	133	0.01%	0.001%
45	7.320	1941	1953	1972	rBV	641154	1121277	74.26%	10.133%
46	7.625	2039	2048	2083	rVB	96807	176090	11.66%	1.591%
47	7.821	2108	2109	2111	rVB2	242	87	0.01%	0.001%
48	7.838	2111	2114	2117	rBV2	261	185	0.01%	0.002%
49	7.892	2129	2131	2134	rBV	253	177	0.01%	0.002%
50	7.940	2142	2146	2148	rBV3	881	660	0.04%	0.006%
51	8.095	2184	2194	2226	rBV2	311789	641343	42.47%	5.796%
52	8.551	2334	2336	2339	rVB	333	139	0.01%	0.001%
53	8.616	2354	2356	2363	rVB2	630	497	0.03%	0.004%
54	8.674	2373	2374	2375	rBV	220	46	0.00%	0.000%
55	8.722	2386	2389	2391	rBV2	440	279	0.02%	0.003%
56	8.854	2418	2430	2455	rBV	651864	1066936	70.66%	9.642%
57	9.082	2496	2501	2504	rBV3	378	371	0.02%	0.003%
58	9.124	2511	2514	2516	rBV2	490	291	0.02%	0.003%
59	9.252	2552	2554	2559	rVB	256	156	0.01%	0.001%
60	9.310	2568	2572	2575	rBV2	285	241	0.02%	0.002%
61	9.355	2584	2586	2587	rBV2	192	67	0.00%	0.001%
62	9.403	2599	2601	2603	rBV2	209	87	0.01%	0.001%
63	9.458	2616	2618	2620	rBV	294	149	0.01%	0.001%
64	9.513	2634	2635	2639	rBV	145	74	0.00%	0.001%
65	9.583	2655	2657	2660	rBV2	279	180	0.01%	0.002%
66	9.770	2711	2715	2720	rBV2	392	289	0.02%	0.003%
67	9.934	2763	2766	2770	rVB3	349	194	0.01%	0.002%
68	10.127	2821	2826	2833	rVB3	1371	1655	0.11%	0.015%
69	10.217	2841	2854	2874	rBV	492536	769641	50.97%	6.955%
70	10.590	2965	2970	2971	rBV	459	373	0.02%	0.003%
71	10.616	2977	2978	2979	rVB	132	25	0.00%	0.000%
72	10.628	2979	2982	2987	rBV2	278	312	0.02%	0.003%
73	11.143	3139	3142	3143	rBV	441	219	0.01%	0.002%
74	11.185	3154	3155	3156	rBV	248	87	0.01%	0.001%
75	11.249	3163	3175	3198	rBV	606106	940837	62.31%	8.503%
76	11.390	3217	3219	3226	rBV5	679	680	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026603.D
Acq On : 30 Jun 2022 13:32
Operator : SY/MD
Sample : N3521-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JW6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Title : VOC Analysis

77	11.535	3256	3264	3279	rBV2	7826	14661	0.97%	0.132%
78	11.622	3280	3291	3313	rVV	642414	997149	66.04%	9.011%
79	13.268	3798	3803	3808	rBV3	1076	1072	0.07%	0.010%




Sum of corrected areas: 11065414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026603.D
Acq On : 30 Jun 2022 13:32
Operator : SY/MD
Sample : N3521-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COJW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

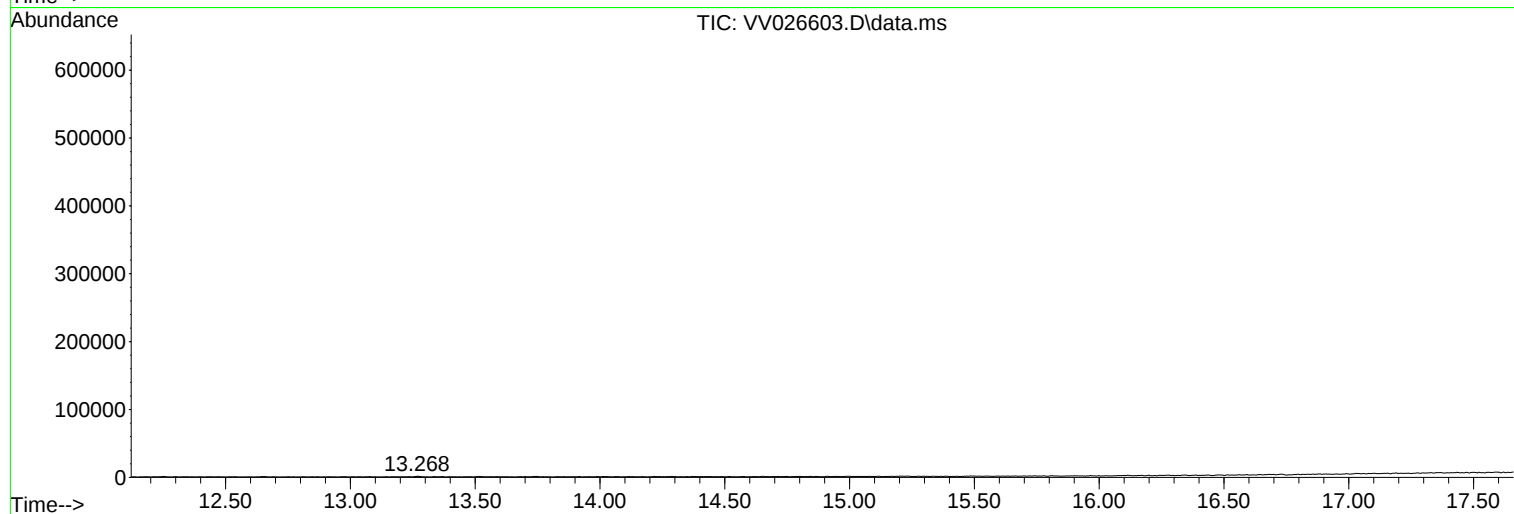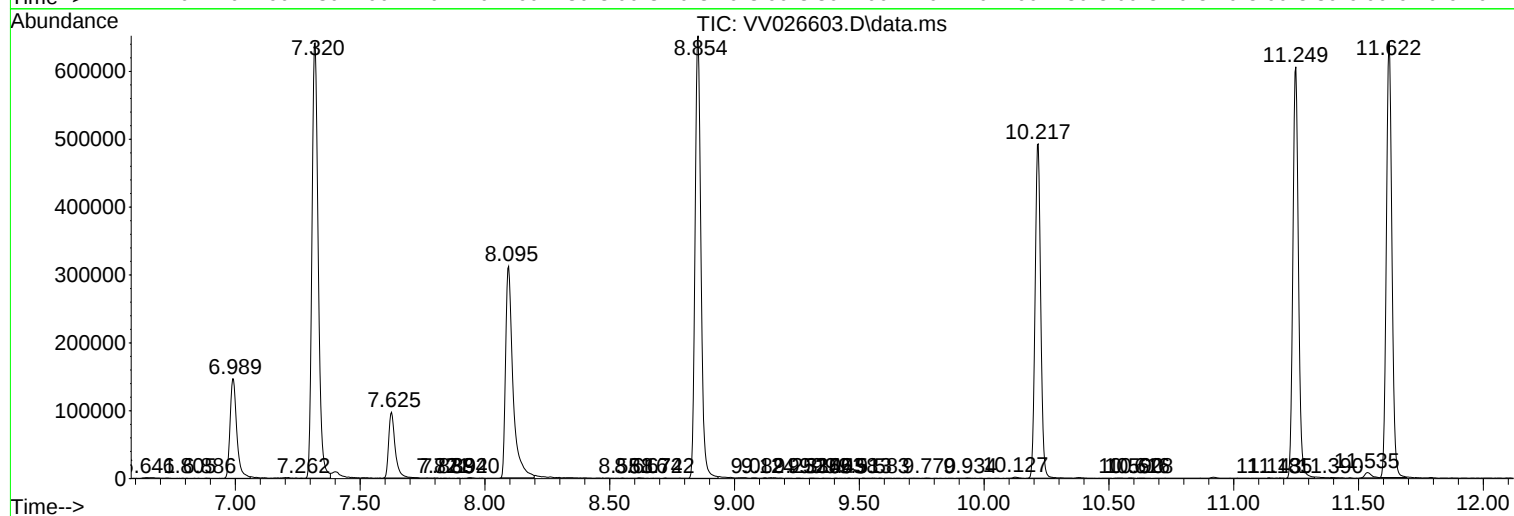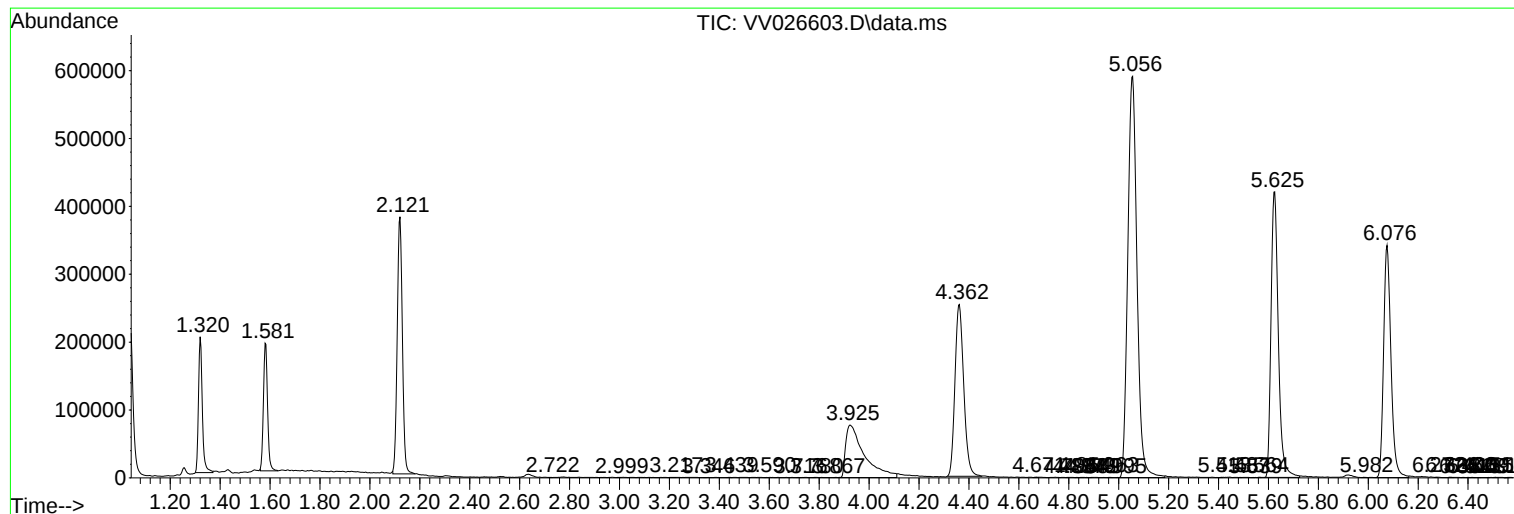

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026603.D
Acq On : 30 Jun 2022 13:32
Operator : SY/MD
Sample : N3521-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026603.D
Acq On : 30 Jun 2022 13:32
Operator : SY/MD
Sample : N3521-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc