

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026604.D
 Acq On : 30 Jun 2022 13:55
 Operator : SY/MD
 Sample : N3521-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	104	rBV	195493	207211	13.83%	1.900%
2	1.584	162	169	185	rVB	185328	212419	14.18%	1.948%
3	2.121	327	336	364	rVB	383942	556676	37.15%	5.105%
4	2.455	437	440	442	rBV3	784	463	0.03%	0.004%
5	2.638	484	497	509	rBV	4929	10297	0.69%	0.094%
6	2.780	539	541	543	rVB	418	169	0.01%	0.002%
7	2.790	543	544	547	rBV2	258	166	0.01%	0.002%
8	2.876	568	571	573	rBV2	340	219	0.01%	0.002%
9	2.912	580	582	588	rVB2	323	282	0.02%	0.003%
10	3.130	648	650	652	rBV	177	66	0.00%	0.001%
11	3.404	732	735	739	rVB3	317	166	0.01%	0.002%
12	3.484	757	760	764	rBV3	318	218	0.01%	0.002%
13	3.606	796	798	803	rBV	154	123	0.01%	0.001%
14	3.674	815	819	821	rBV	179	122	0.01%	0.001%
15	3.764	844	847	852	rVB	253	226	0.02%	0.002%
16	3.790	852	855	858	rBV	301	196	0.01%	0.002%
17	3.860	875	877	880	rBV	129	74	0.00%	0.001%
18	3.880	880	883	885	rBV2	294	222	0.01%	0.002%
19	3.925	885	897	937	rBV2	71226	342330	22.85%	3.139%
20	4.362	1018	1033	1056	rBV	254192	617950	41.24%	5.667%
21	4.683	1131	1133	1134	rBV	199	80	0.01%	0.001%
22	4.761	1155	1157	1160	rVB2	417	233	0.02%	0.002%
23	4.783	1163	1164	1167	rVV	217	89	0.01%	0.001%
24	4.796	1167	1168	1170	rVV	214	80	0.01%	0.001%
25	4.822	1173	1176	1177	rBV	270	131	0.01%	0.001%
26	4.831	1177	1179	1181	rVV2	266	151	0.01%	0.001%
27	4.860	1184	1188	1190	rVB2	264	178	0.01%	0.002%
28	4.905	1199	1202	1205	rBV2	192	116	0.01%	0.001%
29	4.966	1218	1221	1224	rBV3	280	163	0.01%	0.001%
30	5.056	1232	1249	1281	rBV2	588169	1498453	100.00%	13.741%
31	5.326	1331	1333	1341	rVB4	403	416	0.03%	0.004%
32	5.375	1346	1348	1349	rBV2	295	90	0.01%	0.001%
33	5.404	1355	1357	1358	rBV2	252	134	0.01%	0.001%
34	5.503	1385	1388	1391	rBV2	468	336	0.02%	0.003%
35	5.545	1398	1401	1404	rBV2	155	100	0.01%	0.001%
36	5.571	1404	1409	1412	rBV2	223	177	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026604.D
 Acq On : 30 Jun 2022 13:55
 Operator : SY/MD
 Sample : N3521-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	5.625	1412	1426	1451	rBV	415760	838128	55.93%	7.686%
38	5.921	1508	1518	1521	rBV4	3674	5015	0.33%	0.046%
39	5.989	1535	1539	1543	rBV2	338	315	0.02%	0.003%
40	6.076	1553	1566	1593	rBV	338823	685054	45.72%	6.282%
41	6.301	1632	1636	1639	rVB2	332	254	0.02%	0.002%
42	6.413	1669	1671	1674	rBV	204	88	0.01%	0.001%
43	6.436	1674	1678	1680	rBV3	253	214	0.01%	0.002%
44	6.503	1696	1699	1700	rVB	292	113	0.01%	0.001%
45	6.561	1715	1717	1719	rVB3	374	95	0.01%	0.001%
46	6.613	1729	1733	1736	rBV2	403	314	0.02%	0.003%
47	6.645	1740	1743	1750	rBV5	851	1043	0.07%	0.010%
48	6.812	1792	1795	1798	rVB	214	132	0.01%	0.001%
49	6.915	1824	1827	1831	rBV	182	175	0.01%	0.002%
50	6.992	1840	1851	1876	rBV	142996	269975	18.02%	2.476%
51	7.111	1886	1888	1892	rBV4	425	223	0.01%	0.002%
52	7.320	1940	1953	1972	rBV	638250	1119540	74.71%	10.267%
53	7.625	2038	2048	2073	rBV	99548	176710	11.79%	1.621%
54	7.812	2105	2106	2111	rVV3	588	337	0.02%	0.003%
55	7.860	2119	2121	2125	rBV3	434	252	0.02%	0.002%
56	7.879	2125	2127	2132	rVB4	363	258	0.02%	0.002%
57	7.941	2139	2146	2148	rBV3	695	784	0.05%	0.007%
58	8.024	2166	2172	2176	rVB3	283	295	0.02%	0.003%
59	8.053	2178	2181	2184	rBV2	158	110	0.01%	0.001%
60	8.095	2184	2194	2231	rBV2	292797	616912	41.17%	5.657%
61	8.532	2327	2330	2331	rBV2	201	114	0.01%	0.001%
62	8.603	2350	2352	2353	rBV2	376	140	0.01%	0.001%
63	8.625	2356	2359	2364	rBV3	434	366	0.02%	0.003%
64	8.661	2368	2370	2373	rVB	340	135	0.01%	0.001%
65	8.677	2373	2375	2379	rBV2	181	122	0.01%	0.001%
66	8.699	2380	2382	2384	rVB	203	101	0.01%	0.001%
67	8.715	2384	2387	2389	rBV2	273	213	0.01%	0.002%
68	8.770	2401	2404	2405	rBV2	207	110	0.01%	0.001%
69	8.854	2417	2430	2459	rBV	658441	1053993	70.34%	9.666%
70	9.156	2517	2524	2529	rBV3	1008	1212	0.08%	0.011%
71	9.230	2544	2547	2551	rBV2	248	219	0.01%	0.002%
72	9.249	2551	2553	2554	rVV2	365	142	0.01%	0.001%
73	9.272	2558	2560	2562	rBV	251	122	0.01%	0.001%
74	9.362	2585	2588	2591	rBV2	394	222	0.01%	0.002%
75	9.416	2603	2605	2608	rVB3	374	174	0.01%	0.002%
76	9.458	2616	2618	2619	rBV	293	101	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026604.D
 Acq On : 30 Jun 2022 13:55
 Operator : SY/MD
 Sample : N3521-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	9.500	2629	2631	2632	rBV	223	74	0.00%	0.001%
78	9.513	2633	2635	2638	rVV	314	197	0.01%	0.002%
79	9.542	2642	2644	2646	rVB2	170	73	0.00%	0.001%
80	9.555	2646	2648	2652	rBV3	362	273	0.02%	0.003%
81	9.606	2661	2664	2665	rBV3	326	208	0.01%	0.002%
82	9.641	2671	2675	2676	rBV3	304	231	0.02%	0.002%
83	9.677	2683	2686	2690	rBV3	307	230	0.02%	0.002%
84	9.857	2740	2742	2745	rBV	147	65	0.00%	0.001%
85	9.992	2782	2784	2785	rBV	195	95	0.01%	0.001%
86	10.050	2799	2802	2804	rBV	188	110	0.01%	0.001%
87	10.156	2833	2835	2839	rBV	261	134	0.01%	0.001%
88	10.217	2841	2854	2877	rBV	481523	756572	50.49%	6.938%
89	10.381	2898	2905	2914	rVB6	1184	2008	0.13%	0.018%
90	10.420	2915	2917	2918	rBV	179	79	0.01%	0.001%
91	10.847	3048	3050	3053	rBV	280	133	0.01%	0.001%
92	11.130	3137	3138	3139	rBV	255	91	0.01%	0.001%
93	11.249	3163	3175	3196	rBV	589655	924623	61.71%	8.479%
94	11.538	3259	3265	3276	rVB7	1843	3459	0.23%	0.032%
95	11.622	3280	3291	3320	rVV	644077	990297	66.09%	9.081%
96	12.034	3413	3419	3420	rBV	363	341	0.02%	0.003%
97	12.284	3495	3497	3498	rBV	322	107	0.01%	0.001%
98	12.362	3518	3521	3524	rBV	389	238	0.02%	0.002%
99	12.468	3551	3554	3556	rBV	348	238	0.02%	0.002%
100	12.522	3568	3571	3575	rBV2	463	386	0.03%	0.004%



Sum of corrected areas: 10904606

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026604.D
Acq On : 30 Jun 2022 13:55
Operator : SY/MD
Sample : N3521-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

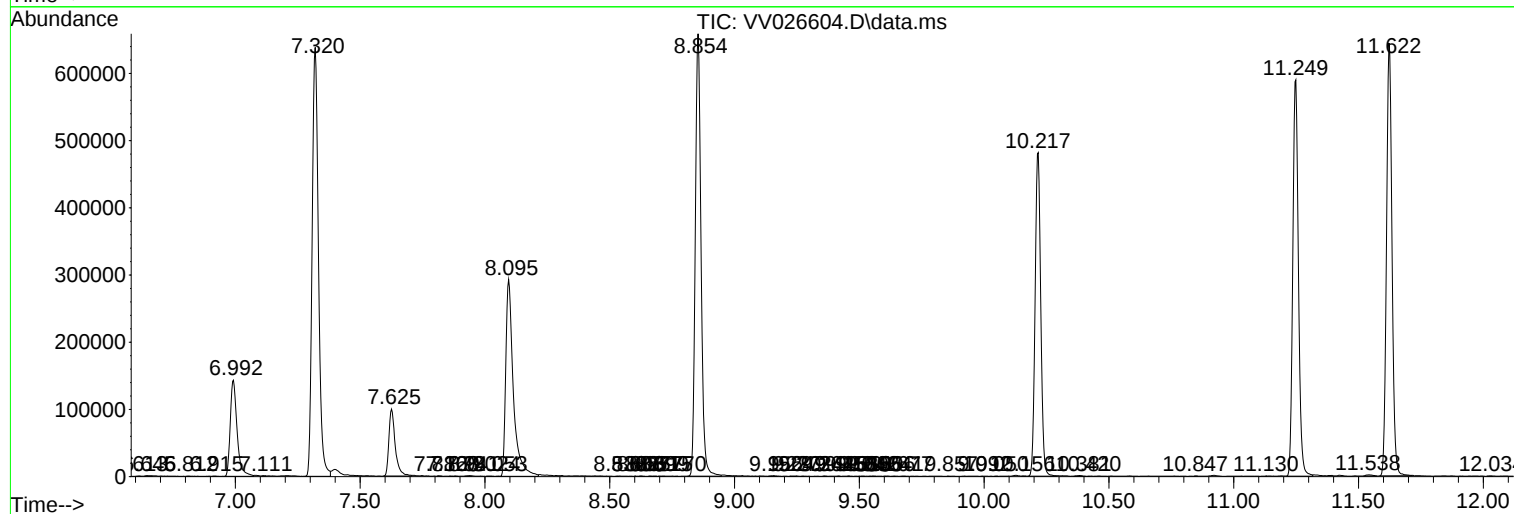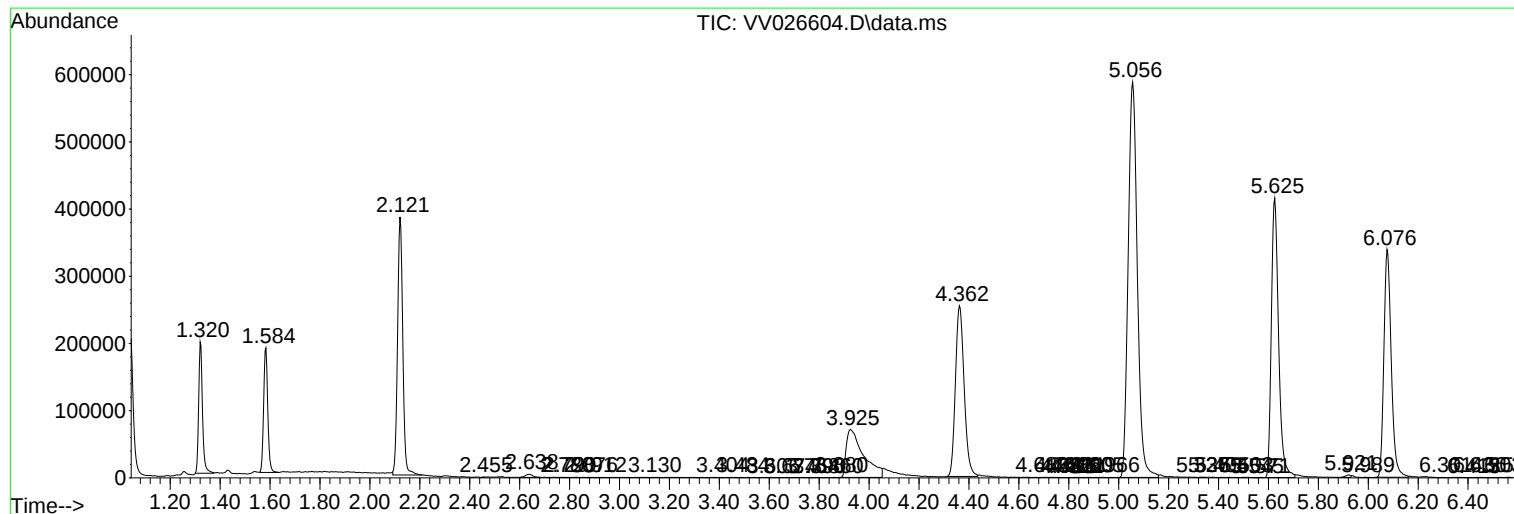

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026604.D
Acq On : 30 Jun 2022 13:55
Operator : SY/MD
Sample : N3521-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026604.D
Acq On : 30 Jun 2022 13:55
Operator : SY/MD
Sample : N3521-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc