

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026605.D
 Acq On : 30 Jun 2022 14:20
 Operator : SY/MD
 Sample : N3521-13DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	101	rBV	186002	197389	12.04%	1.702%
2	1.580	161	168	183	rVB	179017	201968	12.32%	1.741%
3	2.117	326	335	363	rVB	357114	522946	31.91%	4.509%
4	2.433	431	433	435	rBV	404	161	0.01%	0.001%
5	2.449	435	438	441	rBV2	511	366	0.02%	0.003%
6	2.519	452	460	473	rVB2	8446	13703	0.84%	0.118%
7	2.674	506	508	511	rBV	191	97	0.01%	0.001%
8	2.767	533	537	545	rBV2	638	687	0.04%	0.006%
9	3.288	695	699	703	rBV2	224	155	0.01%	0.001%
10	3.314	704	707	711	rBV2	300	255	0.02%	0.002%
11	3.410	734	737	740	rBV2	273	210	0.01%	0.002%
12	3.461	751	753	755	rBV	165	61	0.00%	0.001%
13	3.535	774	776	779	rVB	259	112	0.01%	0.001%
14	3.555	780	782	785	rVV2	213	116	0.01%	0.001%
15	3.593	792	794	798	rVB3	209	148	0.01%	0.001%
16	3.703	826	828	833	rVB3	300	146	0.01%	0.001%
17	3.770	845	849	851	rBV	315	214	0.01%	0.002%
18	3.789	853	855	858	rVB	282	115	0.01%	0.001%
19	3.825	863	866	868	rBV	230	118	0.01%	0.001%
20	3.915	884	894	924	rBV2	59859	231713	14.14%	1.998%
21	4.358	1017	1032	1059	rBV	240146	589681	35.98%	5.084%
22	4.625	1113	1115	1120	rVB3	389	242	0.01%	0.002%
23	4.776	1158	1162	1167	rBV3	454	527	0.03%	0.005%
24	4.799	1167	1169	1173	rVB2	264	184	0.01%	0.002%
25	4.886	1193	1196	1197	rBV	156	96	0.01%	0.001%
26	4.928	1207	1209	1214	rVB2	168	127	0.01%	0.001%
27	5.053	1232	1248	1263	rBV2	555124	1425882	87.01%	12.293%
28	5.413	1356	1360	1362	rBV2	582	471	0.03%	0.004%
29	5.490	1382	1384	1386	rBV3	231	142	0.01%	0.001%
30	5.529	1393	1396	1398	rVB2	287	154	0.01%	0.001%
31	5.622	1413	1425	1454	rBV	382621	775545	47.32%	6.686%
32	5.918	1508	1517	1533	rVB7	3241	7272	0.44%	0.063%
33	5.998	1540	1542	1544	rBV	415	222	0.01%	0.002%
34	6.024	1547	1550	1552	rBV	277	173	0.01%	0.001%
35	6.075	1552	1566	1599	rBV	318107	658290	40.17%	5.675%
36	6.272	1625	1627	1631	rVB3	470	326	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026605.D
 Acq On : 30 Jun 2022 14:20
 Operator : SY/MD
 Sample : N3521-13DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	6.307	1636	1638	1639	rBV3	339	132	0.01%	0.001%
38	6.326	1640	1644	1648	rVB2	351	248	0.02%	0.002%
39	6.358	1649	1654	1659	rVB3	437	411	0.03%	0.004%
40	6.387	1659	1663	1665	rBV	249	156	0.01%	0.001%
41	6.400	1665	1667	1669	rVB	234	89	0.01%	0.001%
42	6.465	1683	1687	1690	rVB2	354	232	0.01%	0.002%
43	6.510	1698	1701	1702	rBV2	320	152	0.01%	0.001%
44	6.545	1709	1712	1714	rBV	311	255	0.02%	0.002%
45	6.648	1736	1744	1747	rBV6	880	1159	0.07%	0.010%
46	6.738	1770	1772	1773	rBV6	155	65	0.00%	0.001%
47	6.812	1794	1795	1798	rVB	233	91	0.01%	0.001%
48	6.831	1798	1801	1802	rBV	191	87	0.01%	0.001%
49	6.989	1839	1850	1878	rBV	136248	254343	15.52%	2.193%
50	7.320	1941	1953	1971	rBV	597283	1037864	63.33%	8.948%
51	7.625	2038	2048	2069	rBV	92724	166732	10.17%	1.437%
52	7.821	2106	2109	2110	rBV	220	128	0.01%	0.001%
53	7.844	2114	2116	2119	rVB3	449	273	0.02%	0.002%
54	7.863	2119	2122	2123	rBV2	415	263	0.02%	0.002%
55	7.937	2138	2145	2146	rBV3	615	540	0.03%	0.005%
56	7.982	2156	2159	2160	rBV2	261	120	0.01%	0.001%
57	8.040	2175	2177	2179	rBV3	144	79	0.00%	0.001%
58	8.053	2179	2181	2183	rBV2	223	114	0.01%	0.001%
59	8.095	2183	2194	2231	rBV2	278988	600058	36.62%	5.173%
60	8.487	2313	2316	2317	rBV2	360	174	0.01%	0.002%
61	8.542	2330	2333	2336	rVB2	342	253	0.02%	0.002%
62	8.587	2344	2347	2349	rBV2	407	244	0.01%	0.002%
63	8.622	2356	2358	2364	rBV3	391	259	0.02%	0.002%
64	8.673	2371	2374	2379	rVB2	354	231	0.01%	0.002%
65	8.767	2400	2403	2406	rVB2	333	213	0.01%	0.002%
66	8.783	2406	2408	2412	rVB2	217	140	0.01%	0.001%
67	8.853	2418	2430	2434	rBV	638500	990915	60.47%	8.543%
68	9.152	2515	2523	2526	rBV5	971	1554	0.09%	0.013%
69	9.201	2536	2538	2541	rBV	256	172	0.01%	0.001%
70	9.236	2547	2549	2550	rBV	198	86	0.01%	0.001%
71	9.349	2581	2584	2586	rBV	166	105	0.01%	0.001%
72	9.551	2645	2647	2655	rVB4	448	415	0.03%	0.004%
73	9.779	2715	2718	2722	rBV2	303	251	0.02%	0.002%
74	9.805	2722	2726	2728	rBV2	207	160	0.01%	0.001%
75	9.908	2756	2758	2761	rBV2	273	147	0.01%	0.001%
76	10.217	2841	2854	2874	rBV	463941	737666	45.01%	6.360%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026605.D
 Acq On : 30 Jun 2022 14:20
 Operator : SY/MD
 Sample : N3521-13DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	10.429	2917	2920	2922	rBV2	375	219	0.01%	0.002%
78	10.506	2940	2944	2949	rBV2	282	322	0.02%	0.003%
79	10.545	2953	2956	2961	rVB3	699	608	0.04%	0.005%
80	10.580	2962	2967	2969	rBV3	501	468	0.03%	0.004%
81	10.725	3009	3012	3014	rBV	246	164	0.01%	0.001%
82	10.799	3031	3035	3039	rBV3	487	492	0.03%	0.004%
83	10.876	3058	3059	3060	rBV3	138	40	0.00%	0.000%
84	10.921	3065	3073	3080	rVB6	1822	2726	0.17%	0.024%
85	10.950	3080	3082	3083	rBV6	223	109	0.01%	0.001%
86	11.185	3145	3155	3164	rBV	35809	55567	3.39%	0.479%
87	11.249	3164	3175	3206	rVB2	606232	1363674	83.21%	11.757%
88	11.548	3264	3268	3273	rBV4	644	691	0.04%	0.006%
89	11.625	3279	3292	3325	rBV2	744011	1638820	100.00%	14.129%
90	12.947	3700	3703	3706	rBV2	439	342	0.02%	0.003%
91	13.262	3791	3801	3817	rBV2	56535	88868	5.42%	0.766%
92	13.744	3943	3951	3965	rBV3	12024	19148	1.17%	0.165%




Sum of corrected areas: 11598848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026605.D
Acq On : 30 Jun 2022 14:20
Operator : SY/MD
Sample : N3521-13DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

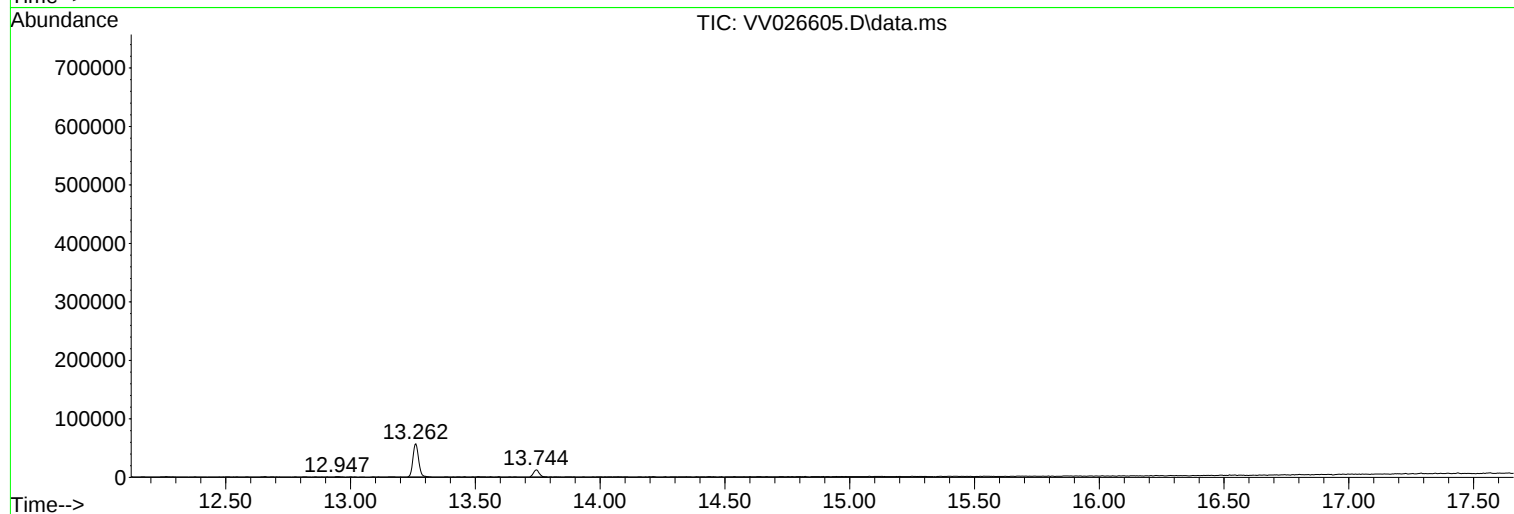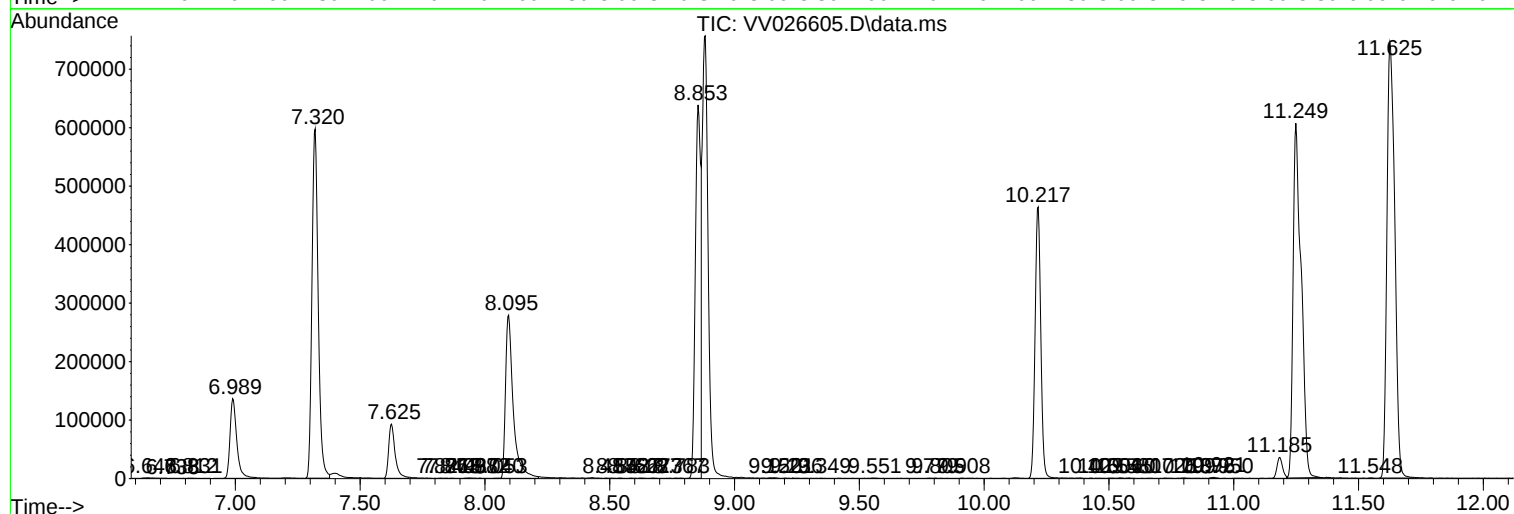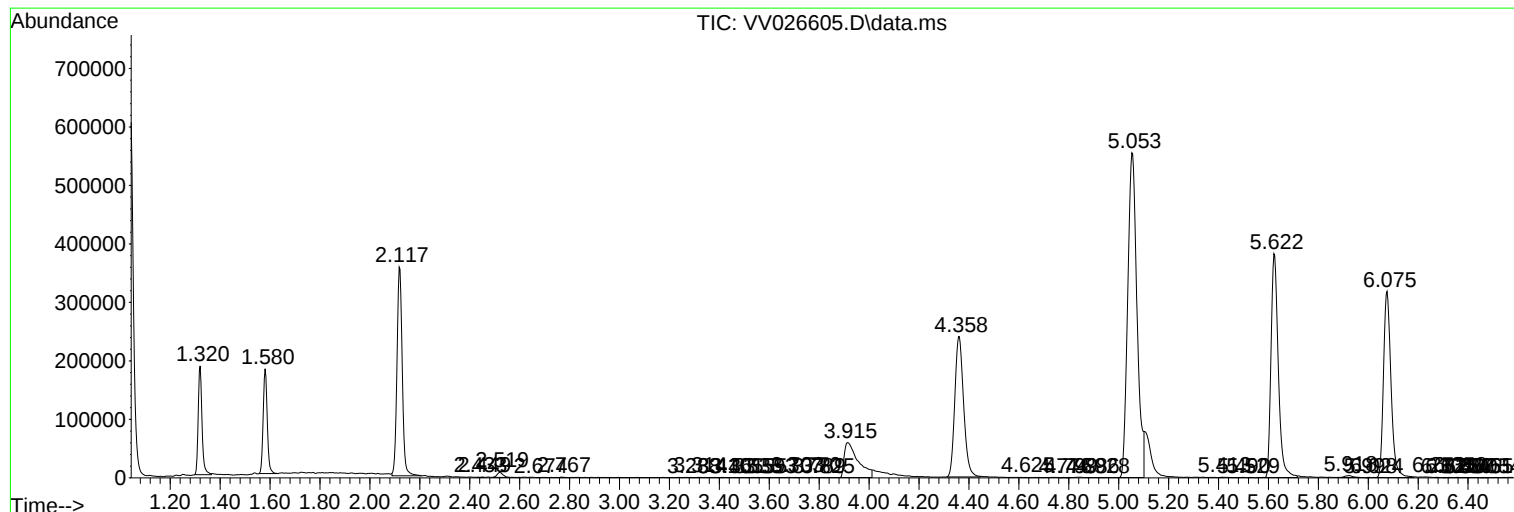

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026605.D
Acq On : 30 Jun 2022 14:20
Operator : SY/MD
Sample : N3521-13DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026605.D
Acq On : 30 Jun 2022 14:20
Operator : SY/MD
Sample : N3521-13DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc