

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026606.D
 Acq On : 30 Jun 2022 14:44
 Operator : SY/MD
 Sample : N3521-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M

Title : VOC Analysis

Signal : TIC: VV026606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	102	rBV	195925	207086	2.68%	0.808%
2	1.581	161	168	183	rBV	187692	215135	2.79%	0.839%
3	2.121	327	336	352	rVB	386523	550353	7.13%	2.147%
4	2.587	477	481	482	rBV2	455	267	0.00%	0.001%
5	2.709	516	519	520	rBV2	212	119	0.00%	0.000%
6	2.854	562	564	567	rBV3	304	149	0.00%	0.001%
7	2.883	570	573	574	rBV	248	117	0.00%	0.000%
8	2.921	582	585	586	rBV	202	129	0.00%	0.001%
9	2.960	595	597	599	rBV	190	110	0.00%	0.000%
10	3.079	631	634	637	rBV	201	118	0.00%	0.000%
11	3.156	656	658	661	rBV2	169	118	0.00%	0.000%
12	3.349	713	718	722	rBV	257	280	0.00%	0.001%
13	3.368	722	724	726	rBV	177	85	0.00%	0.000%
14	3.397	731	733	735	rBV	240	134	0.00%	0.001%
15	3.458	750	752	755	rVB2	191	89	0.00%	0.000%
16	3.529	773	774	782	rVB2	177	151	0.00%	0.001%
17	3.571	782	787	790	rBV	285	254	0.00%	0.001%
18	3.600	794	796	799	rVB	191	93	0.00%	0.000%
19	3.709	827	830	831	rBV	236	121	0.00%	0.000%
20	3.780	843	852	857	rBV6	1425	2249	0.03%	0.009%
21	3.915	884	894	964	rVV2	71342	346207	4.48%	1.350%
22	4.362	1017	1033	1059	rBV	257420	641068	8.30%	2.501%
23	4.751	1151	1154	1158	rBV2	218	220	0.00%	0.001%
24	4.838	1169	1181	1190	rBV6	2718	5826	0.08%	0.023%
25	4.953	1214	1217	1218	rBV	237	118	0.00%	0.000%
26	4.979	1223	1225	1227	rVB	206	86	0.00%	0.000%
27	4.992	1227	1229	1232	rVB	221	82	0.00%	0.000%
28	5.056	1232	1249	1258	rBV2	609219	1498545	19.41%	5.845%
29	5.342	1335	1338	1340	rBV2	556	355	0.00%	0.001%
30	5.413	1357	1360	1364	rBV4	579	385	0.00%	0.002%
31	5.442	1366	1369	1372	rBV2	313	218	0.00%	0.001%
32	5.474	1377	1379	1381	rBV2	250	144	0.00%	0.001%
33	5.490	1381	1384	1385	rBV2	185	102	0.00%	0.000%
34	5.510	1388	1390	1392	rBV2	284	136	0.00%	0.001%
35	5.551	1398	1403	1405	rBV	252	173	0.00%	0.001%
36	5.564	1405	1407	1408	rVB2	275	87	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026606.D
 Acq On : 30 Jun 2022 14:44
 Operator : SY/MD
 Sample : N3521-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	5.625	1411	1426	1450	rBV	433914	879981	11.40%	3.433%
38	5.924	1508	1519	1522	rBV6	3029	5180	0.07%	0.020%
39	5.979	1530	1536	1538	rBV4	309	313	0.00%	0.001%
40	6.014	1543	1547	1551	rBV2	275	305	0.00%	0.001%
41	6.076	1551	1566	1589	rBV	338850	699003	9.05%	2.727%
42	6.288	1630	1632	1635	rVB2	223	99	0.00%	0.000%
43	6.313	1635	1640	1645	rVB3	533	545	0.01%	0.002%
44	6.336	1645	1647	1648	rBV	255	85	0.00%	0.000%
45	6.346	1648	1650	1651	rBV	208	83	0.00%	0.000%
46	6.375	1656	1659	1660	rBV	162	96	0.00%	0.000%
47	6.423	1671	1674	1675	rBV	169	108	0.00%	0.000%
48	6.465	1684	1687	1692	rVB2	276	164	0.00%	0.001%
49	6.497	1692	1697	1701	rBV	178	177	0.00%	0.001%
50	6.519	1701	1704	1708	rVB3	227	146	0.00%	0.001%
51	6.542	1708	1711	1715	rBV3	471	336	0.00%	0.001%
52	6.625	1736	1737	1738	rBV	368	127	0.00%	0.000%
53	6.773	1781	1783	1786	rBV	239	125	0.00%	0.000%
54	6.815	1791	1796	1801	rBV2	353	319	0.00%	0.001%
55	6.928	1828	1831	1835	rBV	141	88	0.00%	0.000%
56	6.989	1840	1850	1870	rBV	148861	275604	3.57%	1.075%
57	7.320	1940	1953	1972	rBV	665881	1150225	14.90%	4.487%
58	7.584	2030	2035	2038	rBV2	416	423	0.01%	0.002%
59	7.625	2038	2048	2065	rBV	104034	179696	2.33%	0.701%
60	7.793	2097	2100	2103	rVV2	317	220	0.00%	0.001%
61	7.809	2103	2105	2108	rVB2	250	141	0.00%	0.001%
62	7.841	2113	2115	2117	rVB3	263	104	0.00%	0.000%
63	7.854	2117	2119	2120	rBV	252	106	0.00%	0.000%
64	7.908	2134	2136	2138	rVV2	188	80	0.00%	0.000%
65	8.095	2182	2194	2222	rBV2	334354	670527	8.69%	2.616%
66	8.477	2311	2313	2320	rVB2	586	386	0.01%	0.002%
67	8.519	2323	2326	2329	rBV4	508	321	0.00%	0.001%
68	8.616	2354	2356	2358	rBV2	187	109	0.00%	0.000%
69	8.657	2366	2369	2373	rBV2	308	306	0.00%	0.001%
70	8.728	2388	2391	2392	rBV	322	157	0.00%	0.001%
71	8.741	2392	2395	2397	rVV	264	140	0.00%	0.001%
72	8.773	2402	2405	2407	rBV2	248	176	0.00%	0.001%
73	8.879	2418	2438	2478	rBV2	4207046	7719910	100.00%	30.114%
74	9.416	2602	2605	2608	rVB2	325	177	0.00%	0.001%
75	9.442	2610	2613	2616	rVV2	592	364	0.00%	0.001%
76	9.468	2616	2621	2625	rVB3	473	482	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026606.D
 Acq On : 30 Jun 2022 14:44
 Operator : SY/MD
 Sample : N3521-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	9.497	2628	2630	2632	rVB2	395	133	0.00%	0.001%
78	9.526	2637	2639	2644	rVB3	449	272	0.00%	0.001%
79	9.551	2644	2647	2649	rBV	415	339	0.00%	0.001%
80	9.593	2658	2660	2663	rBV2	509	272	0.00%	0.001%
81	9.680	2683	2687	2689	rBV	454	302	0.00%	0.001%
82	9.818	2727	2730	2735	rBV	157	166	0.00%	0.001%
83	9.860	2740	2743	2747	rBV2	210	183	0.00%	0.001%
84	9.976	2776	2779	2783	rBV	281	255	0.00%	0.001%
85	10.130	2820	2827	2834	rVB5	1718	2293	0.03%	0.009%
86	10.214	2841	2853	2876	rBV	502711	802497	10.40%	3.130%
87	10.362	2897	2899	2902	rBV3	443	246	0.00%	0.001%
88	10.542	2952	2955	2957	rBV2	564	425	0.01%	0.002%
89	10.664	2991	2993	2997	rVB2	307	149	0.00%	0.001%
90	10.686	2998	3000	3004	rBV	225	169	0.00%	0.001%
91	10.744	3015	3018	3020	rBV2	229	183	0.00%	0.001%
92	10.773	3025	3027	3032	rVB	199	141	0.00%	0.001%
93	10.850	3049	3051	3052	rBV	231	112	0.00%	0.000%
94	10.918	3067	3072	3080	rVB5	1404	1707	0.02%	0.007%
95	11.104	3127	3130	3132	rBV2	264	179	0.00%	0.001%
96	11.181	3143	3154	3164	rBV	199386	307808	3.99%	1.201%
97	11.271	3165	3182	3206	rVB2	1939107	3939756	51.03%	15.368%
98	11.638	3279	3296	3322	rBV2	2560867	4844169	62.75%	18.896%
99	13.259	3789	3800	3818	rBV	363981	557632	7.22%	2.175%
100	13.744	3941	3951	3963	rBV	76530	118708	1.54%	0.463%



Sum of corrected areas: 25635939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026606.D
Acq On : 30 Jun 2022 14:44
Operator : SY/MD
Sample : N3521-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

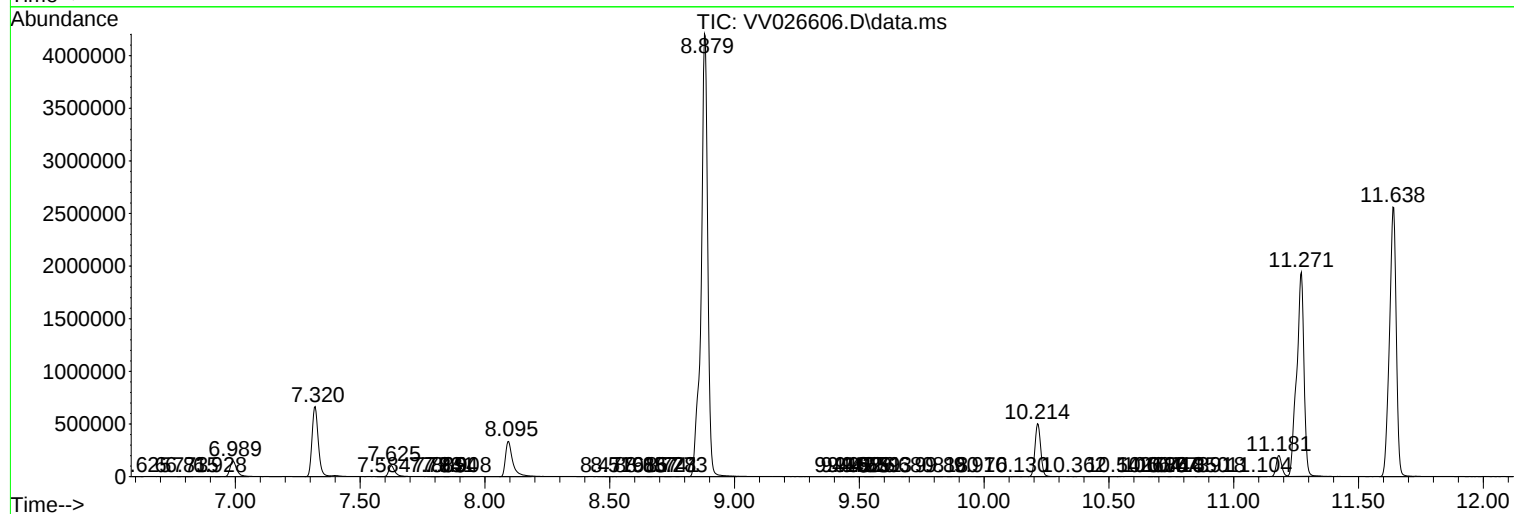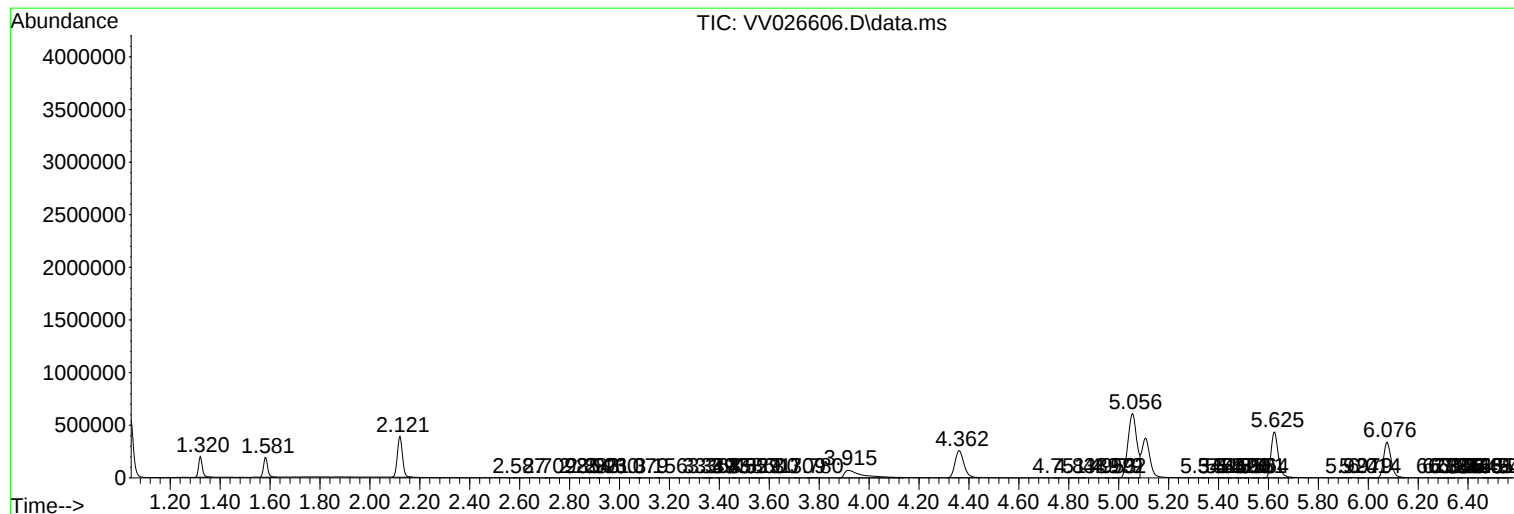

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026606.D
Acq On : 30 Jun 2022 14:44
Operator : SY/MD
Sample : N3521-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026606.D
Acq On : 30 Jun 2022 14:44
Operator : SY/MD
Sample : N3521-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
