

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026608.D
 Acq On : 30 Jun 2022 15:32
 Operator : SY/MD
 Sample : N3521-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JT3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	80	88	102	rBV	181846	201464	10.04%	1.624%
2	1.584	161	169	182	rBV	176997	201723	10.06%	1.626%
3	2.121	326	336	355	rVB	363090	517667	25.81%	4.172%
4	2.481	446	448	452	rVV2	508	320	0.02%	0.003%
5	2.523	455	461	473	rVB8	2288	4066	0.20%	0.033%
6	2.616	486	490	491	rBV2	644	431	0.02%	0.003%
7	2.632	491	495	501	rVV3	932	1054	0.05%	0.008%
8	2.790	541	544	547	rVV3	361	233	0.01%	0.002%
9	2.857	563	565	571	rVB3	437	345	0.02%	0.003%
10	2.941	586	591	594	rBV2	201	221	0.01%	0.002%
11	3.217	672	677	680	rBV2	283	268	0.01%	0.002%
12	3.327	705	711	712	rBV	273	236	0.01%	0.002%
13	3.545	776	779	783	rVB3	319	226	0.01%	0.002%
14	3.584	789	791	799	rVB2	269	306	0.02%	0.002%
15	3.773	846	850	858	rVB3	458	404	0.02%	0.003%
16	3.822	858	865	867	rBV2	262	268	0.01%	0.002%
17	3.915	883	894	931	rBV	66461	262689	13.10%	2.117%
18	4.362	1016	1033	1061	rBV	243229	602385	30.03%	4.855%
19	4.609	1105	1110	1116	rVB5	649	707	0.04%	0.006%
20	4.645	1118	1121	1124	rVB3	375	256	0.01%	0.002%
21	4.680	1124	1132	1136	rBV3	461	708	0.04%	0.006%
22	4.793	1163	1167	1173	rBV2	328	376	0.02%	0.003%
23	4.973	1219	1223	1226	rVB2	324	249	0.01%	0.002%
24	4.995	1226	1230	1233	rBV3	318	241	0.01%	0.002%
25	5.056	1233	1249	1295	rBV2	562981	1455083	72.54%	11.727%
26	5.420	1356	1362	1366	rBV4	557	548	0.03%	0.004%
27	5.564	1404	1407	1411	rVB2	314	233	0.01%	0.002%
28	5.625	1411	1426	1458	rBV	416257	849514	42.35%	6.847%
29	5.838	1489	1492	1493	rBV2	428	244	0.01%	0.002%
30	5.928	1509	1520	1526	rBV4	3042	6452	0.32%	0.052%
31	6.018	1545	1548	1553	rBV2	306	285	0.01%	0.002%
32	6.076	1553	1566	1597	rBV	326025	665320	33.17%	5.362%
33	6.336	1643	1647	1649	rVV2	336	224	0.01%	0.002%
34	6.455	1680	1684	1687	rVV2	307	243	0.01%	0.002%
35	6.645	1737	1743	1744	rBV	784	549	0.03%	0.004%
36	6.706	1761	1762	1767	rVB2	371	222	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026608.D
 Acq On : 30 Jun 2022 15:32
 Operator : SY/MD
 Sample : N3521-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JT3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	6.883	1812	1817	1821	rBV	420	430	0.02%	0.003%
38	6.992	1837	1851	1883	rBV	137250	263512	13.14%	2.124%
39	7.204	1909	1917	1926	rVB8	911	1638	0.08%	0.013%
40	7.320	1941	1953	1972	rBV	620779	1067585	53.22%	8.604%
41	7.558	2025	2027	2031	rVB3	455	283	0.01%	0.002%
42	7.625	2037	2048	2068	rBV	96138	173085	8.63%	1.395%
43	7.722	2076	2078	2085	rVB5	1054	979	0.05%	0.008%
44	7.992	2159	2162	2166	rBV3	351	306	0.02%	0.002%
45	8.095	2183	2194	2226	rBV2	289307	609990	30.41%	4.916%
46	8.497	2316	2319	2325	rVB2	443	423	0.02%	0.003%
47	8.567	2340	2341	2348	rVB3	469	388	0.02%	0.003%
48	8.606	2348	2353	2360	rBV4	433	568	0.03%	0.005%
49	8.635	2360	2362	2367	rVB2	396	267	0.01%	0.002%
50	8.786	2405	2409	2410	rBV2	446	268	0.01%	0.002%
51	8.854	2418	2430	2465	rBV2	657666	1260935	62.86%	10.163%
52	9.133	2514	2517	2518	rBV2	464	241	0.01%	0.002%
53	9.149	2518	2522	2525	rVV4	571	539	0.03%	0.004%
54	9.526	2634	2639	2641	rBV2	353	234	0.01%	0.002%
55	9.564	2648	2651	2655	rVB3	423	276	0.01%	0.002%
56	9.664	2677	2682	2685	rBV2	312	270	0.01%	0.002%
57	9.744	2703	2707	2713	rVV3	225	282	0.01%	0.002%
58	9.841	2733	2737	2739	rBV3	287	242	0.01%	0.002%
59	10.127	2817	2826	2835	rVB4	1714	2304	0.11%	0.019%
60	10.217	2841	2854	2875	rBV	480911	749877	37.38%	6.044%
61	10.342	2891	2893	2897	rVB3	347	225	0.01%	0.002%
62	10.384	2901	2906	2911	rVB4	704	812	0.04%	0.007%
63	10.471	2932	2933	2941	rVV2	317	290	0.01%	0.002%
64	10.577	2962	2966	2972	rBV5	654	705	0.04%	0.006%
65	10.702	3000	3005	3008	rVV2	258	247	0.01%	0.002%
66	10.776	3025	3028	3034	rVB	374	325	0.02%	0.003%
67	10.850	3047	3051	3053	rBV3	356	230	0.01%	0.002%
68	10.921	3061	3073	3080	rBV7	1721	2528	0.13%	0.020%
69	10.985	3090	3093	3098	rBV	330	277	0.01%	0.002%
70	11.185	3146	3155	3164	rBV2	22105	33275	1.66%	0.268%
71	11.249	3164	3175	3206	rVB	638469	1095660	54.62%	8.831%
72	11.429	3227	3231	3240	rVB7	1478	1900	0.09%	0.015%
73	11.468	3240	3243	3246	rBV3	336	231	0.01%	0.002%
74	11.545	3262	3267	3269	rVV2	588	384	0.02%	0.003%
75	11.632	3279	3294	3329	rBV2	849046	2005919	100.00%	16.167%
76	11.966	3394	3398	3402	rBV2	360	383	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026608.D
 Acq On : 30 Jun 2022 15:32
 Operator : SY/MD
 Sample : N3521-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JT3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M

Title : VOC Analysis

77	12.095	3434	3438	3447	rVB	614	615	0.03%	0.005%
78	12.291	3495	3499	3503	rBV2	248	308	0.02%	0.002%
79	12.368	3521	3523	3526	rBV2	330	260	0.01%	0.002%
80	12.403	3529	3534	3535	rBV	484	365	0.02%	0.003%
81	12.493	3559	3562	3568	rVB2	610	522	0.03%	0.004%
82	12.644	3601	3609	3622	rBV2	6279	11658	0.58%	0.094%
83	12.706	3625	3628	3632	rVV2	298	235	0.01%	0.002%
84	12.725	3632	3634	3638	rVB2	403	237	0.01%	0.002%
85	12.754	3639	3643	3648	rVB3	1090	1069	0.05%	0.009%
86	13.034	3723	3730	3733	rBV2	297	361	0.02%	0.003%
87	13.259	3790	3800	3818	rBV	136317	211568	10.55%	1.705%
88	13.355	3826	3830	3833	rBV2	376	256	0.01%	0.002%
89	13.503	3873	3876	3878	rBV2	444	311	0.02%	0.003%
90	13.664	3922	3926	3928	rBV	345	226	0.01%	0.002%
91	13.744	3939	3951	3964	rBV	70665	109414	5.45%	0.882%
92	14.050	4037	4046	4051	rBV4	760	1437	0.07%	0.012%
93	14.156	4073	4079	4092	rBV4	2198	3158	0.16%	0.025%
94	14.246	4101	4107	4111	rBV3	425	502	0.03%	0.004%
95	14.744	4258	4262	4269	rBV3	453	561	0.03%	0.005%
96	14.821	4280	4286	4290	rBV2	1460	1493	0.07%	0.012%
97	14.921	4313	4317	4322	rBV2	655	476	0.02%	0.004%
98	15.088	4367	4369	4374	rBV4	478	310	0.02%	0.002%
99	15.397	4458	4465	4473	rBV6	5357	7709	0.38%	0.062%
100	15.741	4570	4572	4577	rVB3	617	384	0.02%	0.003%



Sum of corrected areas: 12407508

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026608.D
Acq On : 30 Jun 2022 15:32
Operator : SY/MD
Sample : N3521-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

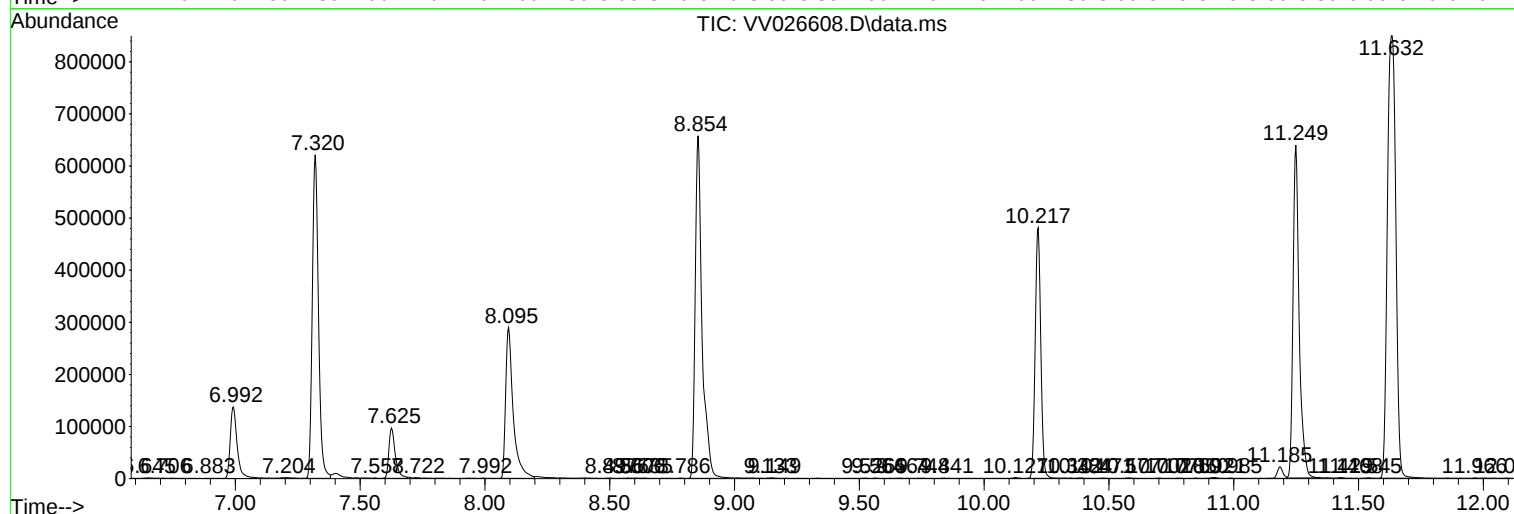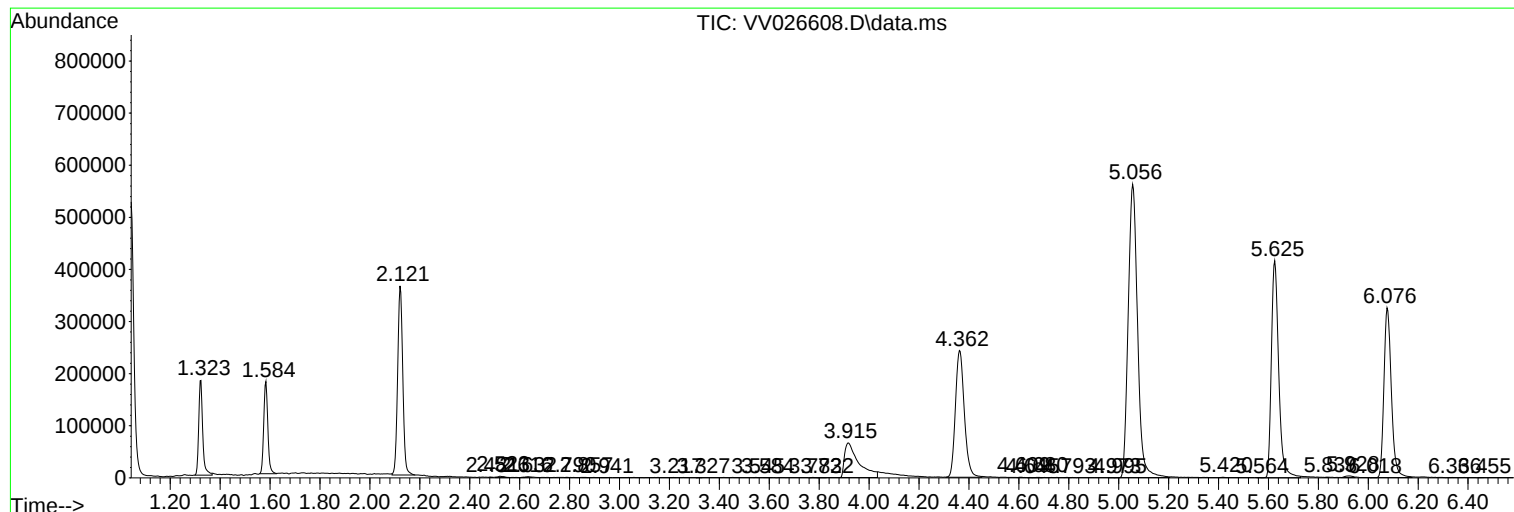

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026608.D
Acq On : 30 Jun 2022 15:32
Operator : SY/MD
Sample : N3521-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026608.D
Acq On : 30 Jun 2022 15:32
Operator : SY/MD
Sample : N3521-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc