

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026610.D
 Acq On : 30 Jun 2022 16:21
 Operator : SY/MD
 Sample : N3534-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	109	rBV	174208	190337	13.54%	1.850%
2	1.584	162	169	187	rVB	171440	196450	13.98%	1.909%
3	2.121	327	336	356	rVB	349027	502148	35.73%	4.880%
4	2.764	533	536	538	rVV3	384	258	0.02%	0.003%
5	2.908	578	581	585	rBV3	275	222	0.02%	0.002%
6	2.944	590	592	595	rBV2	231	105	0.01%	0.001%
7	2.998	606	609	612	rBV2	309	221	0.02%	0.002%
8	3.056	624	627	631	rBV2	586	410	0.03%	0.004%
9	3.133	647	651	653	rBV2	241	209	0.01%	0.002%
10	3.156	654	658	662	rVV2	268	287	0.02%	0.003%
11	3.249	683	687	689	rBV2	189	131	0.01%	0.001%
12	3.281	695	697	702	rVB2	312	182	0.01%	0.002%
13	3.323	707	710	712	rBV	193	123	0.01%	0.001%
14	3.426	739	742	745	rBV2	136	108	0.01%	0.001%
15	3.465	751	754	755	rBV	274	164	0.01%	0.002%
16	3.510	764	768	769	rBV	236	165	0.01%	0.002%
17	3.555	780	782	783	rBV	244	116	0.01%	0.001%
18	3.587	788	792	796	rBV	171	132	0.01%	0.001%
19	3.645	807	810	813	rBV2	145	105	0.01%	0.001%
20	3.715	828	832	836	rBV2	275	314	0.02%	0.003%
21	3.825	861	866	867	rBV2	143	109	0.01%	0.001%
22	3.915	884	894	934	rBV	61992	241005	17.15%	2.342%
23	4.362	1017	1033	1063	rBV	244334	600358	42.72%	5.834%
24	4.635	1115	1118	1121	rBV	213	128	0.01%	0.001%
25	4.722	1143	1145	1147	rBV	198	108	0.01%	0.001%
26	4.754	1152	1155	1158	rVB2	235	205	0.01%	0.002%
27	4.770	1158	1160	1162	rBV	237	149	0.01%	0.001%
28	4.831	1173	1179	1181	rBV3	220	239	0.02%	0.002%
29	4.902	1199	1201	1203	rBV2	226	109	0.01%	0.001%
30	4.989	1224	1228	1231	rBV2	231	189	0.01%	0.002%
31	5.056	1232	1249	1294	rBV2	547493	1405249	100.00%	13.656%
32	5.403	1352	1357	1359	rBV	404	382	0.03%	0.004%
33	5.436	1360	1367	1371	rVB4	704	787	0.06%	0.008%
34	5.458	1371	1374	1375	rBV	224	112	0.01%	0.001%
35	5.503	1386	1388	1391	rVB	212	107	0.01%	0.001%
36	5.625	1407	1426	1457	rBV	409439	838282	59.65%	8.146%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026610.D
 Acq On : 30 Jun 2022 16:21
 Operator : SY/MD
 Sample : N3534-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	5.915	1508	1516	1531	rBV9	3215	7119	0.51%	0.069%
38	6.075	1551	1566	1602	rBV	313812	648165	46.12%	6.299%
39	6.268	1624	1626	1630	rVB3	288	219	0.02%	0.002%
40	6.339	1645	1648	1651	rVB	280	177	0.01%	0.002%
41	6.407	1666	1669	1670	rBV	398	188	0.01%	0.002%
42	6.529	1702	1707	1709	rVB3	266	172	0.01%	0.002%
43	6.542	1709	1711	1715	rVB2	308	154	0.01%	0.001%
44	6.561	1715	1717	1723	rVB2	263	163	0.01%	0.002%
45	6.596	1723	1728	1730	rBV	274	228	0.02%	0.002%
46	6.641	1735	1742	1746	rBV4	1170	1470	0.10%	0.014%
47	6.992	1838	1851	1876	rBV	135495	254634	18.12%	2.474%
48	7.178	1907	1909	1910	rBV2	393	165	0.01%	0.002%
49	7.262	1933	1935	1940	rBV	236	182	0.01%	0.002%
50	7.320	1940	1953	1972	rBV	580695	1020093	72.59%	9.913%
51	7.625	2038	2048	2069	rBV	91011	162291	11.55%	1.577%
52	7.892	2128	2131	2134	rBV	230	154	0.01%	0.001%
53	8.014	2166	2169	2171	rBV3	259	168	0.01%	0.002%
54	8.027	2171	2173	2178	rVB3	316	163	0.01%	0.002%
55	8.050	2178	2180	2182	rBV	378	175	0.01%	0.002%
56	8.095	2183	2194	2226	rBV2	277497	598361	42.58%	5.815%
57	8.342	2268	2271	2276	rBV4	530	380	0.03%	0.004%
58	8.426	2294	2297	2300	rBV3	336	253	0.02%	0.002%
59	8.471	2308	2311	2312	rBV2	353	206	0.01%	0.002%
60	8.554	2335	2337	2340	rBV	329	167	0.01%	0.002%
61	8.570	2340	2342	2343	rBV	235	99	0.01%	0.001%
62	8.609	2350	2354	2355	rBV	432	314	0.02%	0.003%
63	8.786	2407	2409	2414	rBV2	243	161	0.01%	0.002%
64	8.853	2414	2430	2460	rBV	642751	1039539	73.98%	10.102%
65	9.191	2533	2535	2537	rBV	276	150	0.01%	0.001%
66	9.271	2558	2560	2562	rVB	279	107	0.01%	0.001%
67	9.329	2576	2578	2581	rVB	254	119	0.01%	0.001%
68	9.381	2592	2594	2598	rVB	301	164	0.01%	0.002%
69	9.458	2614	2618	2619	rBV	179	120	0.01%	0.001%
70	9.497	2627	2630	2633	rVB2	212	153	0.01%	0.001%
71	9.561	2647	2650	2655	rVB2	348	346	0.02%	0.003%
72	9.619	2663	2668	2671	rBV3	391	319	0.02%	0.003%
73	9.648	2674	2677	2682	rVB	398	318	0.02%	0.003%
74	9.673	2682	2685	2687	rBV	187	146	0.01%	0.001%
75	9.802	2723	2725	2729	rBV2	187	121	0.01%	0.001%
76	9.902	2754	2756	2763	rVB2	376	286	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026610.D
 Acq On : 30 Jun 2022 16:21
 Operator : SY/MD
 Sample : N3534-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	9.937	2763	2767	2769	rBV2	280	182	0.01%	0.002%
78	10.098	2814	2817	2819	rBV2	264	168	0.01%	0.002%
79	10.127	2821	2826	2832	rVB3	1089	1321	0.09%	0.013%
80	10.217	2838	2854	2872	rBV	470486	732859	52.15%	7.122%
81	10.384	2898	2906	2912	rVB6	1706	2257	0.16%	0.022%
82	10.416	2912	2916	2919	rBV	321	284	0.02%	0.003%
83	10.638	2982	2985	2989	rVB2	439	348	0.02%	0.003%
84	10.750	3017	3020	3022	rBV	166	107	0.01%	0.001%
85	10.873	3055	3058	3061	rBV2	230	200	0.01%	0.002%
86	10.921	3065	3073	3082	rVV6	1119	1951	0.14%	0.019%
87	11.194	3156	3158	3161	rVB	569	218	0.02%	0.002%
88	11.249	3164	3175	3198	rBV	585426	902312	64.21%	8.768%
89	11.467	3240	3243	3246	rBV2	299	252	0.02%	0.002%
90	11.622	3279	3291	3319	rBV	578821	925405	65.85%	8.993%
91	11.908	3377	3380	3383	rBV	398	236	0.02%	0.002%
92	11.966	3392	3398	3401	rBV3	443	444	0.03%	0.004%
93	12.339	3512	3514	3517	rBV2	282	198	0.01%	0.002%
94	12.377	3523	3526	3529	rBV	260	143	0.01%	0.001%
95	12.490	3558	3561	3562	rBV	238	166	0.01%	0.002%
96	12.818	3660	3663	3666	rBV2	355	253	0.02%	0.002%
97	12.863	3674	3677	3681	rBV3	537	393	0.03%	0.004%
98	13.268	3797	3803	3809	rVB6	1329	1635	0.12%	0.016%
99	13.522	3874	3882	3883	rBV2	586	706	0.05%	0.007%
100	13.754	3948	3954	3962	rBV5	677	1065	0.08%	0.010%



Sum of corrected areas: 10290717

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026610.D
Acq On : 30 Jun 2022 16:21
Operator : SY/MD
Sample : N3534-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

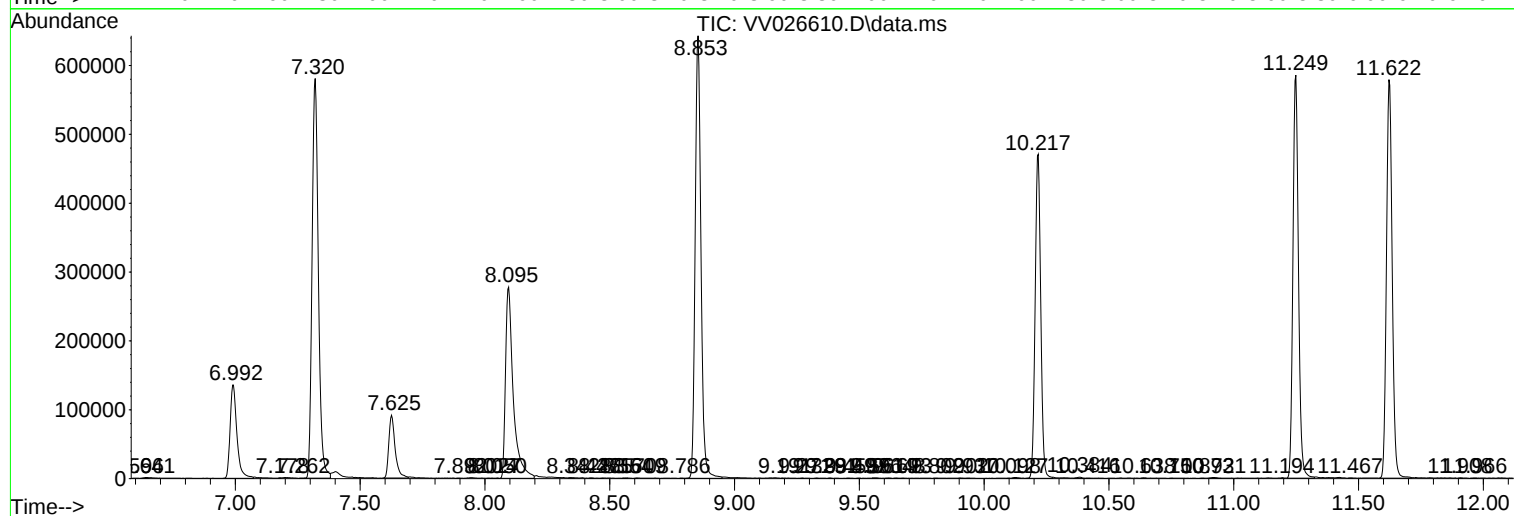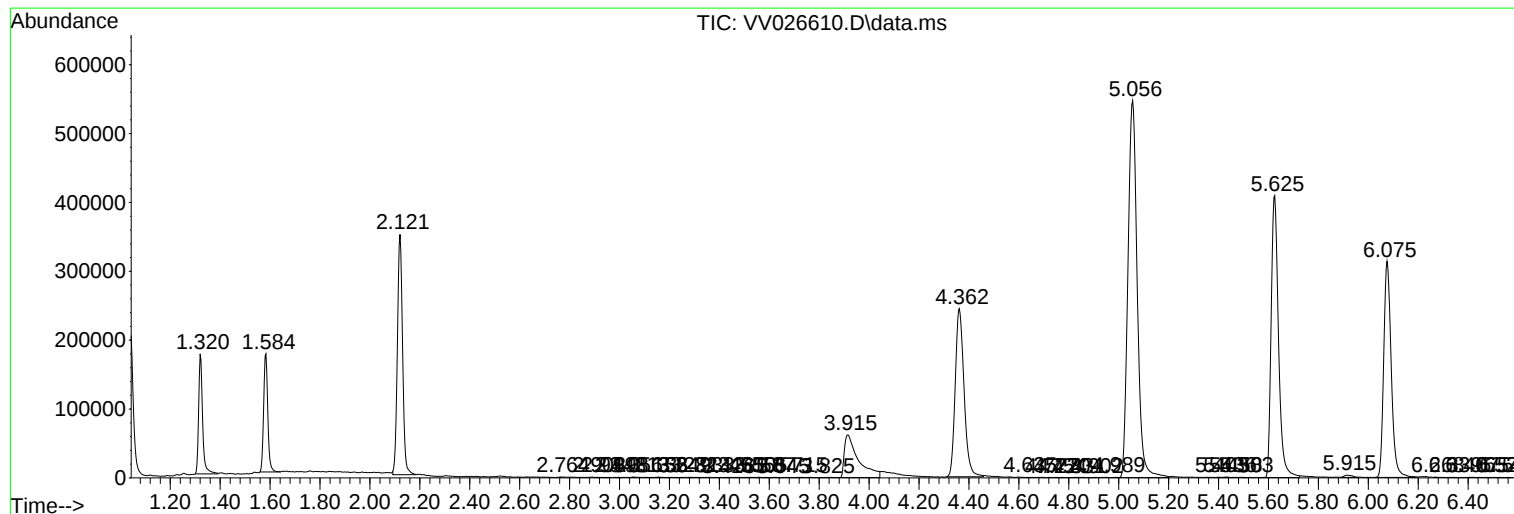

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026610.D
Acq On : 30 Jun 2022 16:21
Operator : SY/MD
Sample : N3534-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026610.D
Acq On : 30 Jun 2022 16:21
Operator : SY/MD
Sample : N3534-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------