

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026612.D
 Acq On : 30 Jun 2022 17:11
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M

Title : VOC Analysis

Signal : TIC: VV026612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	104	rBV	178722	192323	13.35%	1.814%
2	1.584	162	169	183	rVB	172221	196672	13.65%	1.855%
3	2.121	327	336	358	rVB	353986	515477	35.79%	4.862%
4	2.519	455	460	469	rBV4	2072	3139	0.22%	0.030%
5	2.593	481	483	485	rBV2	287	156	0.01%	0.001%
6	2.667	503	506	510	rBV2	378	348	0.02%	0.003%
7	2.751	530	532	534	rBV3	236	131	0.01%	0.001%
8	2.854	561	564	566	rBV3	256	154	0.01%	0.001%
9	2.879	570	572	574	rBV	269	142	0.01%	0.001%
10	3.040	619	622	627	rBV2	375	264	0.02%	0.002%
11	3.076	630	633	635	rBV	185	112	0.01%	0.001%
12	3.172	659	663	664	rBV	308	164	0.01%	0.002%
13	3.198	670	671	674	rVB	194	93	0.01%	0.001%
14	3.223	674	679	680	rBV	367	288	0.02%	0.003%
15	3.291	696	700	704	rBV2	261	165	0.01%	0.002%
16	3.384	727	729	732	rVB	191	98	0.01%	0.001%
17	3.477	756	758	761	rVB2	276	153	0.01%	0.001%
18	3.523	768	772	775	rVV2	191	157	0.01%	0.001%
19	3.542	776	778	780	rBV2	162	103	0.01%	0.001%
20	3.568	782	786	791	rVB2	380	274	0.02%	0.003%
21	3.590	791	793	796	rBV2	231	146	0.01%	0.001%
22	3.664	812	816	820	rVB	317	223	0.02%	0.002%
23	3.699	825	827	829	rBV2	154	100	0.01%	0.001%
24	3.738	837	839	843	rVB2	277	148	0.01%	0.001%
25	3.822	863	865	867	rVB	244	87	0.01%	0.001%
26	3.860	873	877	880	rBV2	264	197	0.01%	0.002%
27	3.915	884	894	932	rBV	66158	270161	18.76%	2.548%
28	4.362	1018	1033	1059	rBV	246033	601729	41.78%	5.676%
29	4.632	1114	1117	1119	rBV2	232	160	0.01%	0.002%
30	4.670	1126	1129	1130	rBV2	386	183	0.01%	0.002%
31	4.725	1141	1146	1147	rBV3	316	216	0.01%	0.002%
32	4.828	1176	1178	1180	rVB2	302	161	0.01%	0.002%
33	4.866	1186	1190	1196	rBV3	306	314	0.02%	0.003%
34	4.924	1200	1208	1211	rBV2	328	486	0.03%	0.005%
35	5.056	1229	1249	1287	rBV3	566699	1440352	100.00%	13.586%
36	5.538	1397	1399	1402	rBV2	175	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026612.D
 Acq On : 30 Jun 2022 17:11
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	5.574	1407	1410	1412	rBV2	350	177	0.01%	0.002%
38	5.625	1413	1426	1456	rBV	396991	807189	56.04%	7.614%
39	5.863	1497	1500	1504	rBV2	351	323	0.02%	0.003%
40	5.921	1508	1518	1523	rBV5	3708	6867	0.48%	0.065%
41	6.005	1540	1544	1545	rBV	361	287	0.02%	0.003%
42	6.075	1552	1566	1594	rBV	324558	664679	46.15%	6.270%
43	6.329	1643	1645	1653	rVB2	287	232	0.02%	0.002%
44	6.387	1660	1663	1664	rBV	201	100	0.01%	0.001%
45	6.426	1671	1675	1677	rVB2	178	142	0.01%	0.001%
46	6.445	1677	1681	1683	rBV	325	172	0.01%	0.002%
47	6.555	1709	1715	1716	rBV2	431	376	0.03%	0.004%
48	6.638	1737	1741	1743	rBV2	808	711	0.05%	0.007%
49	6.751	1769	1776	1780	rVB2	422	485	0.03%	0.005%
50	6.786	1784	1787	1789	rVV2	373	218	0.02%	0.002%
51	6.809	1792	1794	1798	rVB2	353	220	0.02%	0.002%
52	6.841	1798	1804	1808	rBV2	182	195	0.01%	0.002%
53	6.860	1808	1810	1811	rBV	192	84	0.01%	0.001%
54	6.992	1839	1851	1883	rBV	139187	261358	18.15%	2.465%
55	7.320	1941	1953	1972	rBV	617796	1056617	73.36%	9.967%
56	7.554	2023	2026	2029	rBV4	415	293	0.02%	0.003%
57	7.625	2038	2048	2071	rBV	94991	169830	11.79%	1.602%
58	7.860	2116	2121	2122	rBV2	192	153	0.01%	0.001%
59	7.882	2126	2128	2131	rVV3	253	134	0.01%	0.001%
60	7.931	2141	2143	2144	rBV	307	104	0.01%	0.001%
61	7.995	2159	2163	2166	rVB2	440	252	0.02%	0.002%
62	8.014	2166	2169	2177	rBV2	315	380	0.03%	0.004%
63	8.050	2177	2180	2183	rBV	287	212	0.01%	0.002%
64	8.095	2183	2194	2223	rBV2	317344	651034	45.20%	6.141%
65	8.445	2300	2303	2309	rVB2	562	528	0.04%	0.005%
66	8.477	2309	2313	2314	rBV2	329	190	0.01%	0.002%
67	8.612	2351	2355	2356	rBV	242	154	0.01%	0.001%
68	8.812	2415	2417	2418	rBV2	203	83	0.01%	0.001%
69	8.853	2418	2430	2459	rVV	628350	1015275	70.49%	9.577%
70	9.095	2504	2505	2507	rBV	234	93	0.01%	0.001%
71	9.143	2514	2520	2523	rBV4	720	790	0.05%	0.007%
72	9.217	2541	2543	2545	rVB2	206	85	0.01%	0.001%
73	9.236	2545	2549	2551	rBV2	249	167	0.01%	0.002%
74	9.275	2558	2561	2566	rVB	401	291	0.02%	0.003%
75	9.307	2566	2571	2573	rBV2	450	338	0.02%	0.003%
76	9.397	2590	2599	2600	rBV2	242	354	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026612.D
 Acq On : 30 Jun 2022 17:11
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	9.474	2619	2623	2625	rBV2	239	130	0.01%	0.001%
78	9.773	2710	2716	2718	rBV3	321	297	0.02%	0.003%
79	9.786	2718	2720	2726	rVV	427	286	0.02%	0.003%
80	9.931	2763	2765	2768	rVB3	247	109	0.01%	0.001%
81	9.998	2782	2786	2790	rBV2	217	181	0.01%	0.002%
82	10.095	2814	2816	2818	rBV	177	94	0.01%	0.001%
83	10.124	2820	2825	2827	rBV3	1163	1017	0.07%	0.010%
84	10.217	2841	2854	2879	rBV	488965	773739	53.72%	7.298%
85	10.448	2921	2926	2931	rBV3	329	455	0.03%	0.004%
86	10.519	2946	2948	2951	rBV2	274	133	0.01%	0.001%
87	10.760	3020	3023	3026	rVB	307	218	0.02%	0.002%
88	10.812	3037	3039	3042	rVB	293	136	0.01%	0.001%
89	10.902	3061	3067	3068	rBV2	451	346	0.02%	0.003%
90	11.011	3097	3101	3102	rBV2	342	205	0.01%	0.002%
91	11.140	3138	3141	3147	rVB3	568	532	0.04%	0.005%
92	11.191	3153	3157	3164	rVB4	1368	1734	0.12%	0.016%
93	11.249	3164	3175	3192	rBV	572118	887773	61.64%	8.374%
94	11.551	3263	3269	3270	rBV2	272	285	0.02%	0.003%
95	11.622	3279	3291	3318	rBV	616377	1018902	70.74%	9.611%
96	13.143	3762	3764	3767	rVB2	355	177	0.01%	0.002%
97	13.265	3793	3802	3814	rVB	17963	26548	1.84%	0.250%
98	13.744	3943	3951	3964	rVB3	10761	15776	1.10%	0.149%
99	13.885	3993	3995	3998	rBV	409	301	0.02%	0.003%
100	14.152	4074	4078	4082	rBV	9716	5629	0.39%	0.053%


Sum of corrected areas: 10601372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026612.D
Acq On : 30 Jun 2022 17:11
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

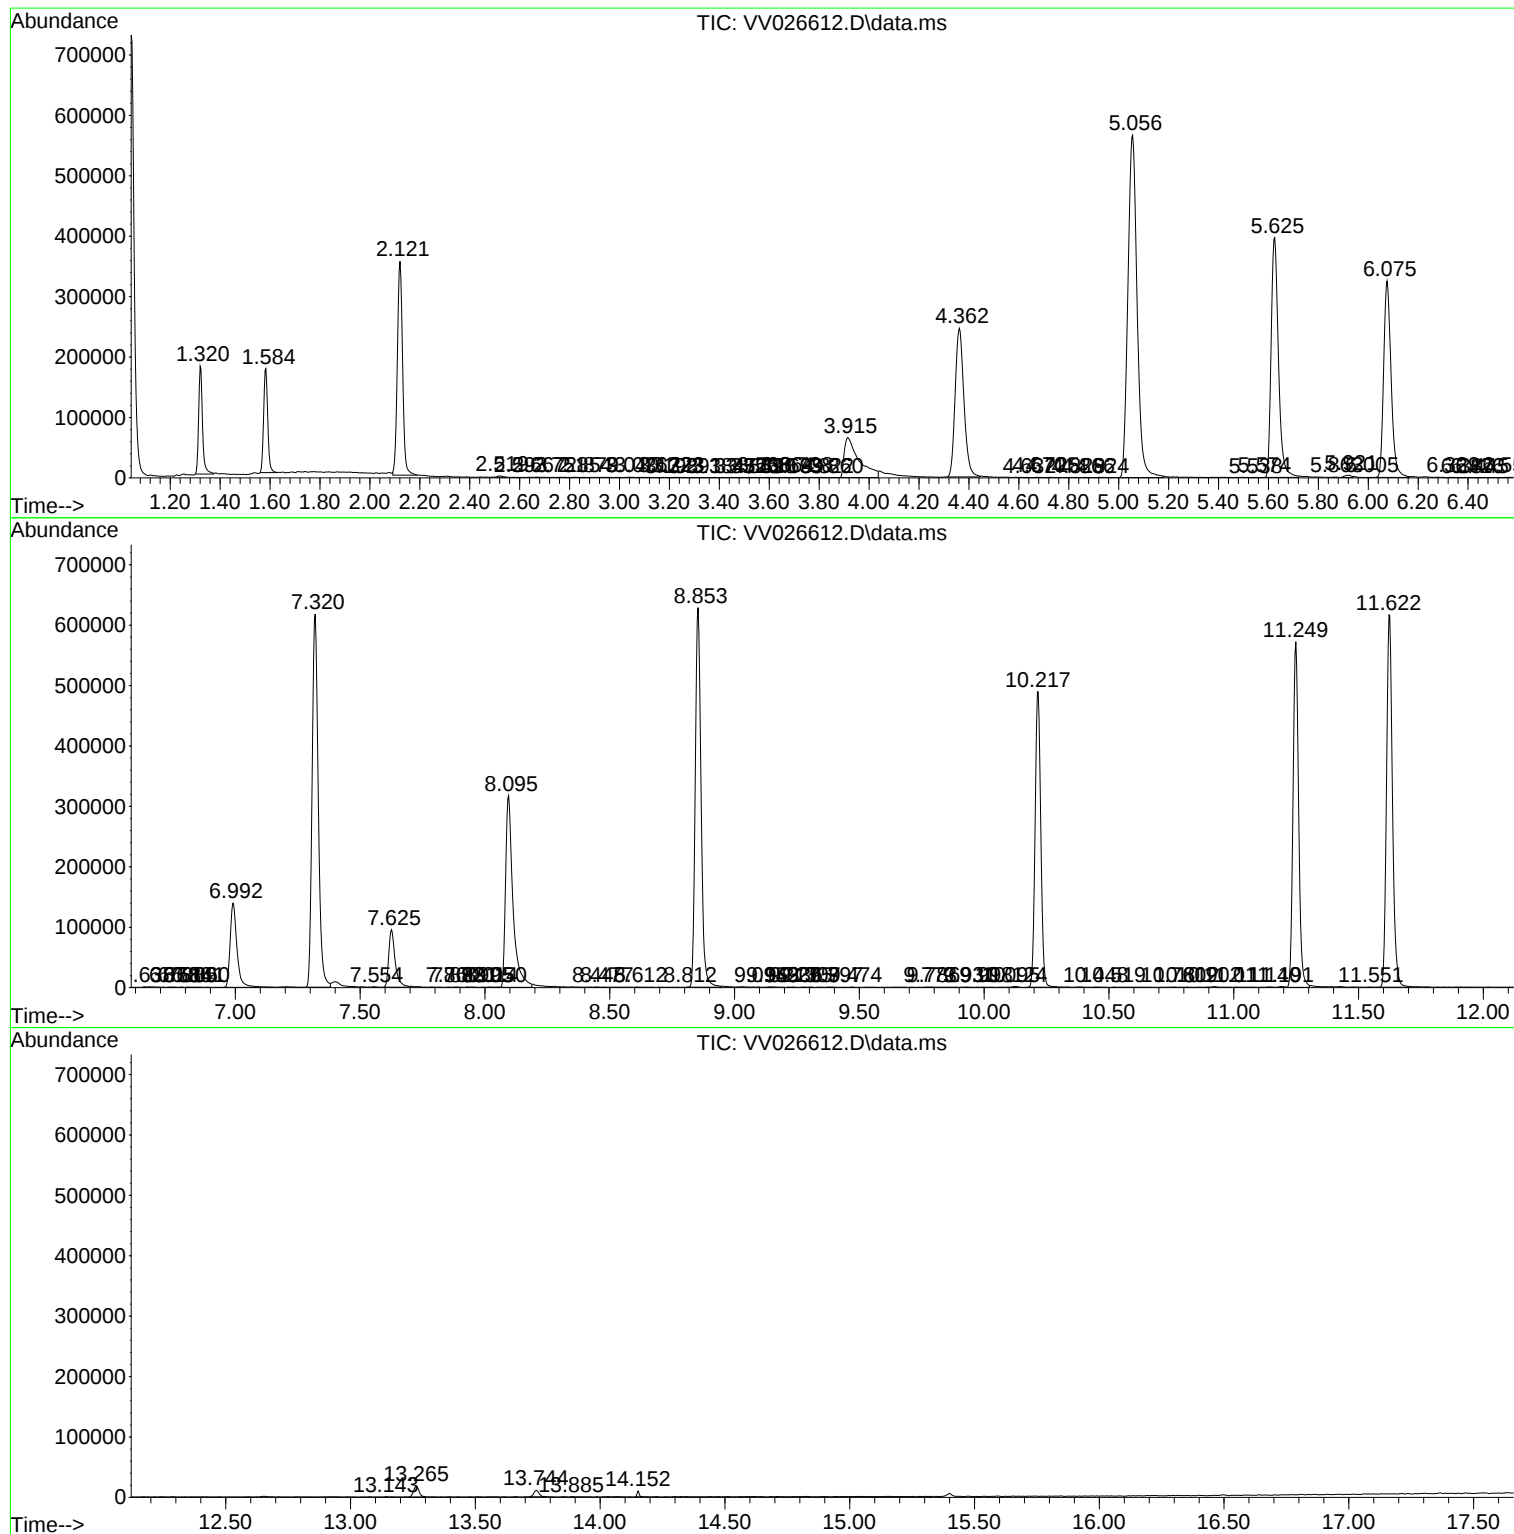

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026612.D
Acq On : 30 Jun 2022 17:11
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026612.D
Acq On : 30 Jun 2022 17:11
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc