

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026613.D
 Acq On : 30 Jun 2022 17:36
 Operator : SY/MD
 Sample : N3534-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

Signal : TIC: VV026613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	81	87	104	rBV	177235	190327	13.22%	1.827%
2	1.584	162	169	181	rBV	169161	192888	13.40%	1.852%
3	2.121	327	336	355	rVB	357621	514105	35.72%	4.935%
4	2.526	455	462	471	rVB6	2844	5173	0.36%	0.050%
5	2.722	519	523	527	rBV	304	304	0.02%	0.003%
6	2.912	578	582	584	rBV2	244	188	0.01%	0.002%
7	2.982	602	604	606	rBV2	206	116	0.01%	0.001%
8	3.140	651	653	654	rBV2	298	144	0.01%	0.001%
9	3.169	660	662	666	rVB2	254	166	0.01%	0.002%
10	3.195	666	670	674	rBV	347	273	0.02%	0.003%
11	3.362	719	722	724	rBV	161	103	0.01%	0.001%
12	3.629	802	805	807	rBV2	142	98	0.01%	0.001%
13	3.706	826	829	831	rBV2	146	93	0.01%	0.001%
14	3.732	835	837	841	rVB2	396	230	0.02%	0.002%
15	3.751	841	843	845	rBV	125	69	0.00%	0.001%
16	3.767	845	848	850	rBV	74	46	0.00%	0.000%
17	3.786	852	854	857	rVB2	167	46	0.00%	0.000%
18	3.825	861	866	868	rBV2	193	166	0.01%	0.002%
19	3.860	873	877	879	rBV2	311	249	0.02%	0.002%
20	3.915	884	894	917	rBV	66856	227130	15.78%	2.180%
21	4.362	1018	1033	1066	rBV	245706	599777	41.67%	5.758%
22	4.613	1109	1111	1118	rVB3	590	394	0.03%	0.004%
23	4.641	1118	1120	1122	rBV	144	88	0.01%	0.001%
24	4.786	1163	1165	1167	rBV	171	64	0.00%	0.001%
25	4.815	1171	1174	1176	rBV2	181	127	0.01%	0.001%
26	4.918	1204	1206	1209	rVB	94	43	0.00%	0.000%
27	4.934	1209	1211	1213	rBV2	188	129	0.01%	0.001%
28	4.995	1227	1230	1231	rBV	198	88	0.01%	0.001%
29	5.056	1231	1249	1285	rBV2	565937	1439396	100.00%	13.818%
30	5.336	1334	1336	1340	rVB3	430	325	0.02%	0.003%
31	5.445	1368	1370	1374	rVB2	336	177	0.01%	0.002%
32	5.487	1381	1383	1386	rVB	285	160	0.01%	0.002%
33	5.625	1413	1426	1449	rBV	390864	798520	55.48%	7.666%
34	5.821	1485	1487	1493	rVB4	928	591	0.04%	0.006%
35	5.915	1509	1516	1518	rBV3	3523	4036	0.28%	0.039%
36	6.075	1552	1566	1596	rBV	318802	667440	46.37%	6.408%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026613.D
 Acq On : 30 Jun 2022 17:36
 Operator : SY/MD
 Sample : N3534-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

37	6.284	1628	1631	1634	rBV	664	428	0.03%	0.004%
38	6.326	1643	1644	1647	rBV2	265	163	0.01%	0.002%
39	6.342	1647	1649	1651	rVB	478	195	0.01%	0.002%
40	6.365	1653	1656	1657	rBV	163	75	0.01%	0.001%
41	6.378	1658	1660	1662	rVV2	237	123	0.01%	0.001%
42	6.407	1666	1669	1671	rBV2	299	173	0.01%	0.002%
43	6.474	1688	1690	1693	rBV	71	52	0.00%	0.000%
44	6.503	1697	1699	1703	rBV2	84	46	0.00%	0.000%
45	6.522	1703	1705	1709	rVB2	211	106	0.01%	0.001%
46	6.548	1709	1713	1716	rBV3	416	343	0.02%	0.003%
47	6.616	1732	1734	1736	rBV	216	101	0.01%	0.001%
48	6.638	1736	1741	1742	rBV5	878	675	0.05%	0.006%
49	6.754	1774	1777	1779	rBV	318	211	0.01%	0.002%
50	6.802	1790	1792	1793	rBV	121	45	0.00%	0.000%
51	6.921	1826	1829	1833	rVB3	190	119	0.01%	0.001%
52	6.989	1839	1850	1875	rBV	135613	256739	17.84%	2.465%
53	7.320	1940	1953	1972	rBV	609090	1056055	73.37%	10.138%
54	7.625	2037	2048	2071	rBV	93216	167345	11.63%	1.607%
55	7.812	2103	2106	2108	rBV2	425	228	0.02%	0.002%
56	7.831	2108	2112	2118	rBV5	458	386	0.03%	0.004%
57	7.873	2124	2125	2128	rVB	272	124	0.01%	0.001%
58	8.046	2176	2179	2183	rVB2	367	262	0.02%	0.003%
59	8.095	2183	2194	2232	rBV2	307319	648210	45.03%	6.223%
60	8.416	2291	2294	2295	rBV2	525	232	0.02%	0.002%
61	8.792	2408	2411	2414	rVB	255	152	0.01%	0.001%
62	8.854	2418	2430	2456	rBV	625375	1010710	70.22%	9.703%
63	9.149	2518	2522	2524	rBV3	844	748	0.05%	0.007%
64	9.188	2531	2534	2536	rBV2	495	266	0.02%	0.003%
65	9.239	2545	2550	2553	rBV2	277	296	0.02%	0.003%
66	9.300	2567	2569	2571	rBV	380	152	0.01%	0.001%
67	9.345	2581	2583	2586	rVB2	407	185	0.01%	0.002%
68	9.371	2586	2591	2593	rVB2	274	234	0.02%	0.002%
69	9.500	2629	2631	2633	rVB	221	60	0.00%	0.001%
70	9.548	2641	2646	2647	rBV2	345	263	0.02%	0.003%
71	9.731	2700	2703	2706	rBV	242	134	0.01%	0.001%
72	9.931	2763	2765	2769	rBV2	264	142	0.01%	0.001%
73	10.069	2805	2808	2811	rBV2	350	237	0.02%	0.002%
74	10.162	2834	2837	2840	rBV2	246	142	0.01%	0.001%
75	10.217	2841	2854	2875	rBV	484872	762801	52.99%	7.323%
76	10.381	2902	2905	2908	rBV2	443	282	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
 Data File : VV026613.D
 Acq On : 30 Jun 2022 17:36
 Operator : SY/MD
 Sample : N3534-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Title : VOC Analysis

77	10.461	2927	2930	2932	rVB	289	179	0.01%	0.002%
78	10.477	2932	2935	2937	rBV	220	154	0.01%	0.001%
79	10.503	2941	2943	2945	rVB	348	156	0.01%	0.001%
80	10.548	2945	2957	2963	rBV2	550	944	0.07%	0.009%
81	10.603	2972	2974	2977	rBV	179	103	0.01%	0.001%
82	10.767	3022	3025	3028	rBV	303	254	0.02%	0.002%
83	10.812	3036	3039	3042	rBV	282	199	0.01%	0.002%
84	10.857	3049	3053	3054	rBV2	400	237	0.02%	0.002%
85	10.979	3089	3091	3092	rBV	228	50	0.00%	0.000%
86	11.146	3140	3143	3144	rBV2	441	280	0.02%	0.003%
87	11.194	3152	3158	3160	rBV	588	610	0.04%	0.006%
88	11.249	3164	3175	3195	rBV	568985	884890	61.48%	8.495%
89	11.461	3238	3241	3245	rBV2	282	223	0.02%	0.002%
90	11.519	3255	3259	3263	rBV2	521	462	0.03%	0.004%
91	11.622	3279	3291	3310	rBV	617264	968286	67.27%	9.296%
92	11.940	3384	3390	3394	rBV2	655	658	0.05%	0.006%
93	12.249	3483	3486	3491	rBV2	460	383	0.03%	0.004%
94	13.040	3729	3732	3734	rBV	378	245	0.02%	0.002%
95	13.178	3772	3775	3776	rBV	338	178	0.01%	0.002%
96	13.268	3797	3803	3814	rVB5	3661	5530	0.38%	0.053%




Sum of corrected areas: 10416530

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026613.D
Acq On : 30 Jun 2022 17:36
Operator : SY/MD
Sample : N3534-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

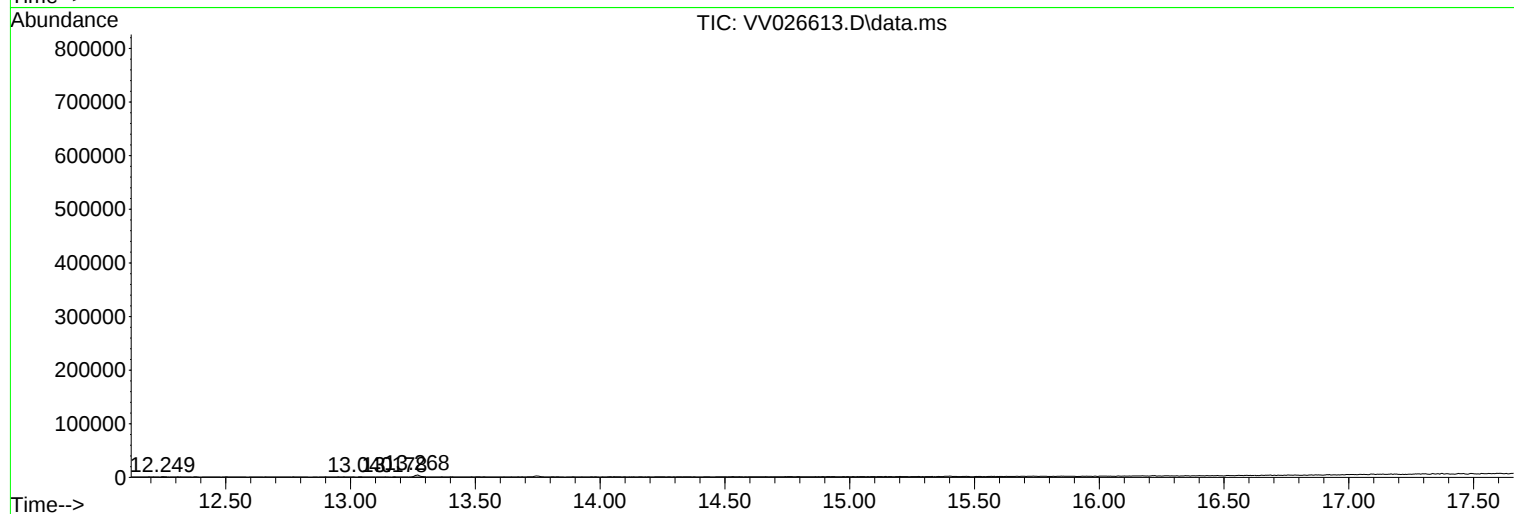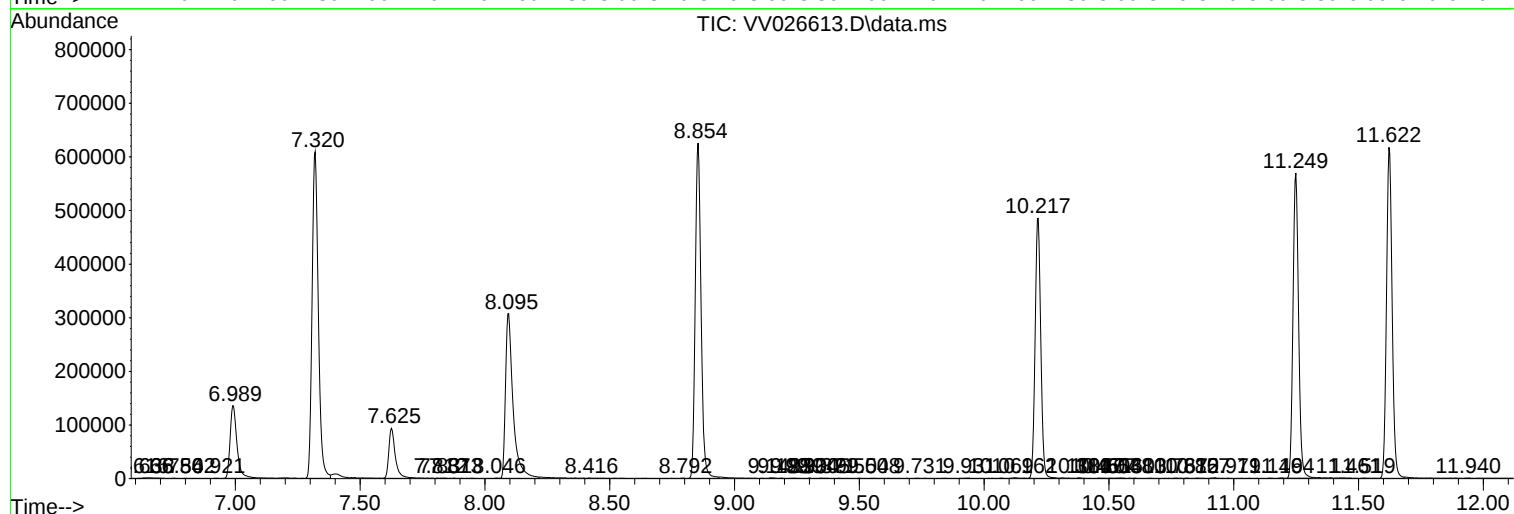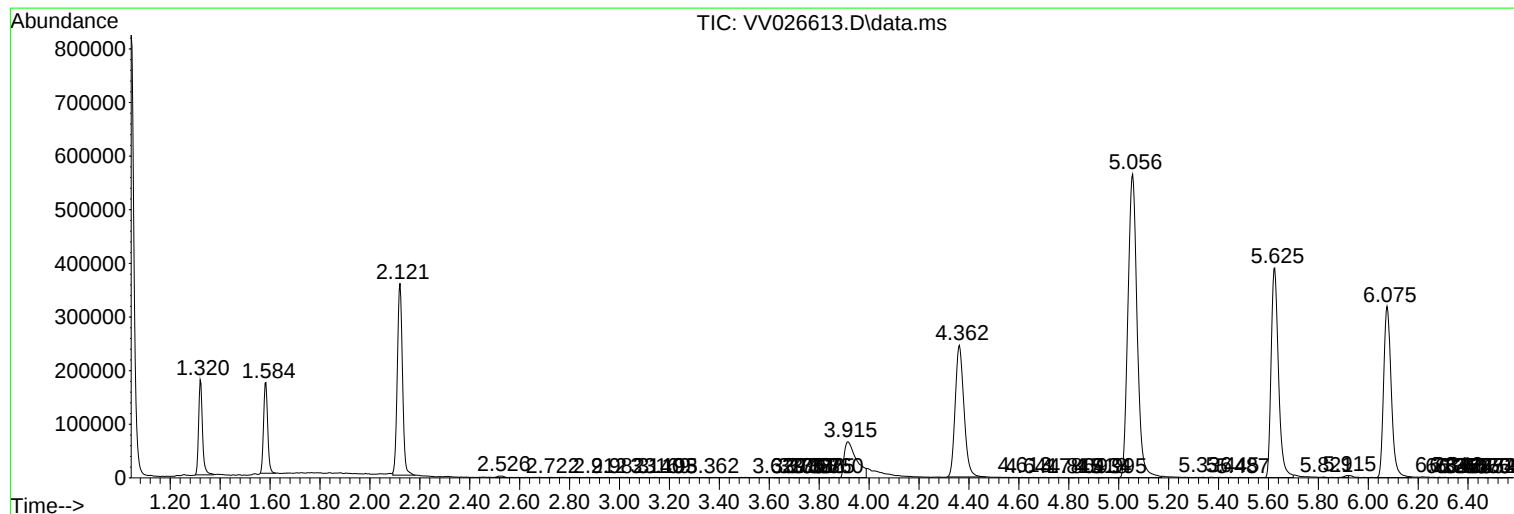

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026613.D
Acq On : 30 Jun 2022 17:36
Operator : SY/MD
Sample : N3534-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026613.D
Acq On : 30 Jun 2022 17:36
Operator : SY/MD
Sample : N3534-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc