

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
 Data File : VV017279.D
 Acq On : 01 Jul 2020 10:47
 Operator : SY/MD
 Sample : L3150-15MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETYJ9MS

Quant Time: Jul 02 03:05:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 02 03:02:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	183108	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	177510	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	80996	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46196	4.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.00%
7) Chloroethane-d5	1.58	69	41743	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	2.13	63	100357	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.00%
20) 2-Butanone-d5	3.93	46	134340	47.96	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.92%
24) Chloroform-d	4.38	84	114686	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.06	65	63815	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	5.08	84	202808	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
36) 1,2-Dichloropropane-d6	6.09	67	61971	4.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.80%
41) Toluene-d8	7.34	98	179552	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
45) trans-1,3-Dichloropropene-	7.64	79	23487	4.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.80%
48) 2-Hexanone-d5	8.11	63	94459	43.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.34%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	44302	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	73590	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Chloroethane	1.60	64	1111	0.167	ug/L #	52
10) 1,1,2-Trichloro-1,2,2-trif	2.13	101	815	0.084	ug/L #	32
12) 1,1-Dichloroethene	2.14	96	47731	5.431	ug/L	94
16) Methylene chloride	2.53	84	1268	0.135	ug/L	77
18) trans-1,2-Dichloroethene	2.78	96	1077	0.116	ug/L	93
22) cis-1,2-Dichloroethene	3.94	96	59833	4.698	ug/L	95
33) Benzene	5.13	78	234683	5.048	ug/L	100
34) Trichloroethene	5.94	95	348989	25.638	ug/L	96
35) Methylcyclohexane	6.09	83	16359	0.773	ug/L #	17
37) 1,2-Dichloropropane	6.10	63	8211	0.714	ug/L #	84
39) cis-1,3-Dichloropropene	7.01	75	2159	0.126	ug/L	85
42) Toluene	7.41	91	257562	4.766	ug/L	99
46) trans-1,3-Dichloropropene	7.64	75	1317	0.089	ug/L #	67
49) Tetrachloroethene	8.00	164	1908	0.174	ug/L	92
50) 2-Hexanone	8.16	43	3793	0.802	ug/L #	55
53) Chlorobenzene	8.90	112	163383	4.849	ug/L	98

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
Data File : VV017279.D
Acq On : 01 Jul 2020 10:47
Operator : SY/MD
Sample : L3150-15MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETYJ9MS

Quant Time: Jul 02 03:05:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 02 03:02:49 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
Data File : VV017279.D
Acq On : 01 Jul 2020 10:47
Operator : SY/MD
Sample : L3150-15MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETYJ9MS

Quant Time: Jul 02 03:05:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 02 03:02:49 2020
Response via : Initial Calibration

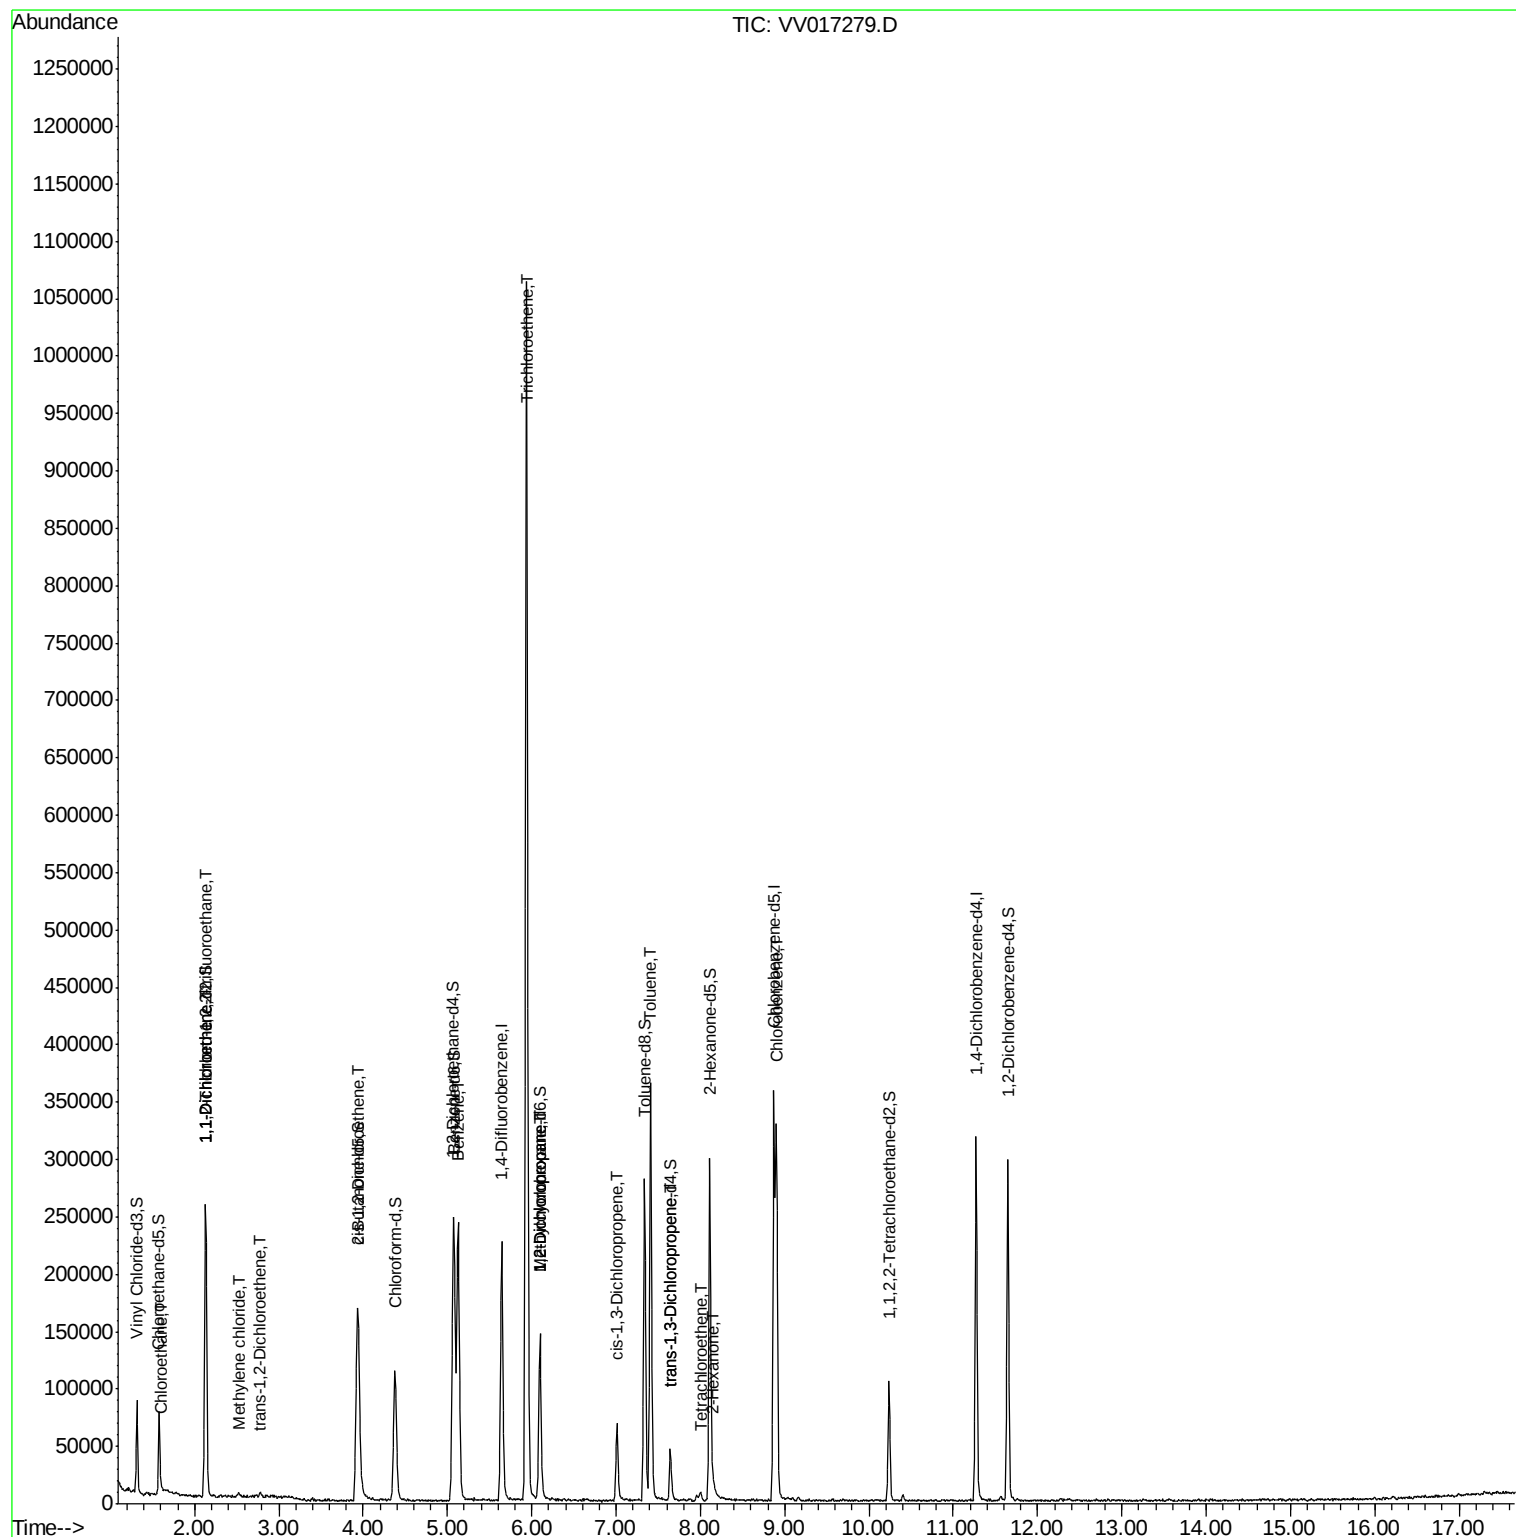



#8

Chloroethane

Concen: 0.167 ug/L

RT: 1.60 min Scan# 160

Delta R.T. 0.01 min

Lab File: VV017279.D

Acq: 01 Jul 2020 10:47

Instrument :

MSVOA_V

ClientSampleId :


ETYJ9MS

Tot Ion: 64 Resp: 1111

Ion Ratio Lower Upper




64 100

66 5.4 22.8 42.4#

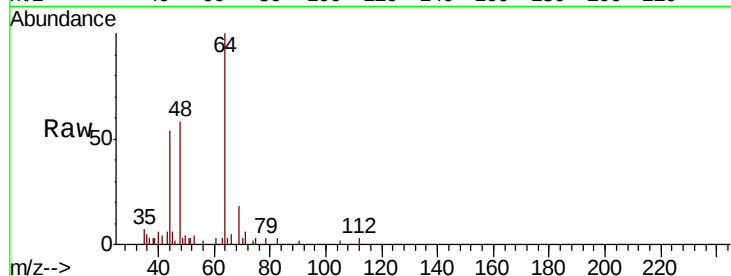

Abundance Ion 64.10 (63.80 to 64.80): VV017279.D (-64) (-)

Ion 66.05 (65.75 to 66.75): VV017279.D (-66) (-)

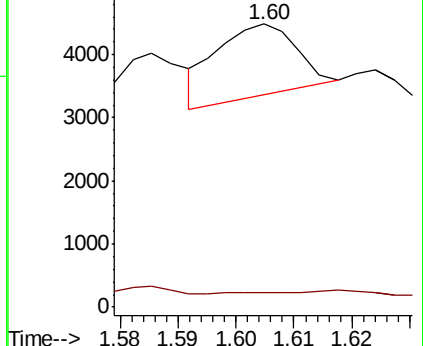

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.084 ug/L

RT: 2.13 min Scan# 323

Delta R.T. -0.00 min

Lab File: VV017279.D

Acq: 01 Jul 2020 10:47


Tgt Ion: 101 Resp: 815

Ion Ratio Lower Upper

101 100

85 13.7 35.4 53.2#



151 9.1 63.9 95.9#




Abundance Ion 101.00 (100.70 to 101.70): VV017279.D (-101) (-)

Ion 85.00 (84.70 to 85.70): VV017279.D (-85) (-)

Ion 151.00 (150.70 to 151.70): VV017279.D (-151) (-)



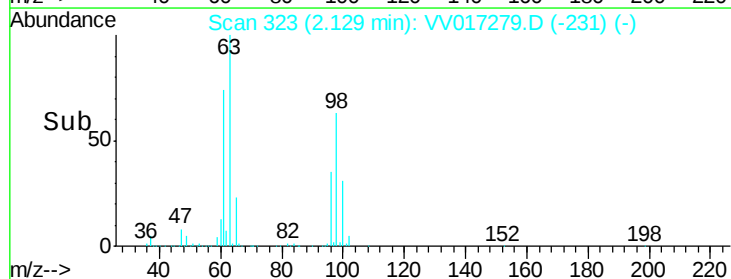
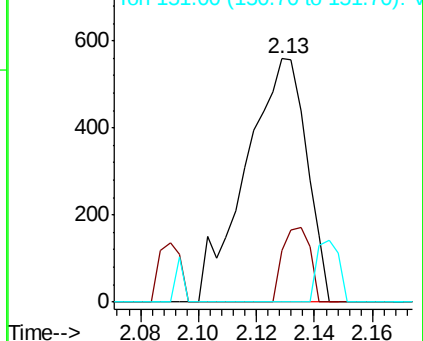




#12
1,1-Dichloroethene
Concen: 5.431 ug/L
RT: 2.14 min Scan# 325
Delta R.T. 0.00 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47




Instrument :
MSVOA_V
ClientSampleId :
ETYJ9MS


Tot Ion	96	Resp	47731
Ion	Ratio	Lower	Upper
96	100		
61	189.3	125.0	232.2
63	152.4	109.8	203.8

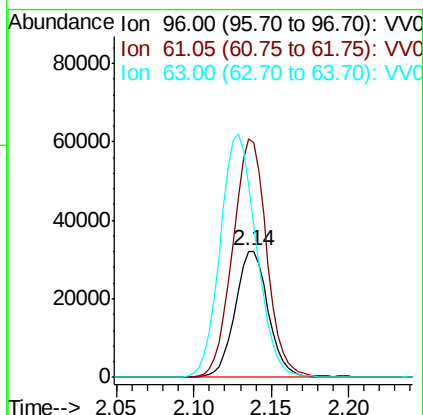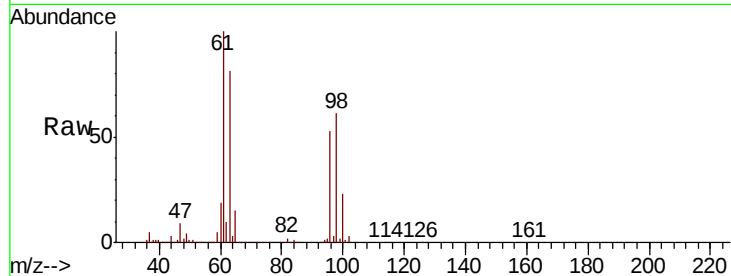

#16
Methylene chloride
Concen: 0.135 ug/L
RT: 2.53 min Scan# 447
Delta R.T. 0.01 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47

Tgt Ion	84	Resp	1268
Ion	Ratio	Lower	Upper
84	100		
86	70.9	45.8	85.0
49	163.7	89.6	166.4

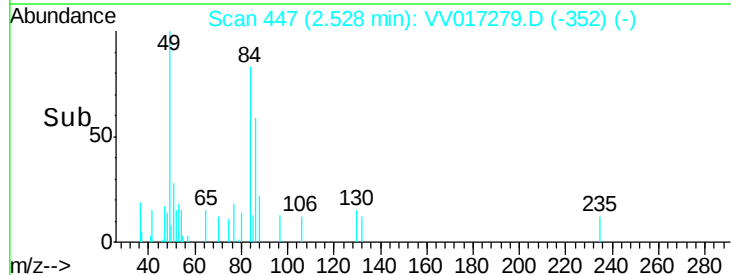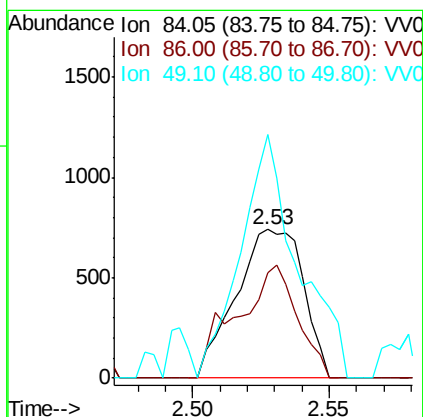


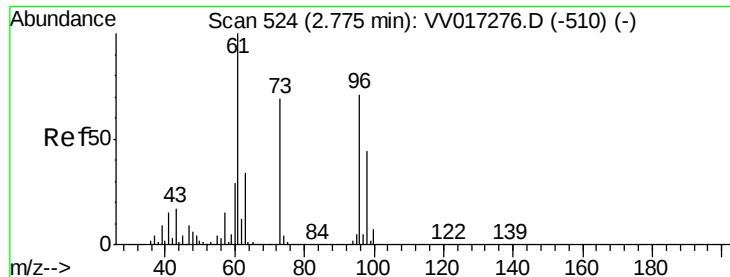




#18
trans-1,2-Dichloroethene
Concen: 0.116 ug/L
RT: 2.78 min Scan# 526
Delta R.T. 0.01 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47

Instrument :
MSVOA_V
ClientSampleId :
ETYJ9MS

Tot Ion: 96 Resp: 1077
Ion Ratio Lower Upper
96 100
61 156.7 102.3 189.9
98 62.0 44.7 82.9

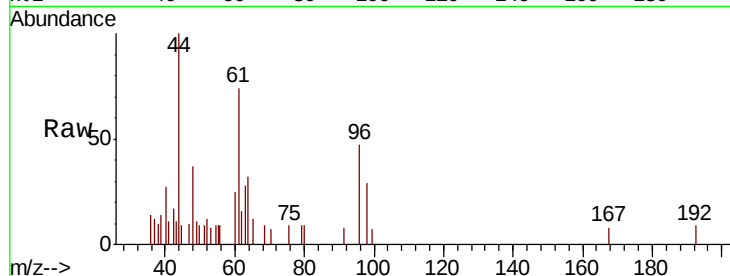


Abundance Ion 96.00 (95.70 to 96.70): VV0
Ion 61.05 (60.75 to 61.75): VV0
Ion 97.95 (97.65 to 98.65): VV0

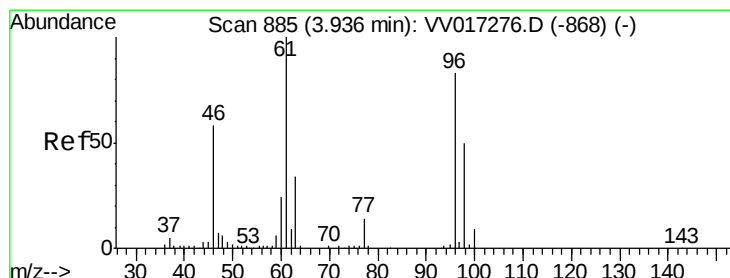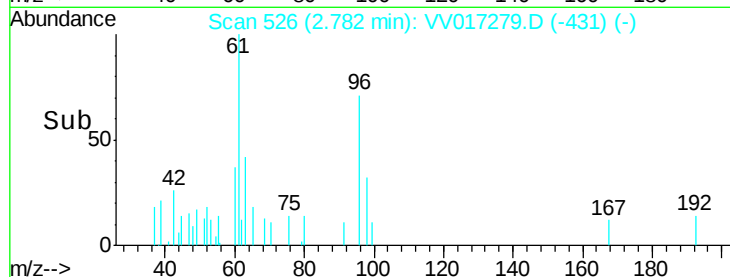
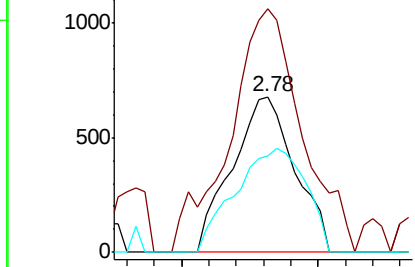



#22
cis-1,2-Dichloroethene
Concen: 4.698 ug/L
RT: 3.94 min Scan# 886
Delta R.T. 0.00 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47

Tgt Ion: 96 Resp: 59833
Ion Ratio Lower Upper
96 100
61 135.7 91.0 169.0
68 0.0 0.0 0.0

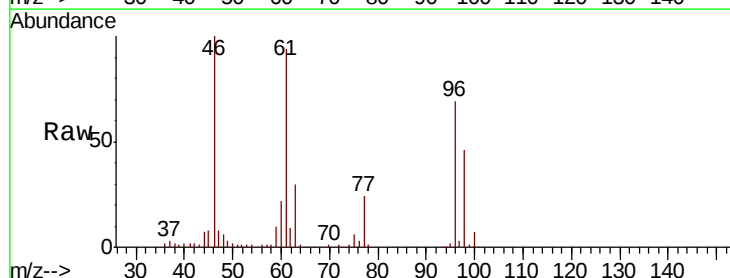

Abundance Ion 96.00 (95.70 to 96.70): VV0
Ion 61.05 (60.75 to 61.75): VV0
Ion 68.15 (67.85 to 68.85): VV0

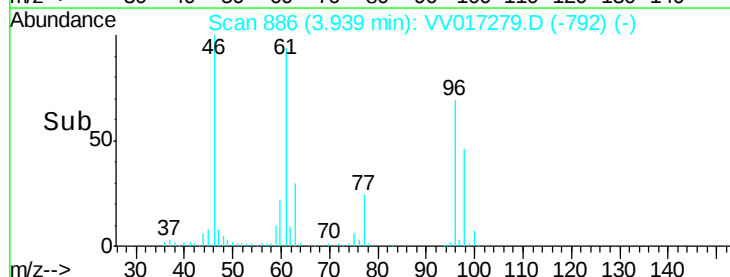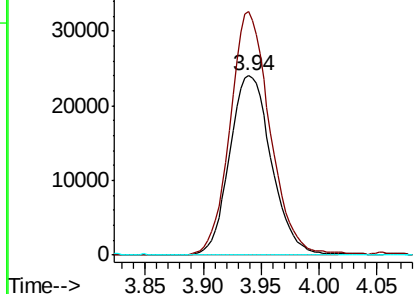



#33

Benzene

Concen: 5.048 ug/L

RT: 5.13 min Scan# 1255

Delta R.T. 0.01 min

Lab File: VV017279.D

Acq: 01 Jul 2020 10:47


Instrument :

MSVOA_V




ClientSampleId :

ETYJ9MS

Tgt Ion: 78 Resp: 234683

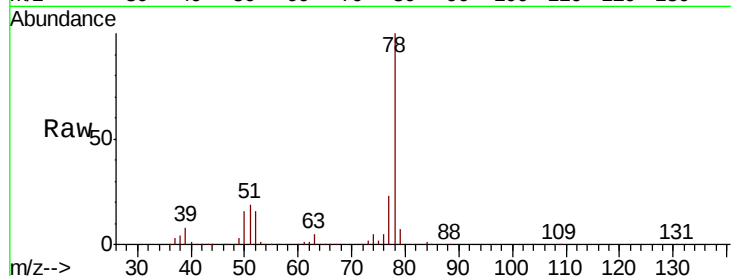

Abundance Ion 78.10 (77.80 to 78.80): VV0

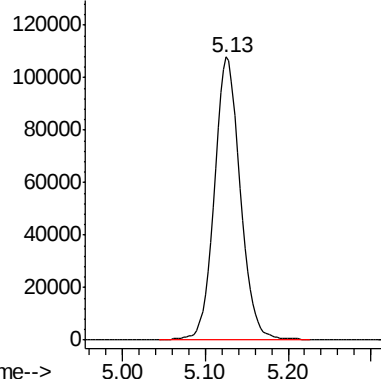

#34

Trichloroethene

Concen: 25.638 ug/L

RT: 5.94 min Scan# 1508

Delta R.T. 0.00 min

Lab File: VV017279.D

Acq: 01 Jul 2020 10:47

Tgt Ion: 95 Resp: 348989

Ion	Ratio	Lower	Upper
95	100		
97	66.0	45.3	84.1
132	101.9	68.8	127.8
130	105.8	70.2	130.4




Ion 95.00 (94.70 to 95.70): VV0


Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): VV0

Ion 129.95 (129.65 to 130.65): VV0

Abundance Ion 95.00 (94.70 to 95.70): VV0


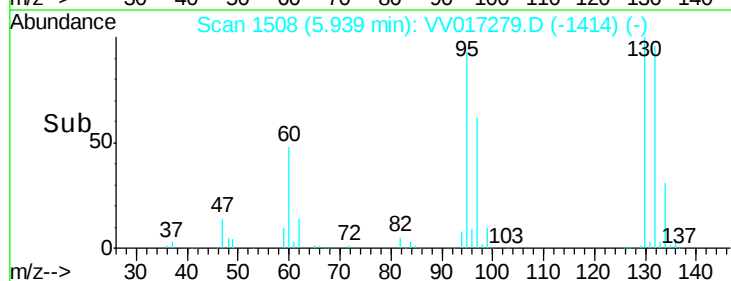

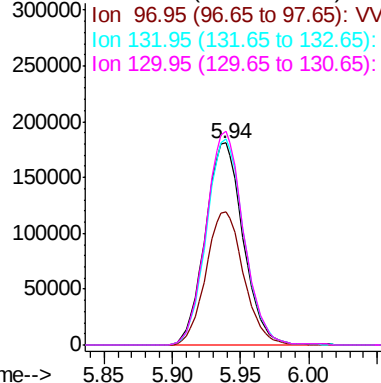


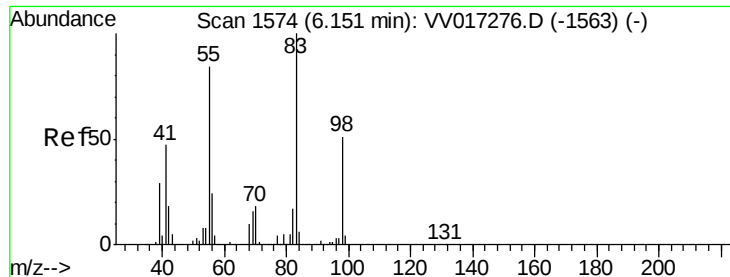

#35
Methvlcvclohexane
Concen: 0.773 ug/L
RT: 6.09 min Scan# 1556
Delta R.T. -0.06 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47




Instrument :
MSVOA_V
ClientSampleId :
ETYJ9MS


Tot Ion: 83 Resp: 16359
Ion Ratio Lower Upper
83 100
55 0.4 63.6 95.4#
98 0.0 38.8 58.2#

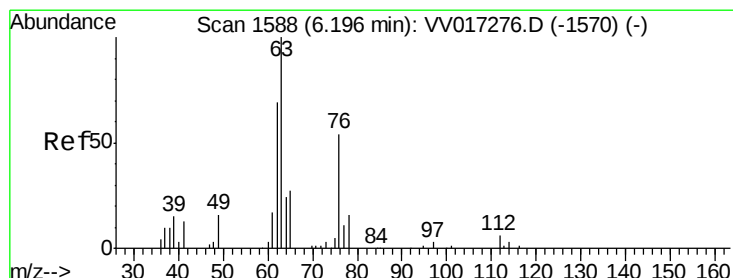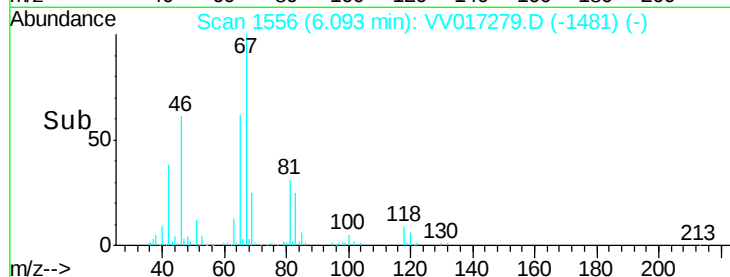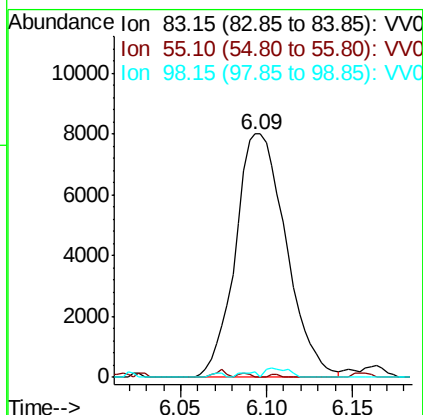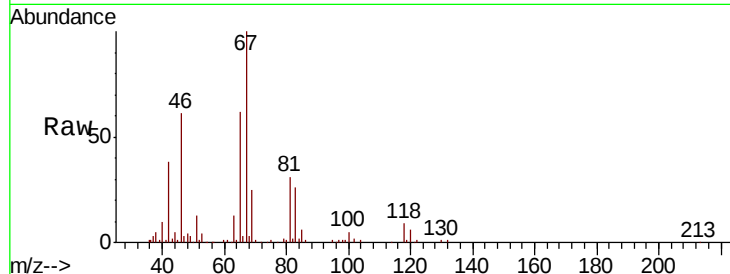

#37
1,2-Dichloropropane
Concen: 0.714 ug/L
RT: 6.10 min Scan# 1557
Delta R.T. -0.10 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47

Tgt Ion: 63 Resp: 8211
Ion Ratio Lower Upper
63 100
112 0.2 4.4 6.6#


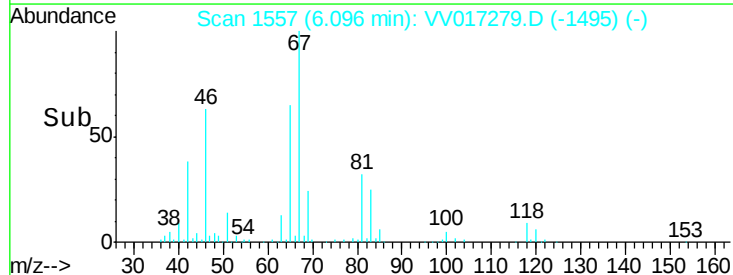
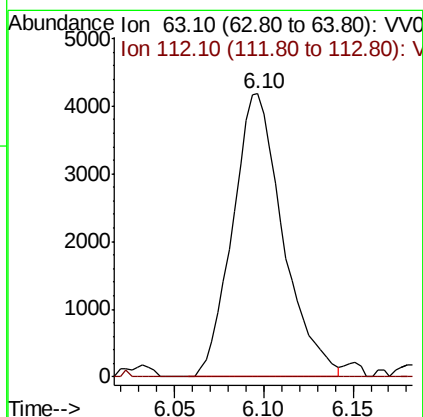
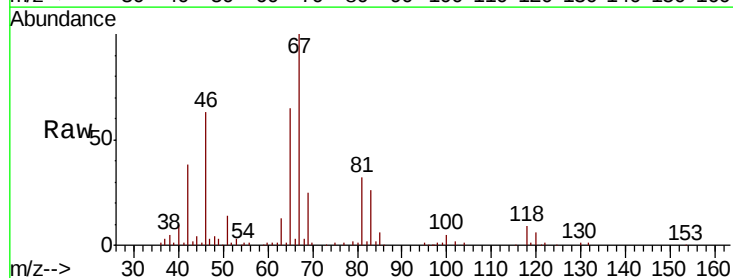




#39
 cis-1,3-Dichloropropene
 Concen: 0.126 ug/L
 RT: 7.01 min Scan# 1840
 Delta R.T. -0.04 min
 Lab File: VV017279.D
 Acq: 01 Jul 2020 10:47




Instrument :
 MSVOA_V
 ClientSampled :
 ETYJ9MS


Tot Ion: 75 Resp: 2159
 Ion Ratio Lower Upper
 75 100
 77 40.4 22.3 41.5

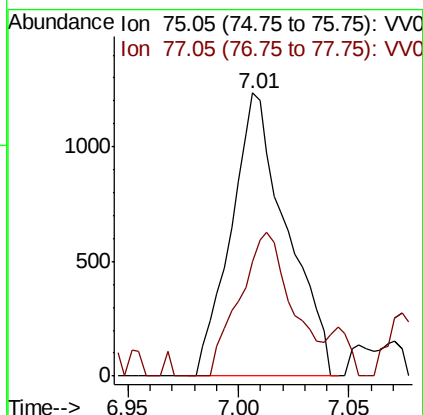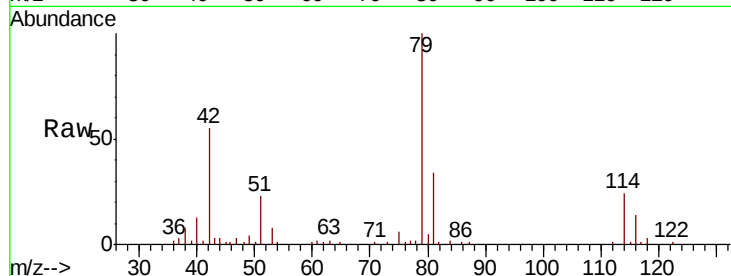

#42
 Toluene
 Concen: 4.766 ug/L
 RT: 7.41 min Scan# 1965
 Delta R.T. 0.00 min
 Lab File: VV017279.D
 Acq: 01 Jul 2020 10:47

Tgt Ion: 91 Resp: 257562
 Ion Ratio Lower Upper
 91 100
 92 56.5 39.9 74.1

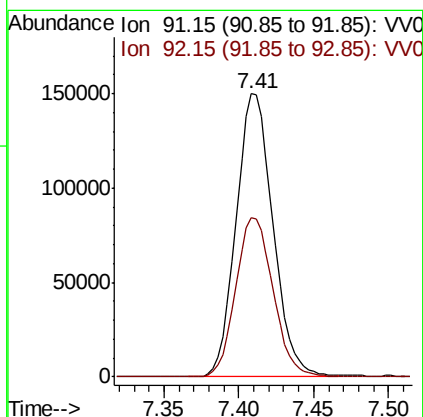

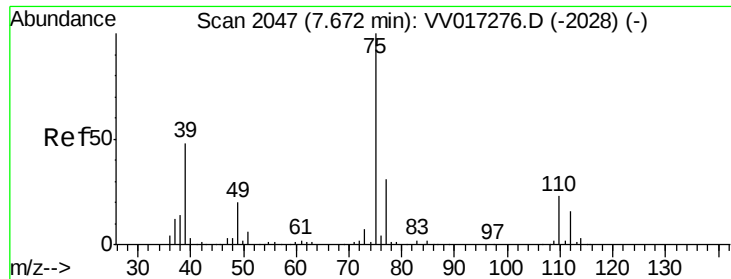

#46

trans-1,3-Dichloropropene

Concen: 0.089 ug/L

RT: 7.64 min Scan# 2038

Delta R.T. -0.03 min

Lab File: VV017279.D

Acq: 01 Jul 2020 10:47

Instrument :

MSVOA_V

ClientSampleId :


ETYJ9MS

Tot Ion: 75 Resp: 1317

Ion Ratio Lower Upper




75 100

77 49.9 22.3 41.3#

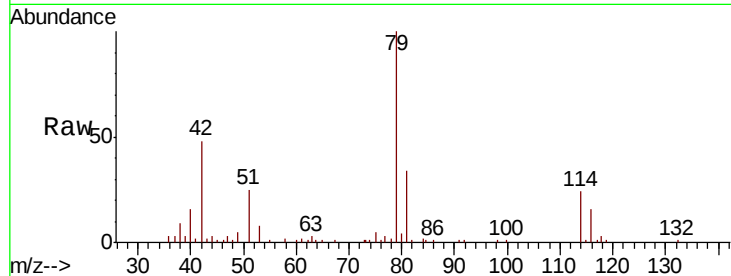

Abundance Ion 75.05 (74.75 to 75.75): VV0

Ion 77.05 (76.75 to 77.75): VV0

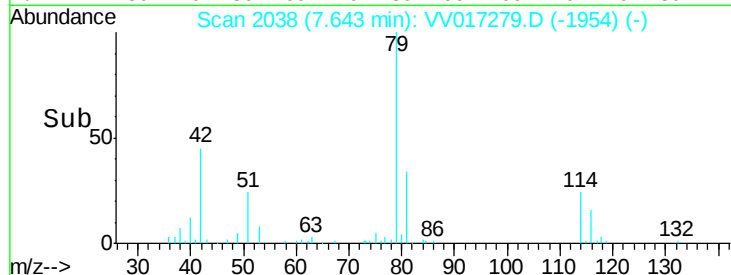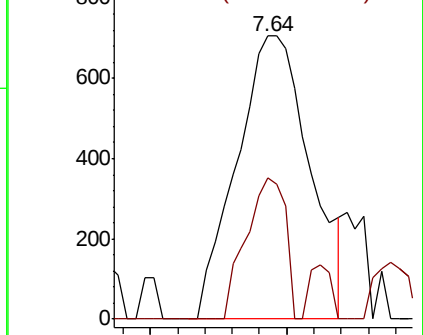

#49

Tetrachloroethene

Concen: 0.174 ug/L

RT: 8.00 min Scan# 2149

Delta R.T. 0.01 min

Lab File: VV017279.D

Acq: 01 Jul 2020 10:47

Tgt Ion:164 Resp: 1908


Ion Ratio Lower Upper

164 100

129 81.4 65.2 121.0

131 81.3 64.1 119.1

166 124.8 90.2 167.4


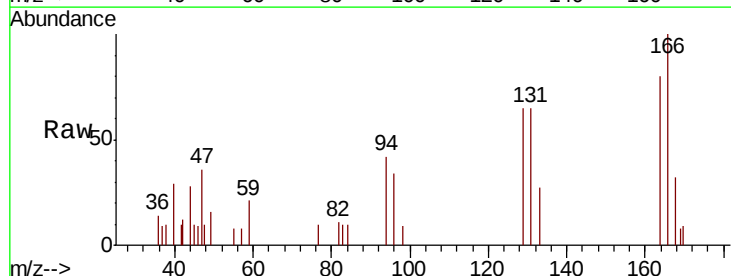



Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

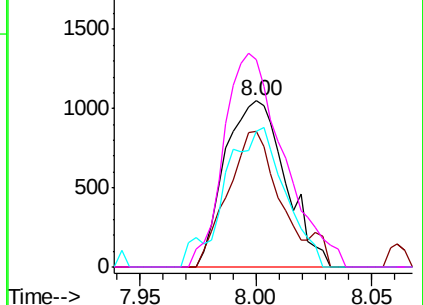


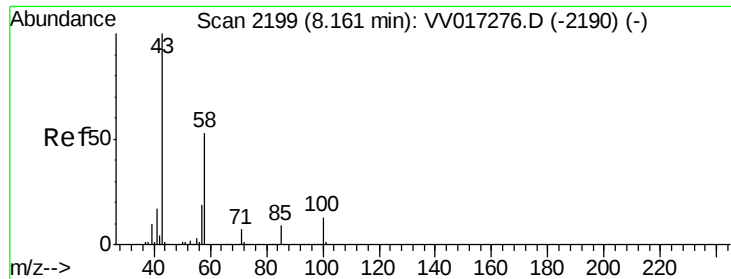

#50
2-Hexanone
Concen: 0.802 ug/L
RT: 8.16 min Scan# 2199
Delta R.T. -0.00 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47

Instrument :
MSVOA_V
ClientSampleId :
ETYJ9MS

Tot Ion	Ratio	Lower	Upper
43	100		
58	12.4	41.6	62.4#
57	0.0	15.4	23.0#
100	14.7	10.1	15.1



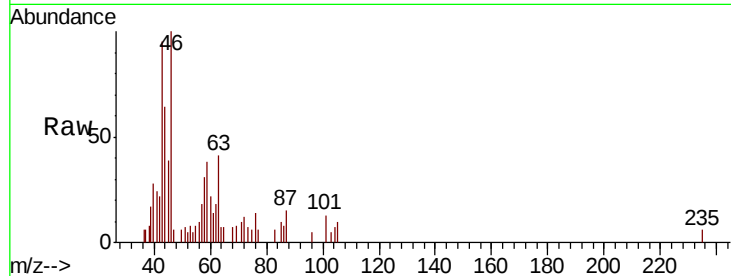


Abundance Ion 43.05 (42.75 to 43.75): VV017279.D (-2106) (-)

Ion 58.05 (57.75 to 58.75): VV017279.D (-2106) (-)


Ion 57.20 (56.90 to 57.90): VV017279.D (-2106) (-)

Ion 100.15 (99.85 to 100.85): VV017279.D (-2106) (-)

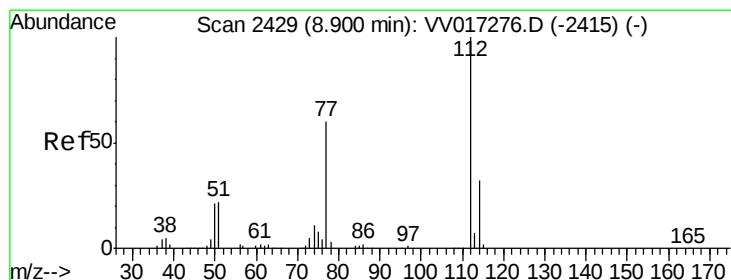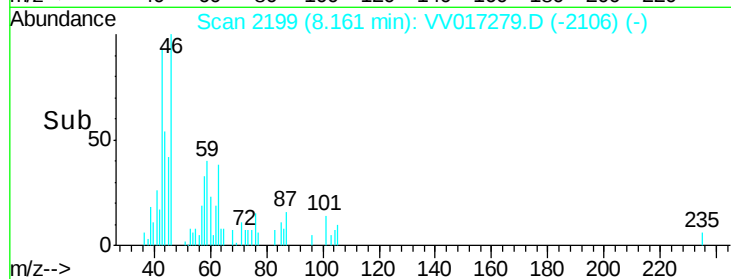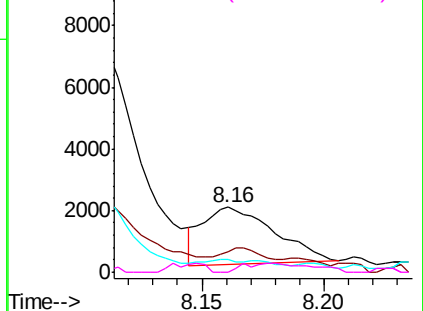

#53
Chlorobenzene
Concen: 4.849 ug/L
RT: 8.90 min Scan# 2430
Delta R.T. 0.00 min
Lab File: VV017279.D
Acq: 01 Jul 2020 10:47

Tgt Ion	Ratio	Lower	Upper
112	100		
114	32.7	22.0	41.0
77	55.9	46.0	69.0



Abundance Ion 112.10 (111.80 to 112.80): VV017279.D (-2336) (-)

Ion 114.05 (113.75 to 114.75): VV017279.D (-2336) (-)

Ion 77.10 (76.80 to 77.80): VV017279.D (-2336) (-)

