

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
 Data File : VV017295.D
 Acq On : 01 Jul 2020 17:34
 Operator : SY/MD
 Sample : L3168-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ9

Quant Time: Jul 02 03:08:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 02 03:02:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	167607	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	160397	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	76890	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45841	4.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.20%
7) Chloroethane-d5	1.58	69	42878	5.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.20%
11) 1,1-Dichloroethene-d2	2.13	63	74309	3.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.60%
20) 2-Butanone-d5	3.92	46	135837	52.98	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.96%
24) Chloroform-d	4.38	84	114210	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
26) 1,2-Dichloroethane-d4	5.06	65	63075	5.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.60%
32) Benzene-d6	5.07	84	205226	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.10	67	63718	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.34	98	183123	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
45) trans-1,3-Dichloropropene-	7.64	79	23501	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
48) 2-Hexanone-d5	8.11	63	88251	44.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.28%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	42328	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	75861	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%

Target Compounds

					Ovalue
3) Chloromethane	1.25	50	821	0.072 ug/L	89
5) Vinyl chloride	1.32	62	1302	0.118 ug/L #	1
8) Chloroethane	1.56	64	35433	5.830 ug/L #	51
10) 1,1,2-Trichloro-1,2,2-trif	2.13	101	1109	0.125 ug/L #	31
12) 1,1-Dichloroethene	2.14	96	2189	0.272 ug/L #	1
13) Acetone	2.20	43	23043	17.780 ug/L	97
15) Methyl Acetate	2.42	43	1943	0.613 ug/L #	54
16) Methylene chloride	2.53	84	2726	0.316 ug/L	96
18) trans-1,2-Dichloroethene	2.78	96	1237	0.145 ug/L #	60
21) 2-Butanone	4.02	43	10667	4.366 ug/L	94
22) cis-1,2-Dichloroethene	3.94	96	49550	4.251 ug/L	93
25) Chloroform	4.41	83	14722	0.704 ug/L	99
29) 1,1,1-Trichloroethane	4.64	97	7071	0.368 ug/L	95
33) Benzene	5.13	78	7501	0.179 ug/L	100
34) Trichloroethene	5.94	95	1295536	105.331 ug/L	99
35) Methylcyclohexane	6.10	83	17002	0.889 ug/L #	17
37) 1,2-Dichloropropane	6.09	63	8310	0.799 ug/L #	84

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
 Data File : VV017295.D
 Acq On : 01 Jul 2020 17:34
 Operator : SY/MD
 Sample : L3168-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ9

Quant Time: Jul 02 03:08:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 02 03:02:49 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
39) cis-1,3-Dichloropropene	7.01	75	2180	0.141	ug/L #	66
42) Toluene	7.41	91	87271	1.787	ug/L	98
43) 1,3,5-Trimethylbenzene	10.56	105	1818	0.042	ug/L	92
44) 1,2,4-Trimethylbenzene	10.94	105	7239	0.163	ug/L	96
46) trans-1,3-Dichloropropene	7.65	75	1464	0.110	ug/L	92
49) Tetrachloroethene	8.00	164	3241	0.327	ug/L	94
50) 2-Hexanone	8.16	43	6417	1.502	ug/L #	42
51) Dibromochloromethane	8.00	129	2874	0.321	ug/L #	11
54) Ethylbenzene	9.04	91	7821	0.150	ug/L	94
55) m,p-xylene	9.16	106	13474	0.659	ug/L	90
56) o-xylene	9.56	106	5164	0.271	ug/L	91
70) Naphthalene	13.54	128	2073	0.096	ug/L #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070120\
Data File : VV017295.D
Acq On : 01 Jul 2020 17:34
Operator : SY/MD
Sample : L3168-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ9

Quant Time: Jul 02 03:08:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 02 03:02:49 2020
Response via : Initial Calibration

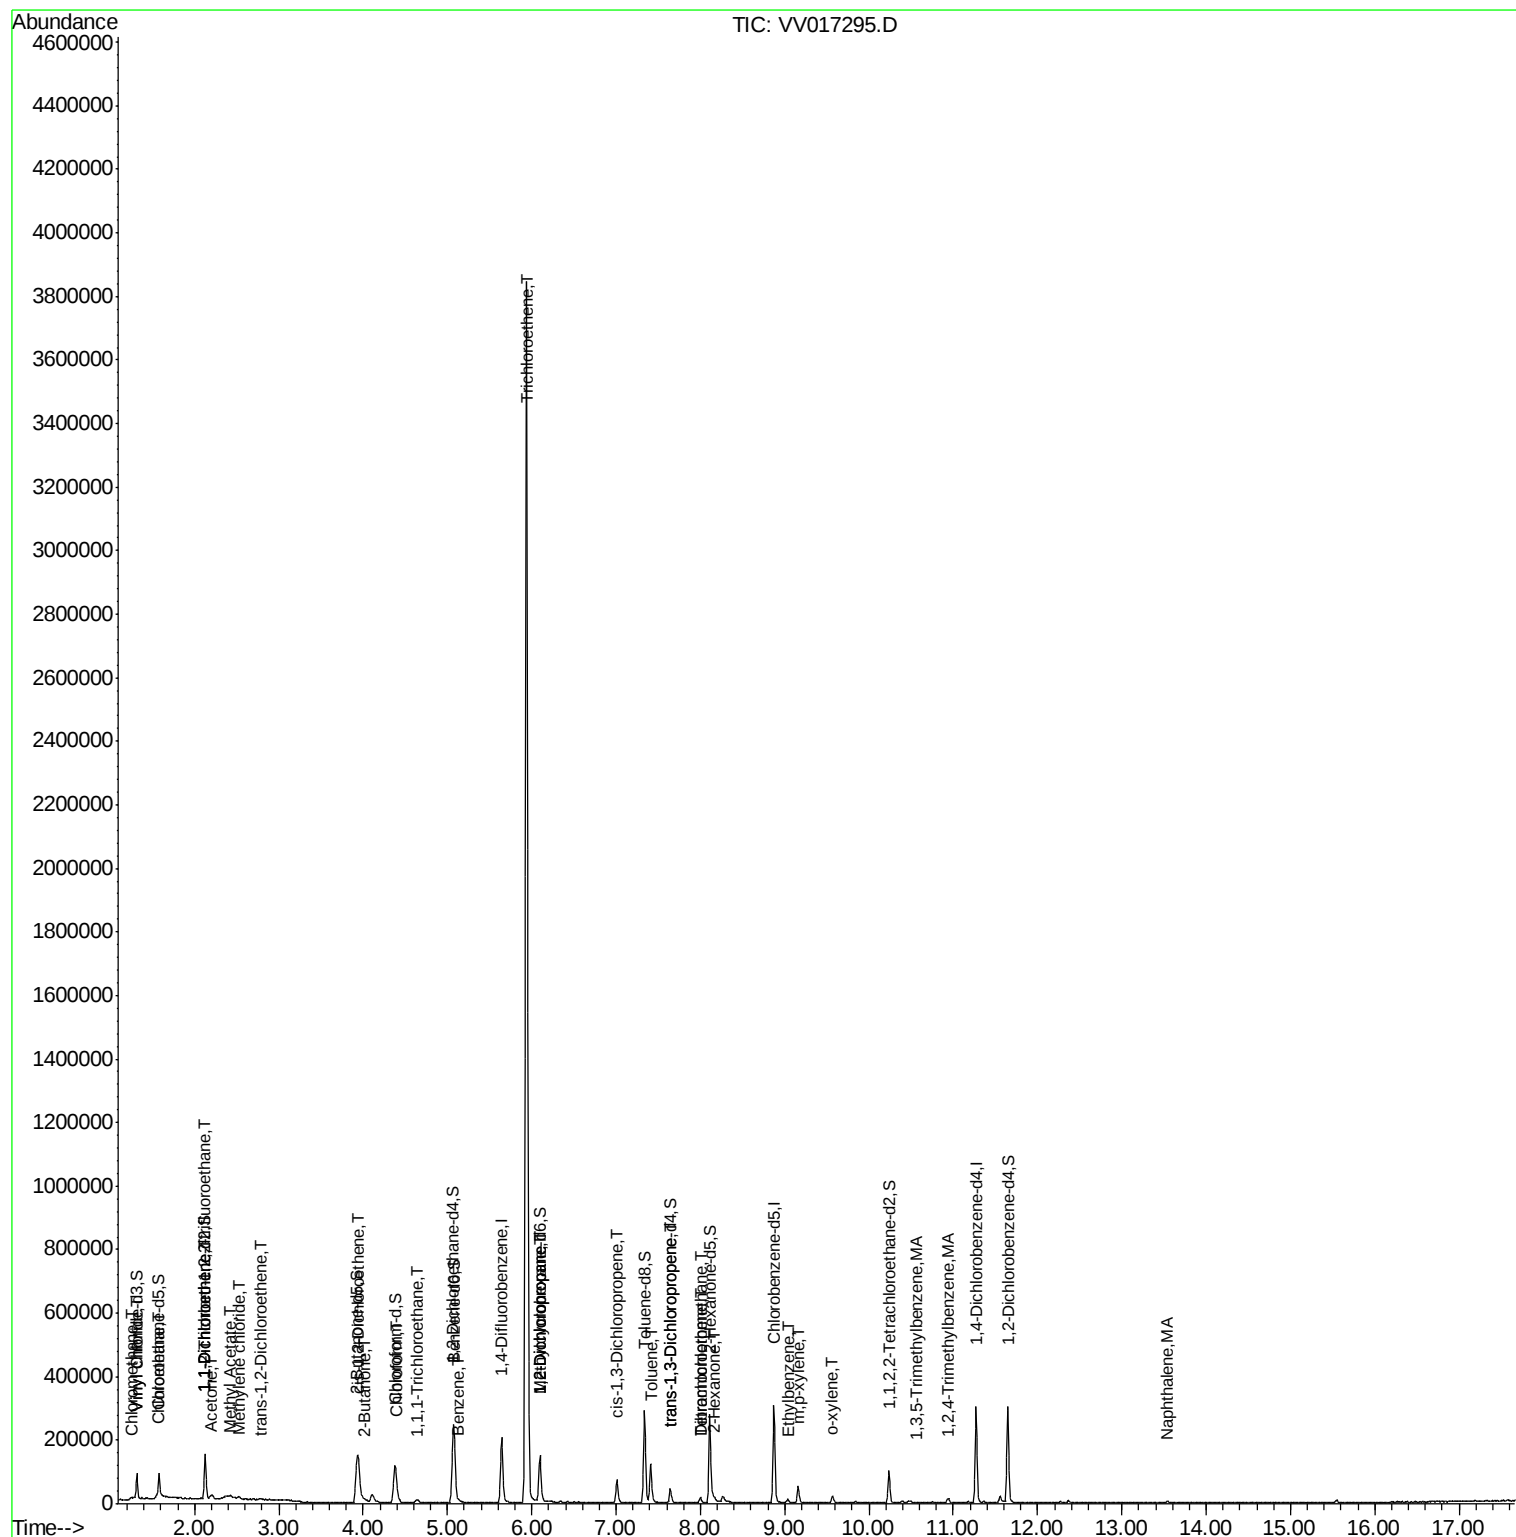



#3

Chloromethane

Concen: 0.072 ug/L

RT: 1.25 min Scan# 50

Delta R.T. 0.00 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampled :


C0AJ9

Tot Ion: 50 Resp: 821

Ion Ratio Lower Upper

50 100

52 38.3 22.5 41.9

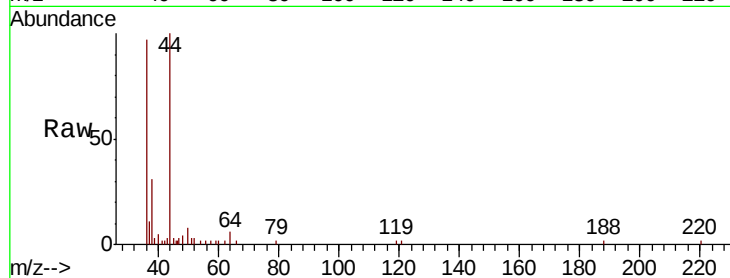

Abundance Ion 50.05 (49.75 to 50.75): VV017276.D (-37) (-)

Ion 52.05 (51.75 to 52.75): VV017295.D (-1) (-)

1.25

1.22 1.24 1.26 1.28 1.30

600

500

400



300

200

100

0

Time-->

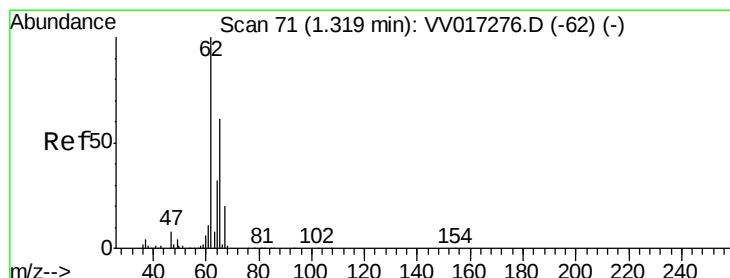

#5

Vinyl chloride

Concen: 0.118 ug/L

RT: 1.32 min Scan# 71

Delta R.T. 0.00 min

Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Tgt Ion: 62 Resp: 1302

Ion Ratio Lower Upper

62 100

64 104.5 22.5 41.7#

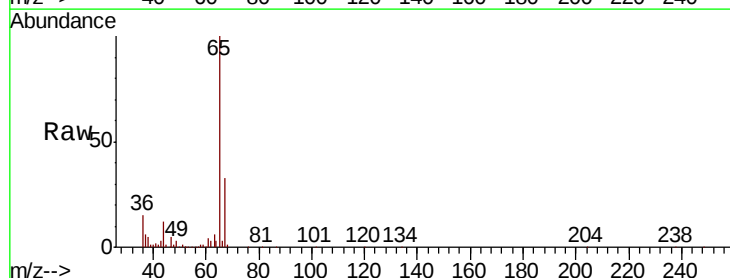

Abundance Ion 62.00 (61.70 to 62.70): VV017276.D (-62) (-)

Ion 64.10 (63.80 to 64.80): VV017295.D (-1) (-)

1.32

1.30 1.35

1200

1000

800


600


400

200

0

Time-->







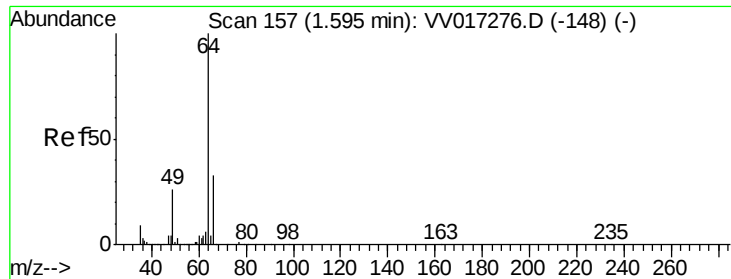

#8
Chloroethane
Concen: 5.830 ug/L
RT: 1.56 min Scan# 146
Delta R.T. -0.04 min
Lab File: VV017295.D
Acq: 01 Jul 2020 17:34




Instrument :
MSVOA_V
ClientSampleId :
C0AJ9


Tot Ion: 64 Resp: 35433
Ion Ratio Lower Upper
64 100
66 5.2 22.8 42.4#

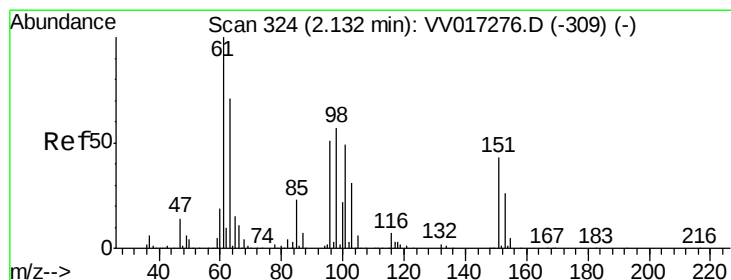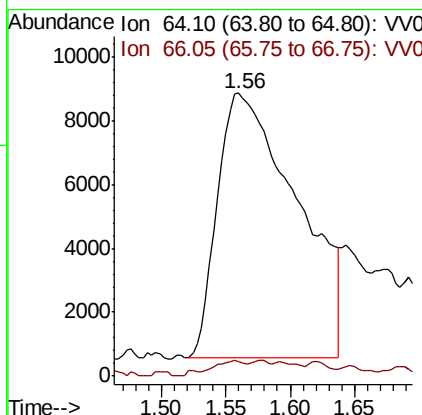

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.125 ug/L
RT: 2.13 min Scan# 324
Delta R.T. 0.00 min
Lab File: VV017295.D
Acq: 01 Jul 2020 17:34

Tgt Ion:101 Resp: 1109
Ion Ratio Lower Upper
101 100
85 24.3 35.4 53.2#
151 0.0 63.9 95.9#

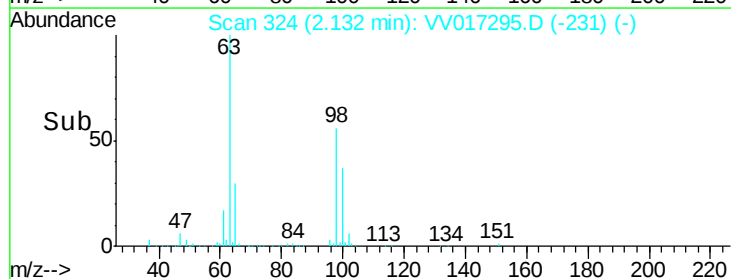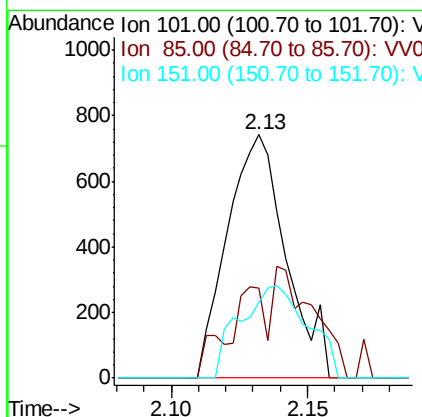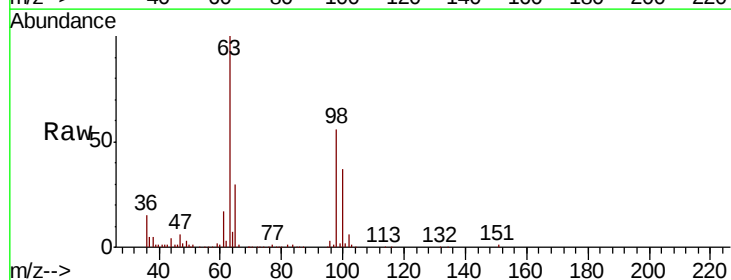

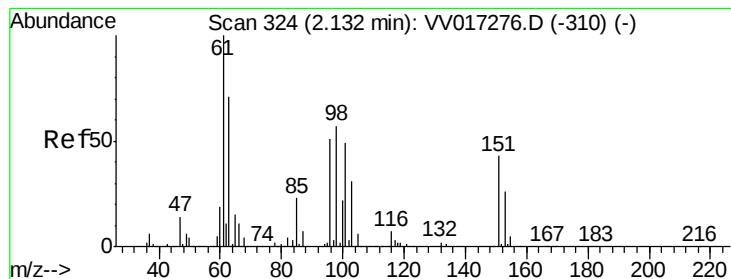

#12

1,1-Dichloroethene

Concen: 0.272 ug/L

RT: 2.14 min Scan# 325

Delta R.T. 0.00 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampleId :

C0AJ9


Tot Ion: 96 Resp: 2189

Ion Ratio Lower Upper

96 100

61 455.7 125.0 232.2#




63 2493.9 109.8 203.8#



Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 63.00 (62.70 to 63.70): VV0

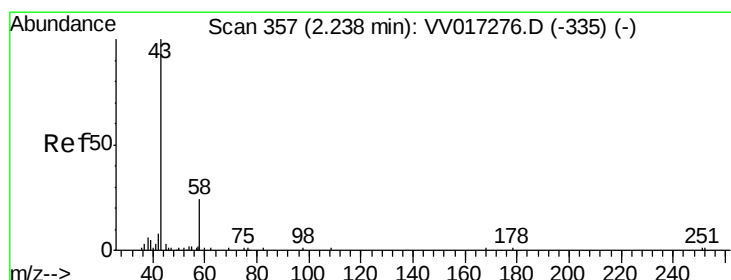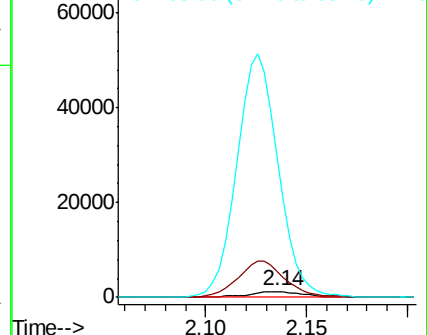

#13

Acetone

Concen: 17.780 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.04 min

Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Tgt Ion: 43 Resp: 23043

Ion Ratio Lower Upper



43 100


58 30.9 0.0 58.4



Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

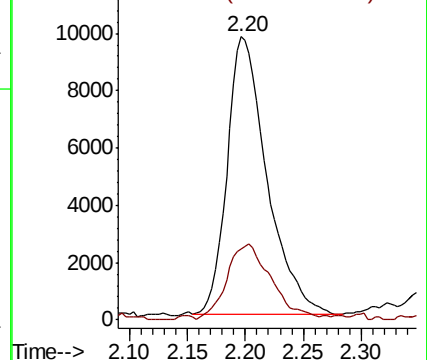



#15

Methyl Acetate

Concen: 0.613 ug/L

RT: 2.42 min Scan# 415

Delta R.T. -0.04 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampled :


C0AJ9

Tot Ion: 43 Resp: 1943

Ion Ratio Lower Upper




43 100

74 1.0 19.1 28.7#

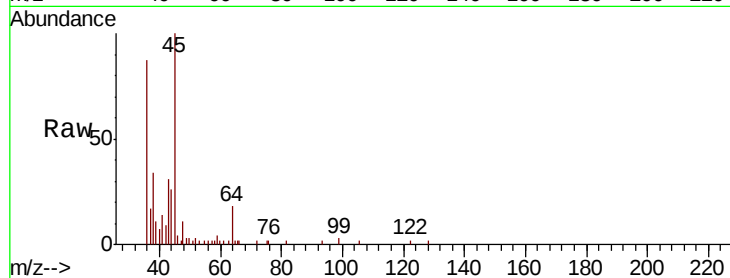

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 74.05 (73.75 to 74.75): VV0

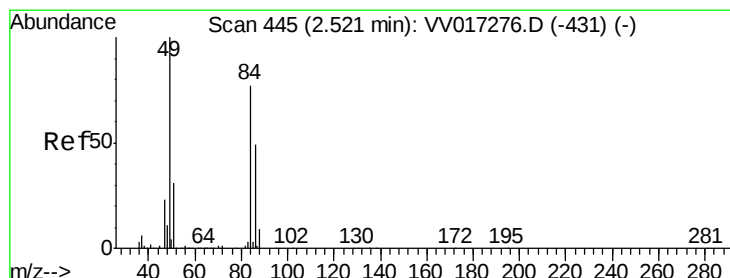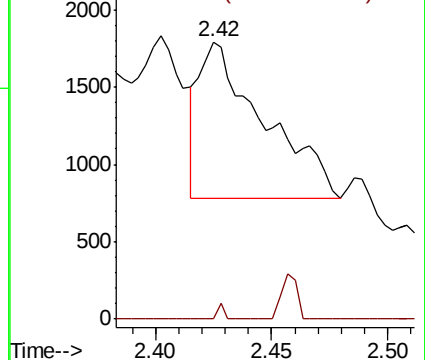

#16

Methylene chloride

Concen: 0.316 ug/L

RT: 2.53 min Scan# 447

Delta R.T. 0.01 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34


Tgt Ion: 84 Resp: 2726

Ion Ratio Lower Upper

84 100

86 70.4 45.8 85.0



49 125.2 89.6 166.4

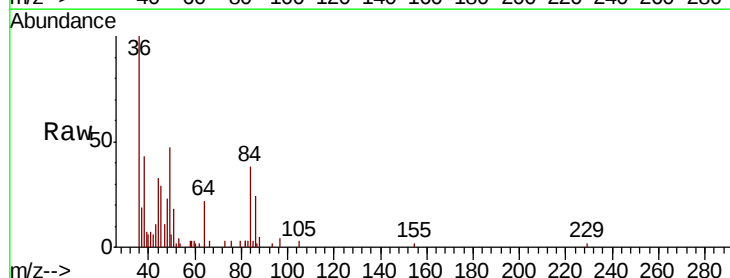


Abundance Ion 84.05 (83.75 to 84.75): VV0

Ion 86.00 (85.70 to 86.70): VV0

Ion 49.10 (48.80 to 49.80): VV0

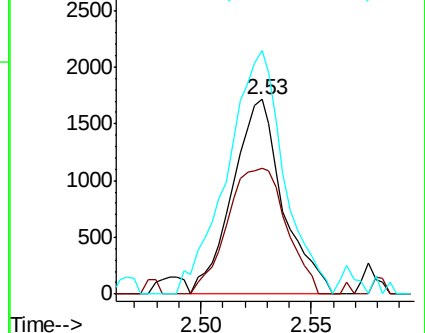

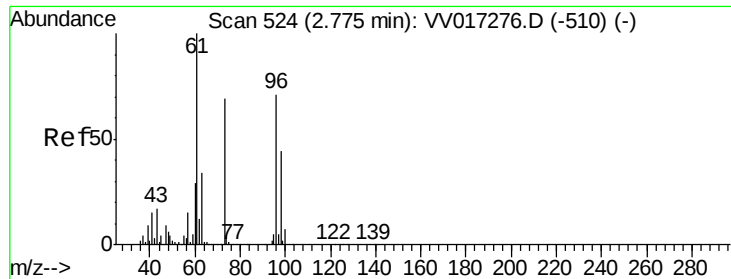

#18

trans-1,2-Dichloroethene

Concen: 0.145 ug/L

RT: 2.78 min Scan# 527

Delta R.T. 0.01 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampled :

C0AJ9


Tot Ion: 96 Resp: 1237

Ion Ratio Lower Upper

96 100

61 87.6 102.3 189.9#




98 44.6 44.7 82.9#

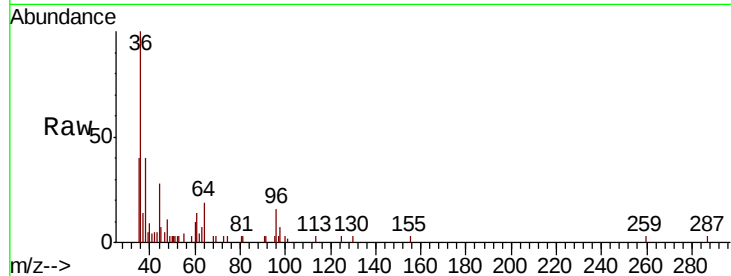

Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 97.95 (97.65 to 98.65): VV0

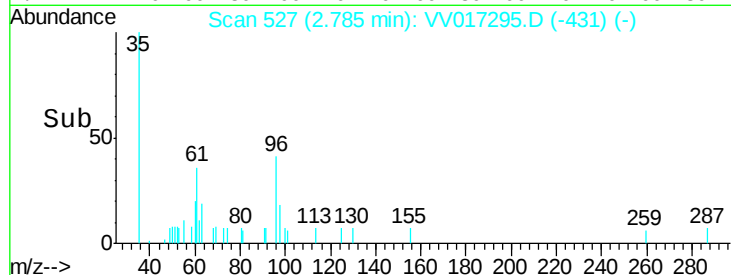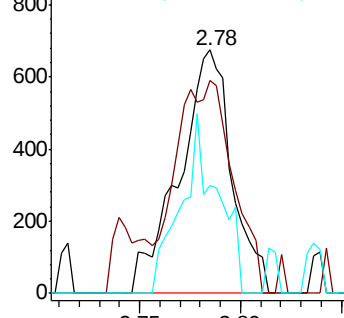

#21

2-Butanone

Concen: 4.366 ug/L

RT: 4.02 min Scan# 911

Delta R.T. -0.02 min

Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Tgt Ion: 43 Resp: 10667

Ion Ratio Lower Upper



43 100


72 28.0 12.4 37.4



Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 72.00 (71.70 to 72.70): VV0




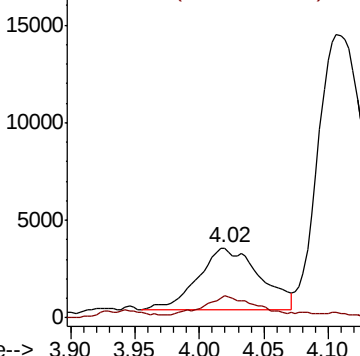


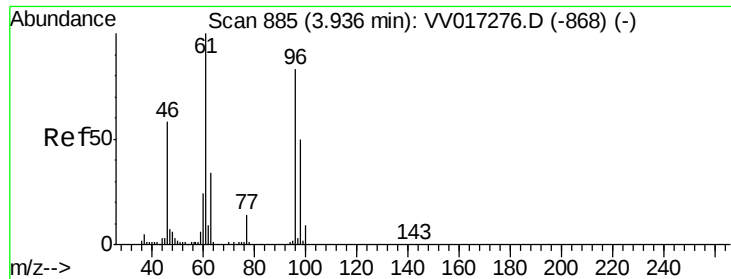

#22
 cis-1,2-Dichloroethene
 Concen: 4.251 ug/L
 RT: 3.94 min Scan# 886
 Delta R.T. 0.00 min
 Lab File: VV017295.D
 Acq: 01 Jul 2020 17:34




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ9


Tot Ion: 96 Resp: 49550
 Ion Ratio Lower Upper
 96 100
 61 138.2 91.0 169.0
 68 0.0 0.0 0.0

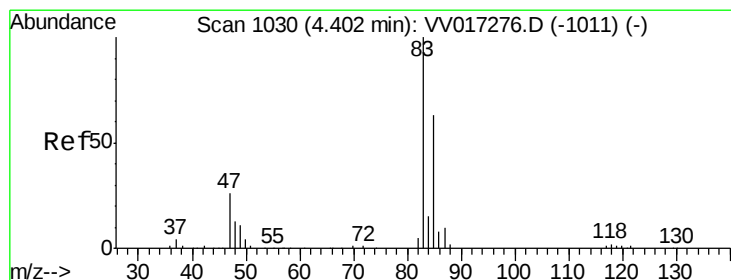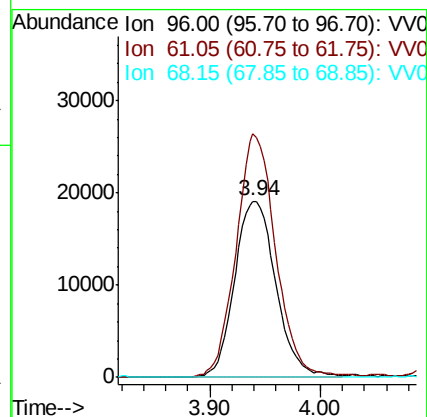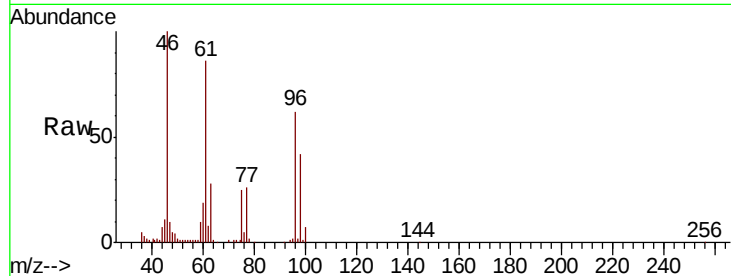

#25
 Chloroform
 Concen: 0.704 ug/L
 RT: 4.41 min Scan# 1031
 Delta R.T. 0.00 min
 Lab File: VV017295.D
 Acq: 01 Jul 2020 17:34

Tgt Ion: 83 Resp: 14722
 Ion Ratio Lower Upper
 83 100
 85 63.6 44.2 82.2

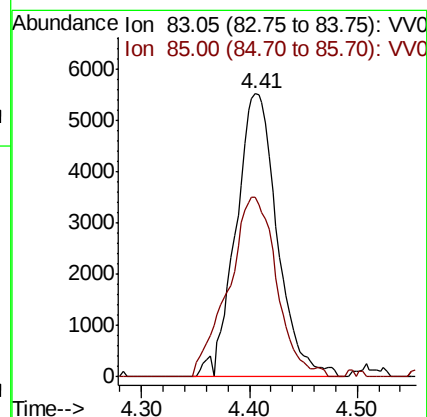

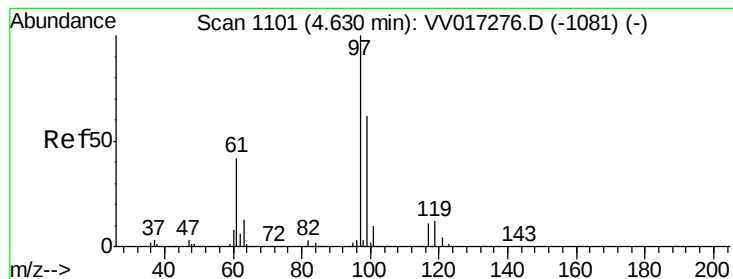

#29

1,1,1-Trichloroethane

Concen: 0.368 ug/L

RT: 4.64 min Scan# 1104

Delta R.T. 0.01 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampleId :

C0AJ9


Tot Ion: 97 Resp: 7071

Ion Ratio Lower Upper

97 100

99 58.5 50.3 75.5




61 47.1 36.0 54.0

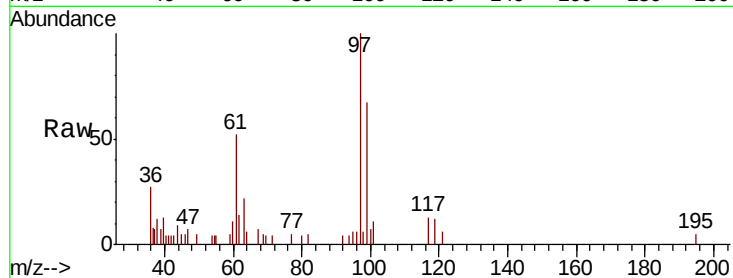

Abundance Ion 96.95 (96.65 to 97.65): VV0

Ion 99.05 (98.75 to 99.75): VV0

Ion 61.05 (60.75 to 61.75): VV0

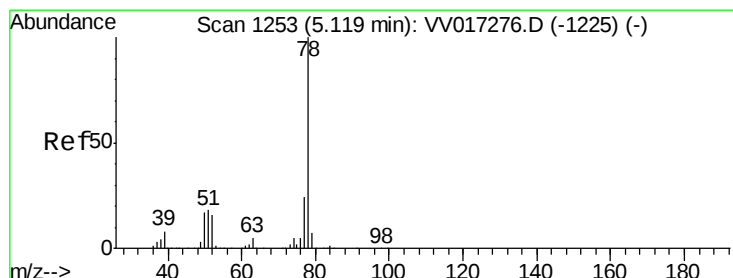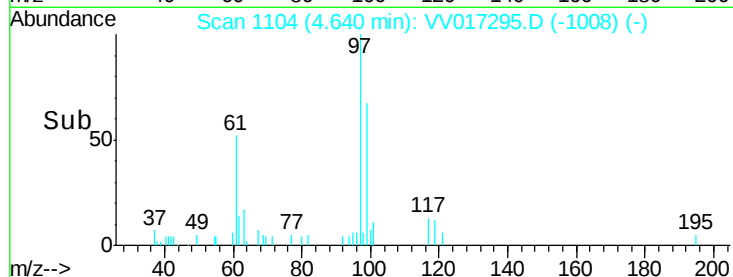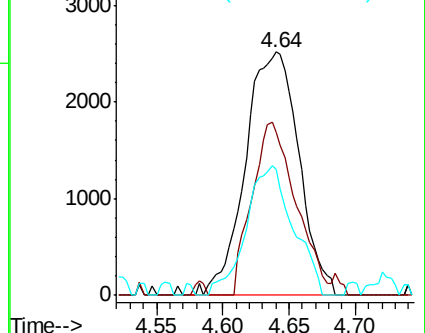

#33

Benzene

Concen: 0.179 ug/L


RT: 5.13 min Scan# 1256

Delta R.T. 0.01 min



Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Tgt Ion: 78 Resp: 7501

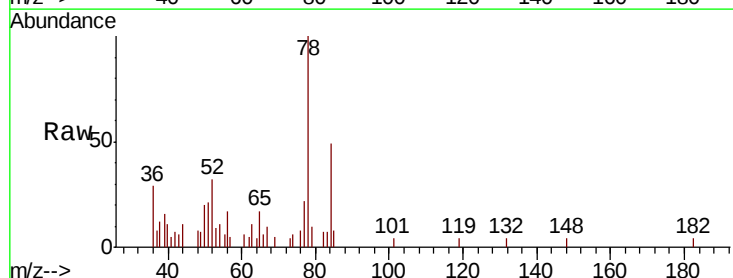

Abundance Ion 78.10 (77.80 to 78.80): VV0

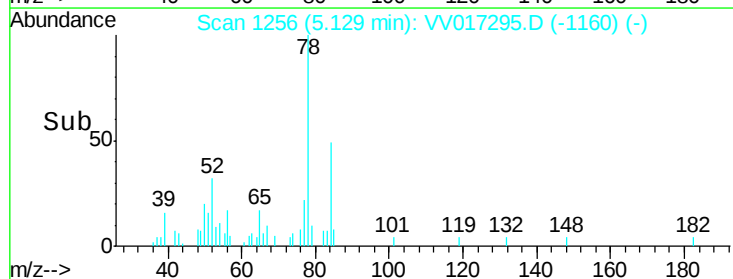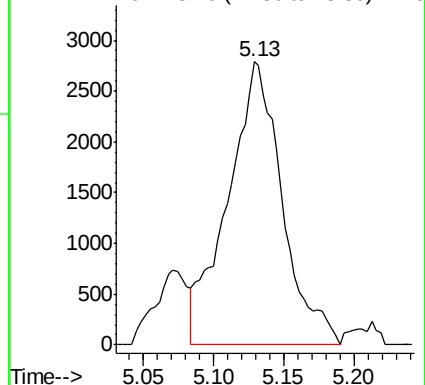


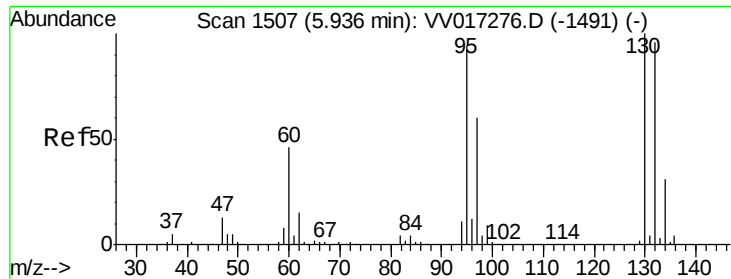




#34
 Trichloroethene
 Concen: 105.331 ug/L
 RT: 5.94 min Scan# 1507
 Delta R.T. 0.00 min
 Lab File: VV017295.D
 Acq: 01 Jul 2020 17:34

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ9

Tot Ion: 95 Resp: 1295536
 Ion Ratio Lower Upper
 95 100
 97 64.0 45.3 84.1
 132 98.7 68.8 127.8
 130 102.8 70.2 130.4

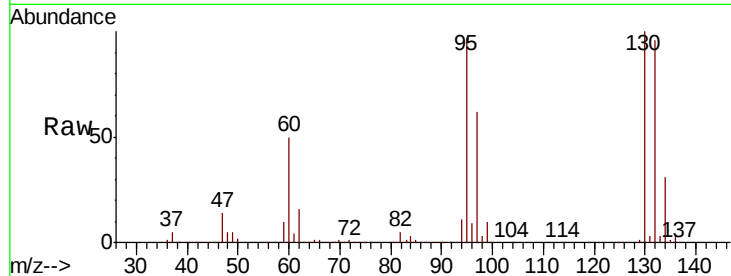


Abundance Ion 95.00 (94.70 to 95.70): VV0
 Ion 96.95 (96.65 to 97.65): VV0
 Ion 131.95 (131.65 to 132.65): VV0
 Ion 129.95 (129.65 to 130.65): VV0


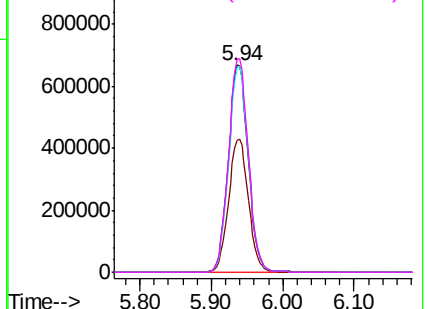



#35
 Methylcyclohexane
 Concen: 0.889 ug/L
 RT: 6.10 min Scan# 1557
 Delta R.T. -0.05 min
 Lab File: VV017295.D
 Acq: 01 Jul 2020 17:34

Tgt Ion: 83 Resp: 17002
 Ion Ratio Lower Upper
 83 100
 55 0.3 63.6 95.4#
 98 0.0 38.8 58.2#



Abundance Ion 83.15 (82.85 to 83.85): VV0
 Ion 55.10 (54.80 to 55.80): VV0
 Ion 98.15 (97.85 to 98.85): VV0



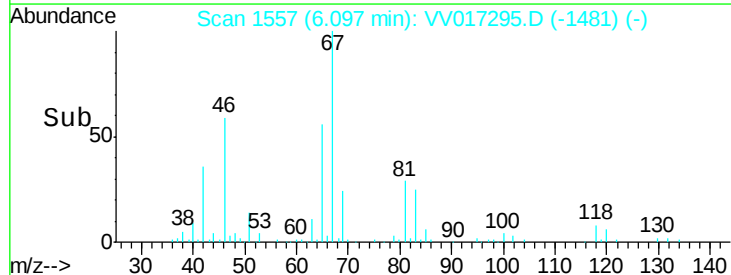
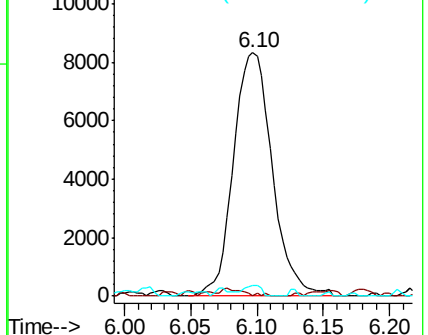




#37
 1,2-Dichloropropane
 Concen: 0.799 ug/L
 RT: 6.09 min Scan# 1556
 Delta R.T. -0.10 min
 Lab File: VV017295.D
 Acq: 01 Jul 2020 17:34




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ9


Tot Ion: 63 Resp: 8310
 Ion Ratio Lower Upper
 63 100
 112 0.2 4.4 6.6#

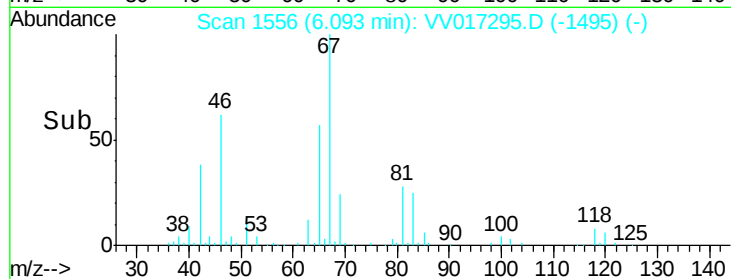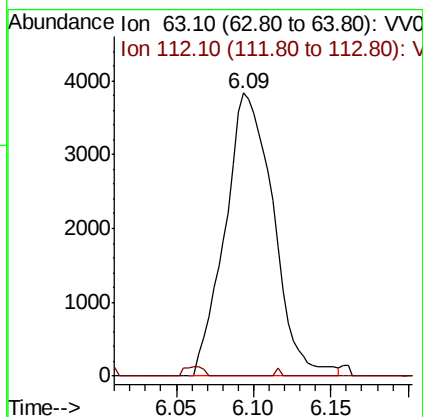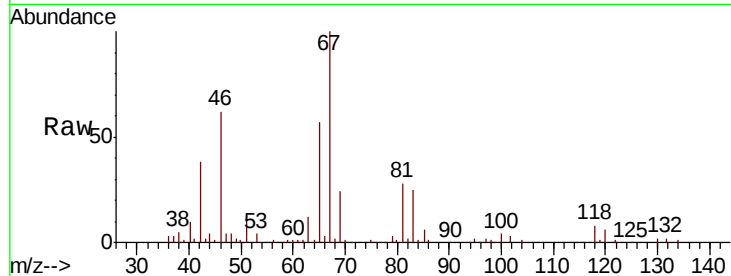

#39
 cis-1,3-Dichloropropene
 Concen: 0.141 ug/L
 RT: 7.01 min Scan# 1842
 Delta R.T. -0.04 min
 Lab File: VV017295.D
 Acq: 01 Jul 2020 17:34

Tgt Ion: 75 Resp: 2180
 Ion Ratio Lower Upper
 75 100
 77 50.7 22.3 41.5#

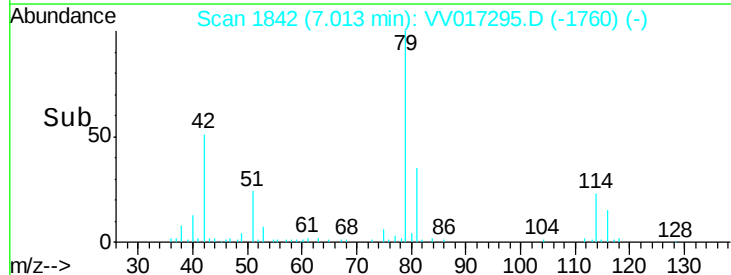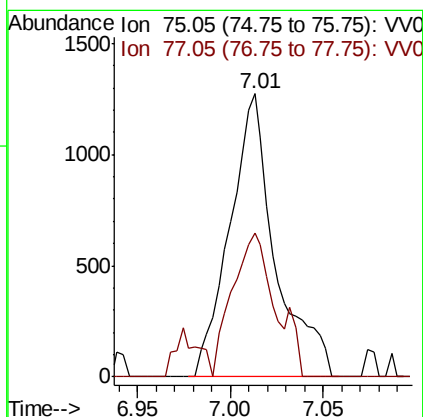

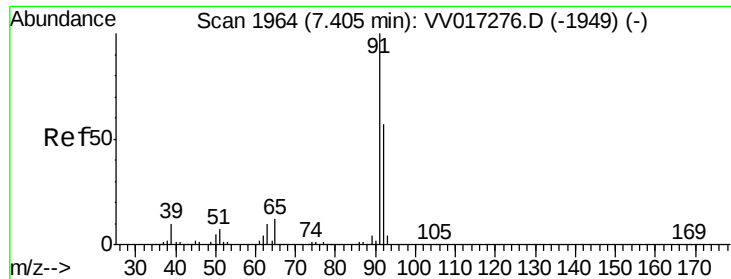

#42

Toluene

Concen: 1.787 ug/L

RT: 7.41 min Scan# 1966

Delta R.T. 0.01 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampled :


C0AJ9

Tot Ion: 91 Resp: 87271

Ion Ratio Lower Upper

91 100

92 55.7 39.9 74.1

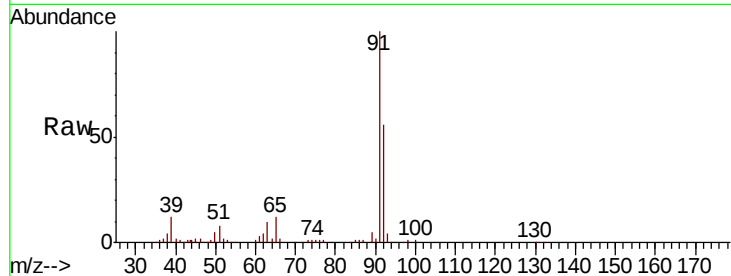

Abundance Ion 91.15 (90.85 to 91.85): VV017276.D (-1949) (-)

Ion 92.15 (91.85 to 92.85): VV017295.D (-1871) (-)

7.41

50000

40000

30000



20000

10000

0

7.35 7.40 7.45 7.50

Time-->



#43

1,3,5-Trimethylbenzene

Concen: 0.042 ug/L

RT: 10.56 min Scan# 2946

Delta R.T. 0.00 min

Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Tgt Ion:105 Resp: 1818

Ion Ratio Lower Upper

105 100

120 42.7 38.6 57.8



Abundance Ion 105.00 (104.70 to 105.70): VV017276.D (-2929) (-)

Ion 120.00 (119.70 to 120.70): VV017295.D (-2323) (-)

1500


1000


500

0

10.50 10.55 10.60

Time-->









#44
1,2,4-Trimethylbenzene
Concen: 0.163 ug/L
RT: 10.94 min Scan# 3063
Delta R.T. 0.00 min
Lab File: VV017295.D
Acq: 01 Jul 2020 17:34




Instrument :
MSVOA_V
ClientSampleId :
C0AJ9


Tot Ion:105 Resp: 7239
Ion Ratio Lower Upper
105 100
120 42.1 35.8 53.8

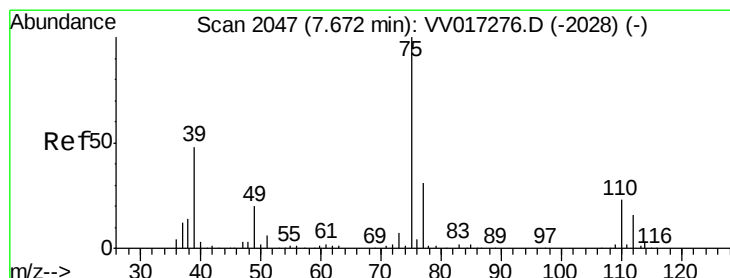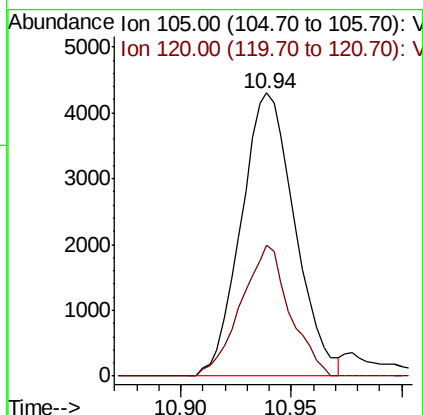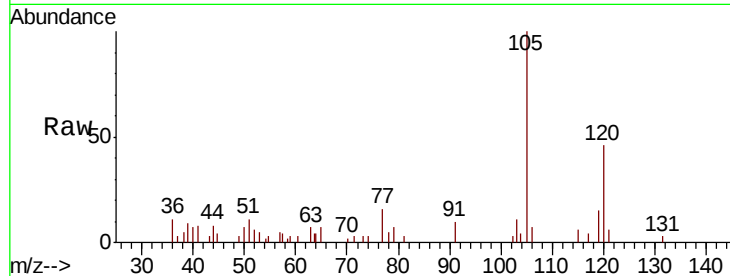

#46
trans-1,3-Dichloropropene
Concen: 0.110 ug/L
RT: 7.65 min Scan# 2040
Delta R.T. -0.02 min
Lab File: VV017295.D
Acq: 01 Jul 2020 17:34

Tgt Ion: 75 Resp: 1464
Ion Ratio Lower Upper
75 100
77 36.0 22.3 41.3

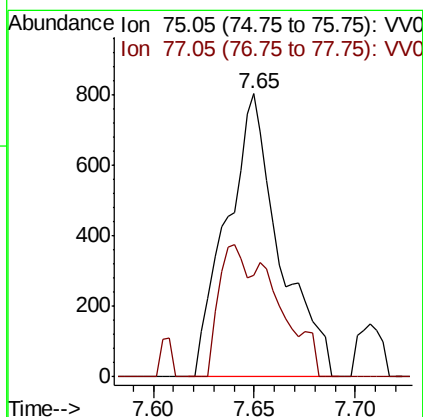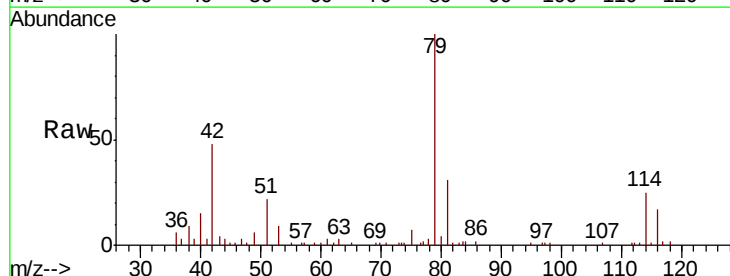

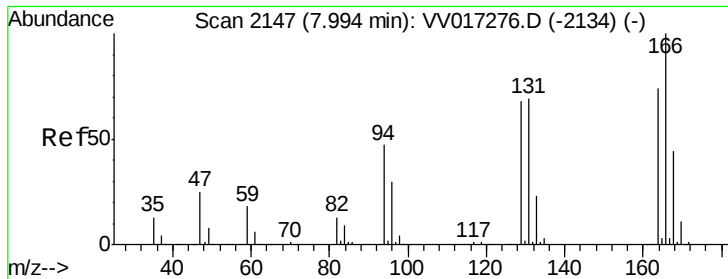

#49

Tetrachloroethene

Concen: 0.327 ug/L

RT: 8.00 min Scan# 2150

Delta R.T. 0.01 min

Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampleId :

C0AJ9

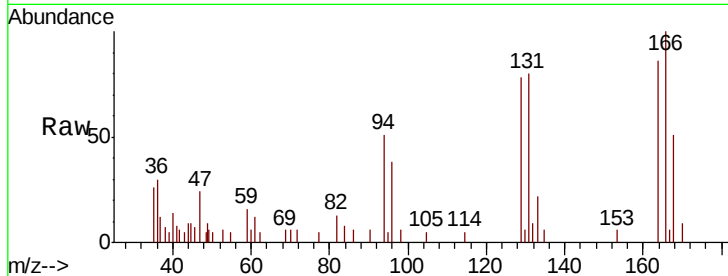

Tot Ion:164 Resp: 3241

Ion Ratio Lower Upper

164 100

129 90.5 65.2 121.0

131 92.2 64.1 119.1




166 115.8 90.2 167.4

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

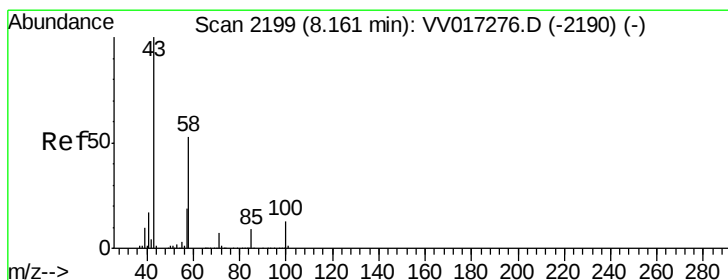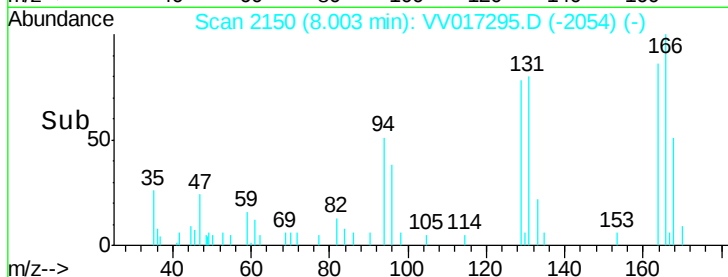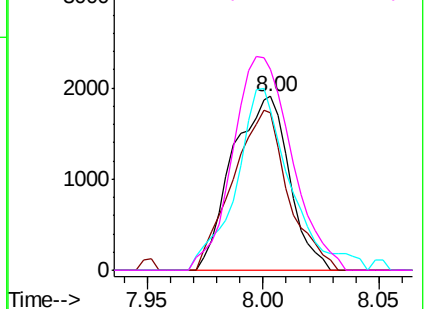

#50

2-Hexanone

Concen: 1.502 ug/L

RT: 8.16 min Scan# 2200

Delta R.T. 0.00 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Tgt Ion: 43 Resp: 6417

Ion Ratio Lower Upper

43 100

58 0.0 41.6 62.4#

57 0.0 15.4 23.0#




100 6.2 10.1 15.1#


Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

Ion 57.20 (56.90 to 57.90): VV0

Ion 100.15 (99.85 to 100.85): VV0

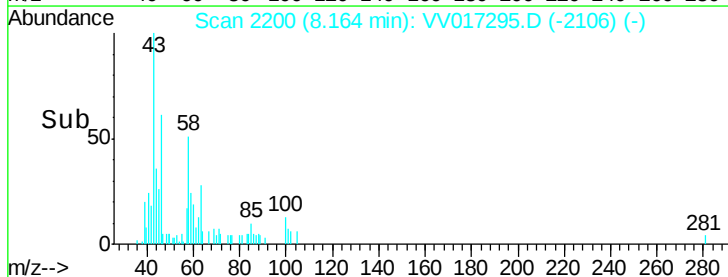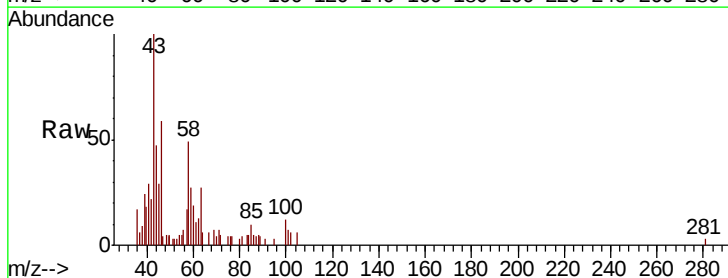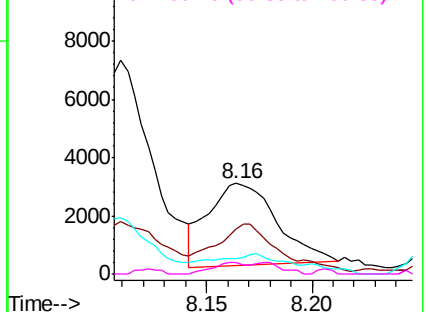



#51

Dibromochloromethane

Concen: 0.321 ug/L

RT: 8.00 min Scan# 2149

Delta R.T. -0.27 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampleId :


C0AJ9

Tot Ion:129 Resp: 2874

Ion Ratio Lower Upper




129 100

127 0.0 54.1 100.5#

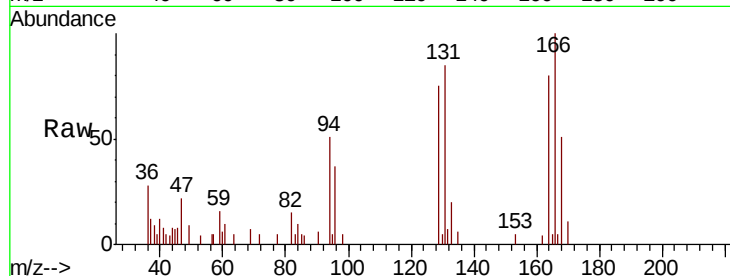

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

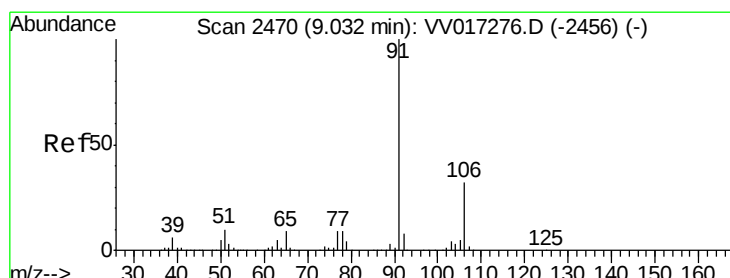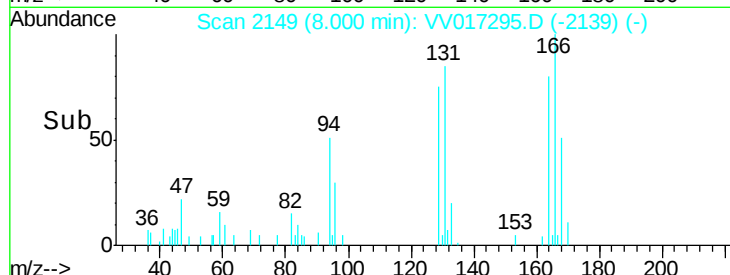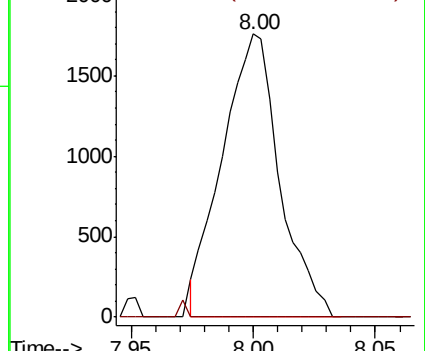

#54

Ethylbenzene

Concen: 0.150 ug/L

RT: 9.04 min Scan# 2471

Delta R.T. 0.00 min

Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Tgt Ion: 91 Resp: 7821

Ion Ratio Lower Upper



91 100


106 33.3 21.1 39.1

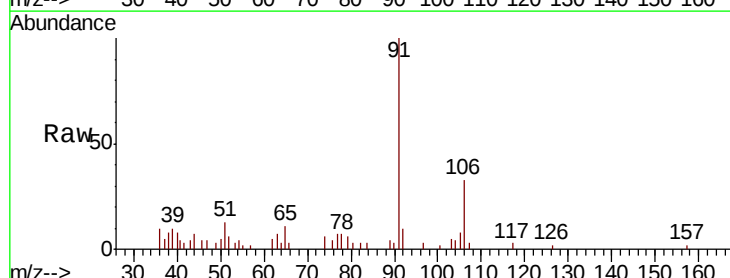

Abundance Ion 91.15 (90.85 to 91.85): VV0

Ion 106.15 (105.85 to 106.85): V

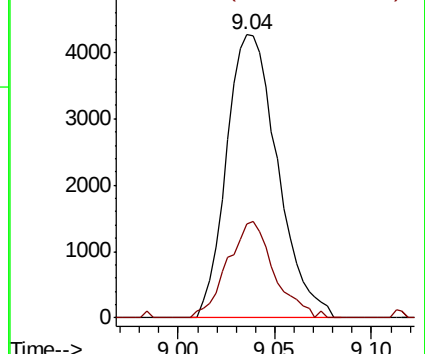

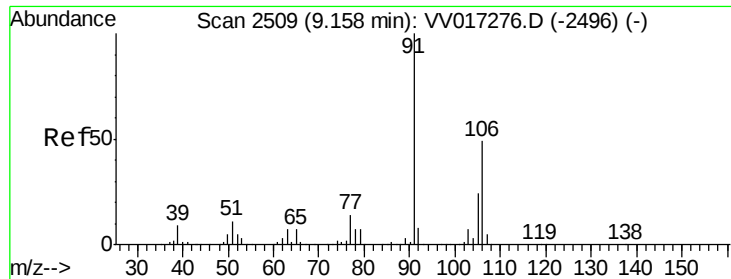

#55

m,p-xylene

Concen: 0.659 ug/L

RT: 9.16 min Scan# 2509

Delta R.T. 0.00 min

Lab File: VV017295.D

Acq: 01 Jul 2020 17:34

Instrument :

MSVOA_V

ClientSampleId :


C0AJ9

Tot Ion:106 Resp: 13474

Ion Ratio Lower Upper




106 100

91 218.5 142.7 264.9

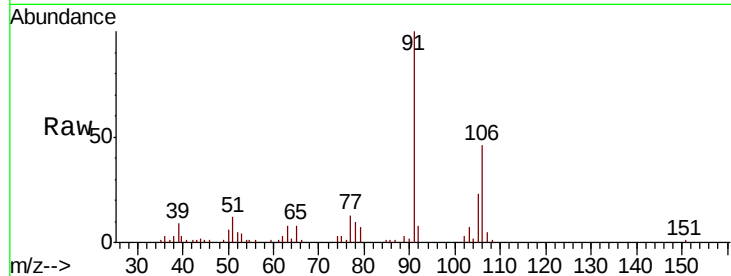

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VV0

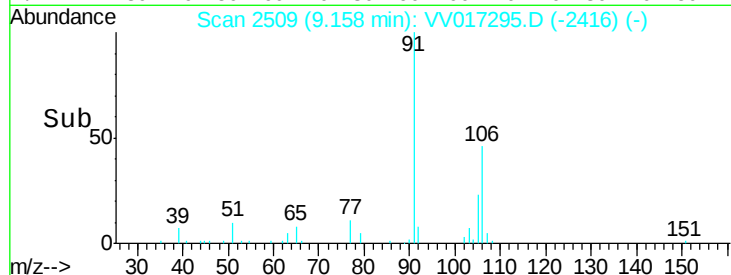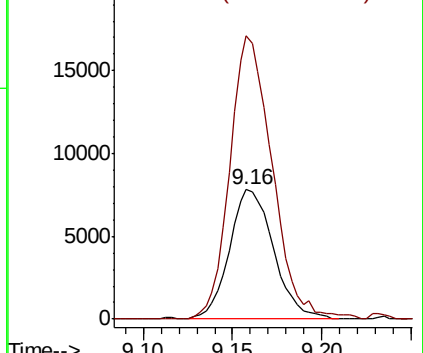

#56

o-xylene

Concen: 0.271 ug/L

RT: 9.56 min Scan# 2635

Delta R.T. 0.00 min

Lab File: VV017295.D


Acq: 01 Jul 2020 17:34

Tgt Ion:106 Resp: 5164

Ion Ratio Lower Upper



106 100


91 205.8 153.6 285.2



Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VV0

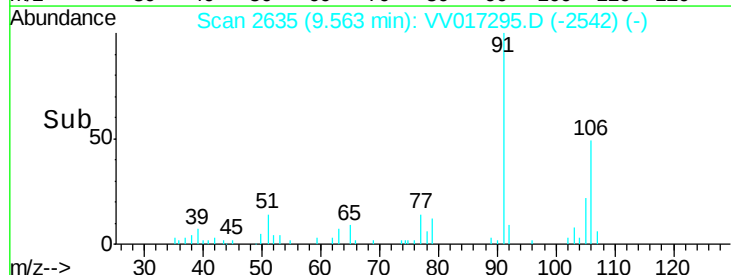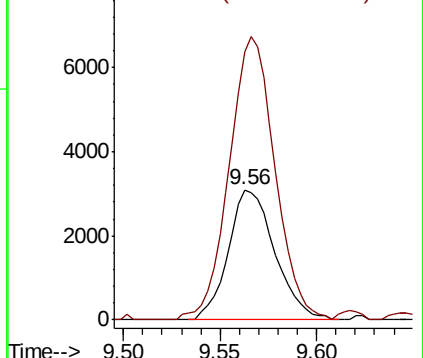




#70
Naphthalene
Concen: 0.096 ug/L
RT: 13.54 min Scan# 3871
Delta R.T. 0.01 min
Lab File: VV017295.D
Acq: 01 Jul 2020 17:34

Instrument :
MSVOA_V
ClientSampleId :
C0AJ9

Tot Ion:128 Resp: 2073
Ion Ratio Lower Upper
128 100
129 16.4 8.8 13.2#
127 13.9 10.5 15.7



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 129.00 (128.70 to 129.70): V
Ion 127.00 (126.70 to 127.70): V

