


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
Data File : VV017278.D
Acq On : 01 Jul 2020 10:23
Operator : SY/MD
Sample : L3150-14
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETYJ9

Manual Integrations
APPROVED

apatel
7/6/2020 10:13:35 AM

Quant Time: Jul 02 03:38:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 02 03:02:49 2020
Response via : Initial Calibration

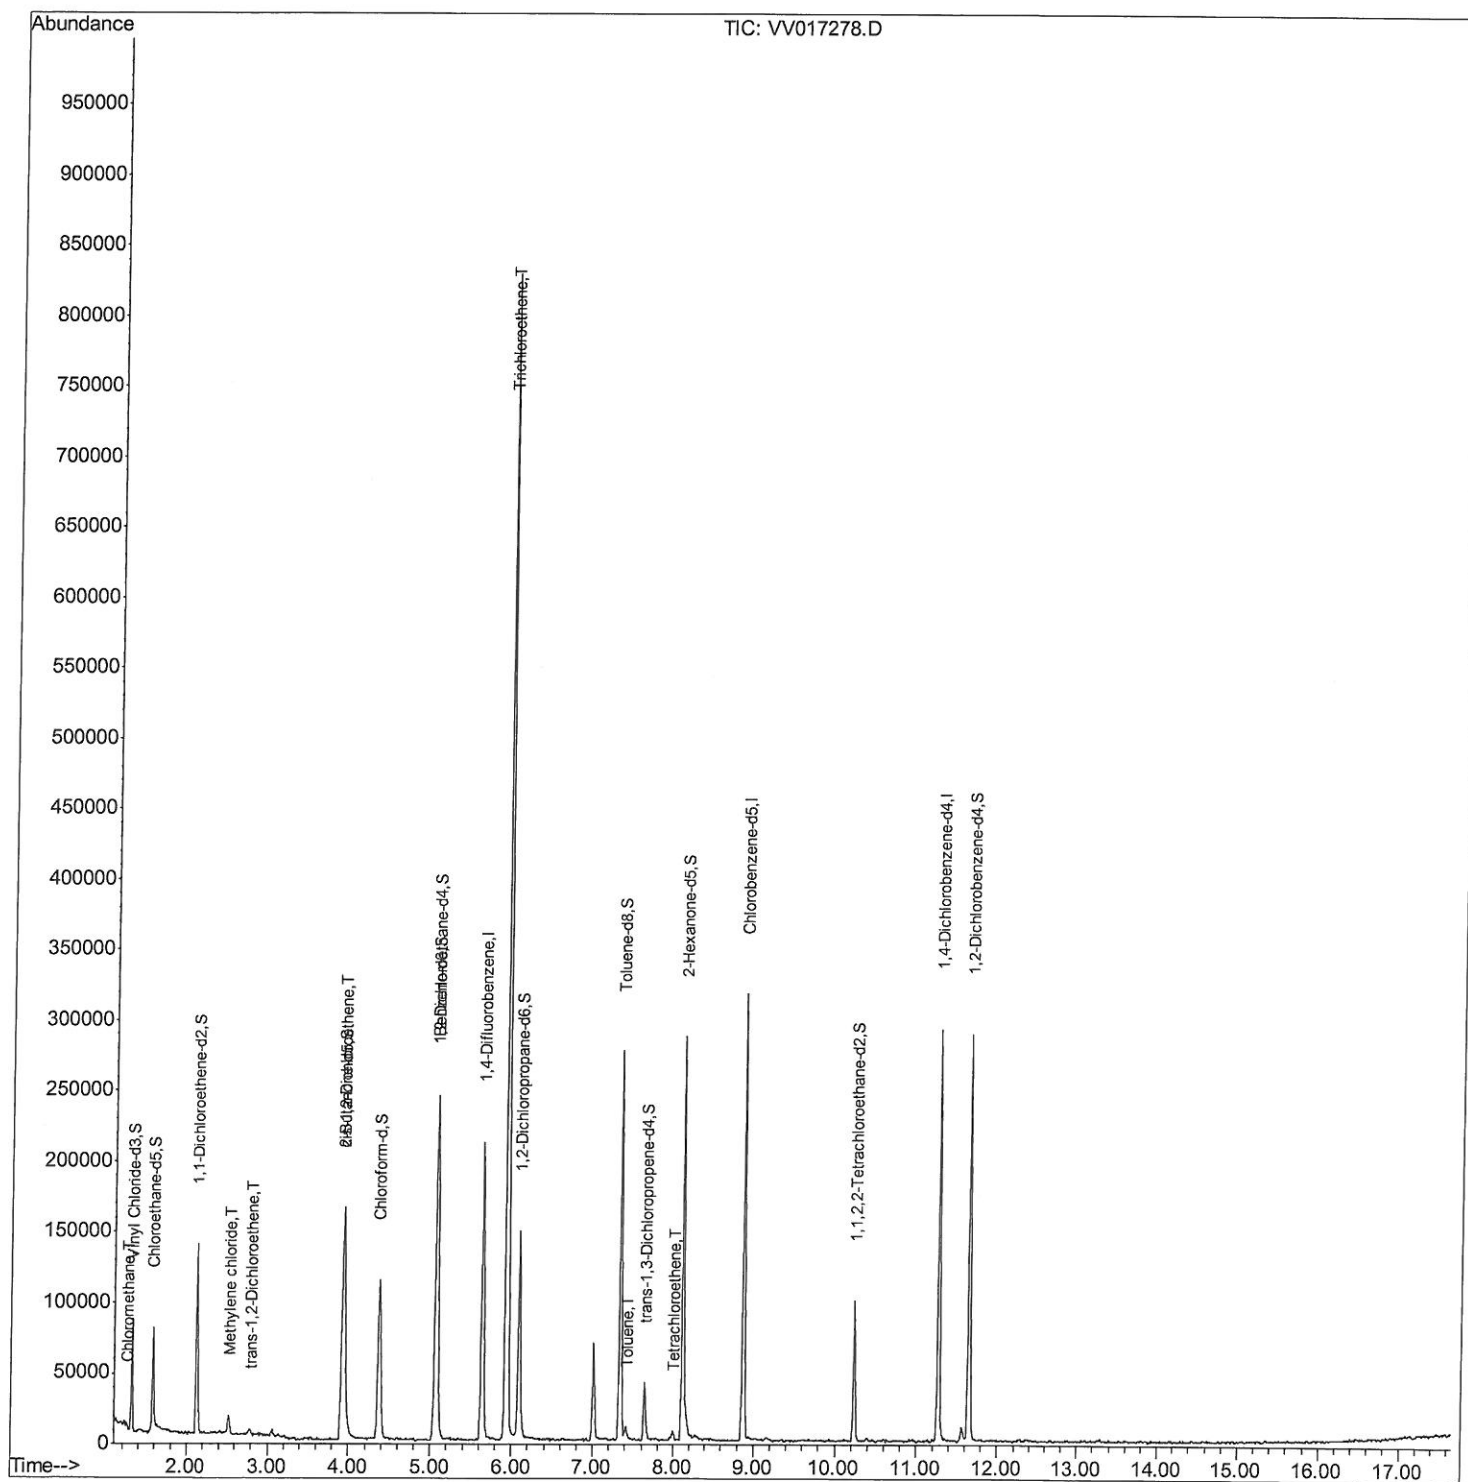

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
Data File : VV017278.D
Acq On : 01 Jul 2020 10:23
Operator : SY/MD
Sample : L3150-14
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETYJ9

Manual Integrations
APPROVED

apatel
7/6/2020 10:13:35 AM

Quant Time: Jul 02 03:36:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 02 03:02:49 2020
Response via : Initial Calibration

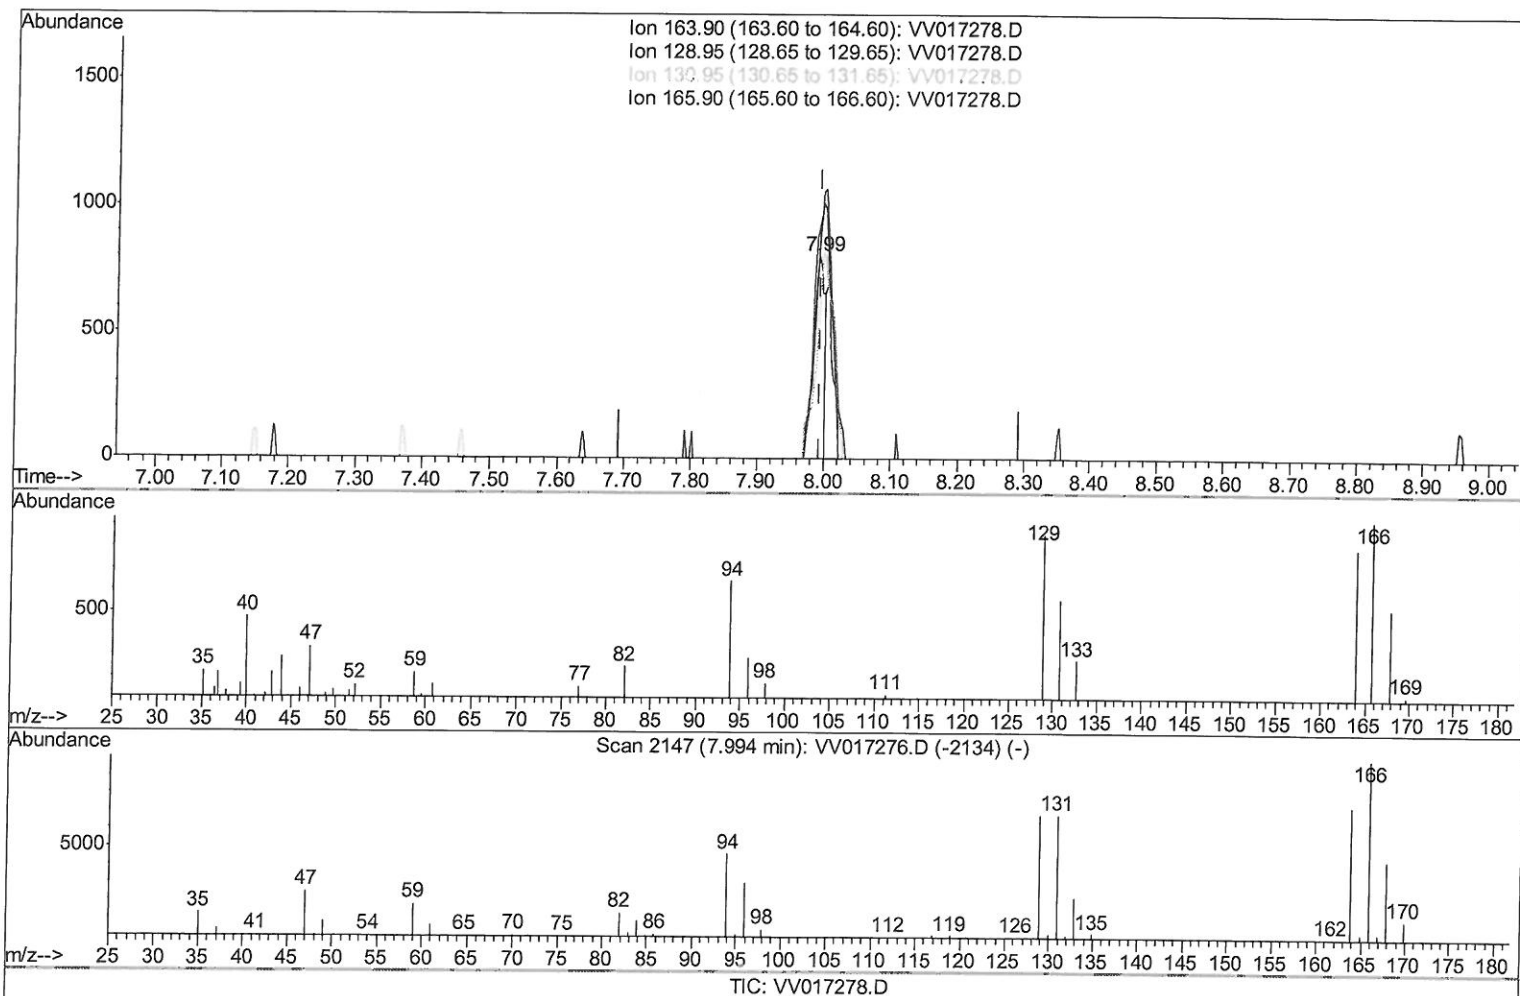

(49) Tetrachloroethene (T)

7.990min (-0.003) 0.09ug/L

response 921

Ion	Exp%	Act%
163.90	100	100
128.95	93.10	107.61
130.95	91.60	69.83
165.90	128.80	115.96

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
 Data File : VV017278.D
 Acq On : 01 Jul 2020 10:23
 Operator : SY/MD
 Sample : L3150-14
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETYJ9

Manual Integrations
 APPROVED

apatel
 7/6/2020 10:13:35 AM

Quant Time: Jul 02 03:36:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 02 03:02:49 2020
 Response via : Initial Calibration

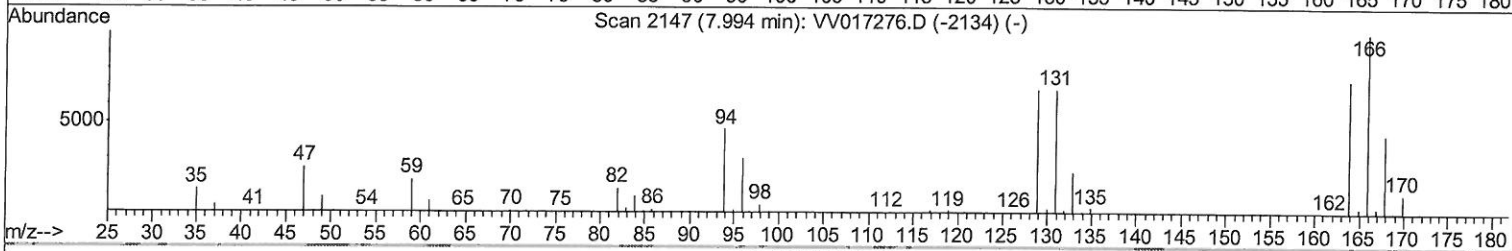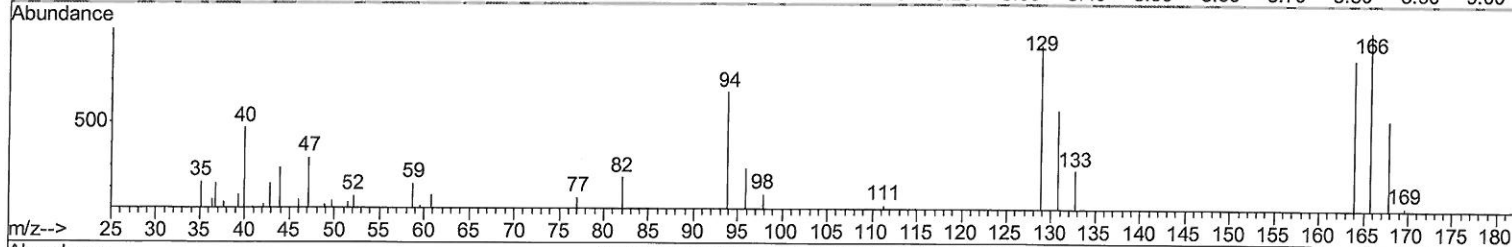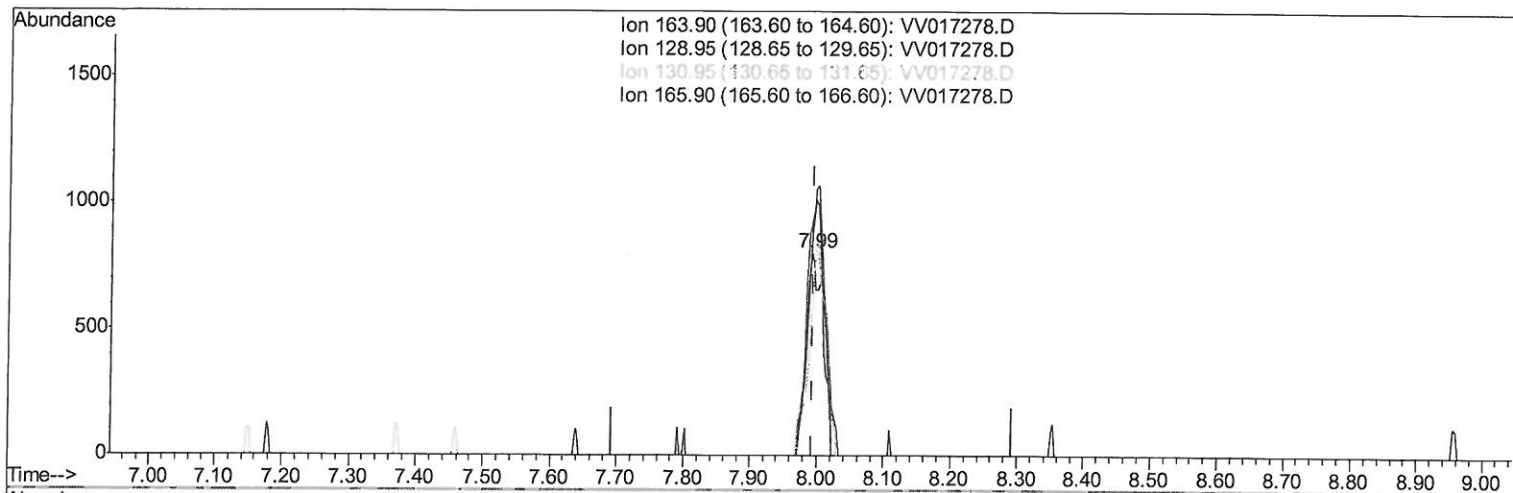

TIC: VV017278.D

(49) Tetrachloroethene (T)

7.990min (-0.003) 0.14ug/L m

response 1474

7 MD
7/6/20

Ion	Exp%	Act%
163.90	100	100
128.95	93.10	107.61
130.95	91.60	69.83
165.90	128.80	115.96

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070120\
 Data File : VV017278.D
 Acq On : 01 Jul 2020 10:23
 Operator : SY/MD
 Sample : L3150-14
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETYJ9

Manual Integrations
 APPROVED

apatel
 7/6/2020 10:13:35 AM

Quant Time: Jul 02 03:38:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 02 03:02:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	171367	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	168083	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	72756	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46511	4.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.40%
7) Chloroethane-d5	1.58	69	40946	5.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.60%
11) 1,1-Dichloroethene-d2	2.13	63	71757	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	3.92	46	136063	51.91	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.82%
24) Chloroform-d	4.37	84	114444	5.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.00%
26) 1,2-Dichloroethane-d4	5.06	65	63208	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.40%
32) Benzene-d6	5.07	84	205177	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.09	67	62027	4.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.00%
41) Toluene-d8	7.34	98	174826	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.40%
45) trans-1,3-Dichloropropene-	7.64	79	23513	4.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.40%
48) 2-Hexanone-d5	8.11	63	92137	44.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.94%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	43356	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	72064	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Chloromethane	1.25	50	2221	0.192	ug/L	95
16) Methylene chloride	2.52	84	5626	0.639	ug/L	97
18) trans-1,2-Dichloroethene	2.78	96	1366	0.157	ug/L	88
22) cis-1,2-Dichloroethene	3.94	96	57108	4.792	ug/L	# 100
34) Trichloroethene	5.94	95	276912	21.484	ug/L	98
42) Toluene	7.41	91	5957	0.116	ug/L	90
49) Tetrachloroethene	7.99	164	1474m	0.142	ug/L	7 MD

(#) = qualifier out of range (m) = manual integration (+) = signals summed