


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV070120\
 Data File : VV017275.D
 Acq On : 01 Jul 2020 08:38
 Operator : SY/MD
 Sample : BFB45
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB45

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 02 03:02:49 2020

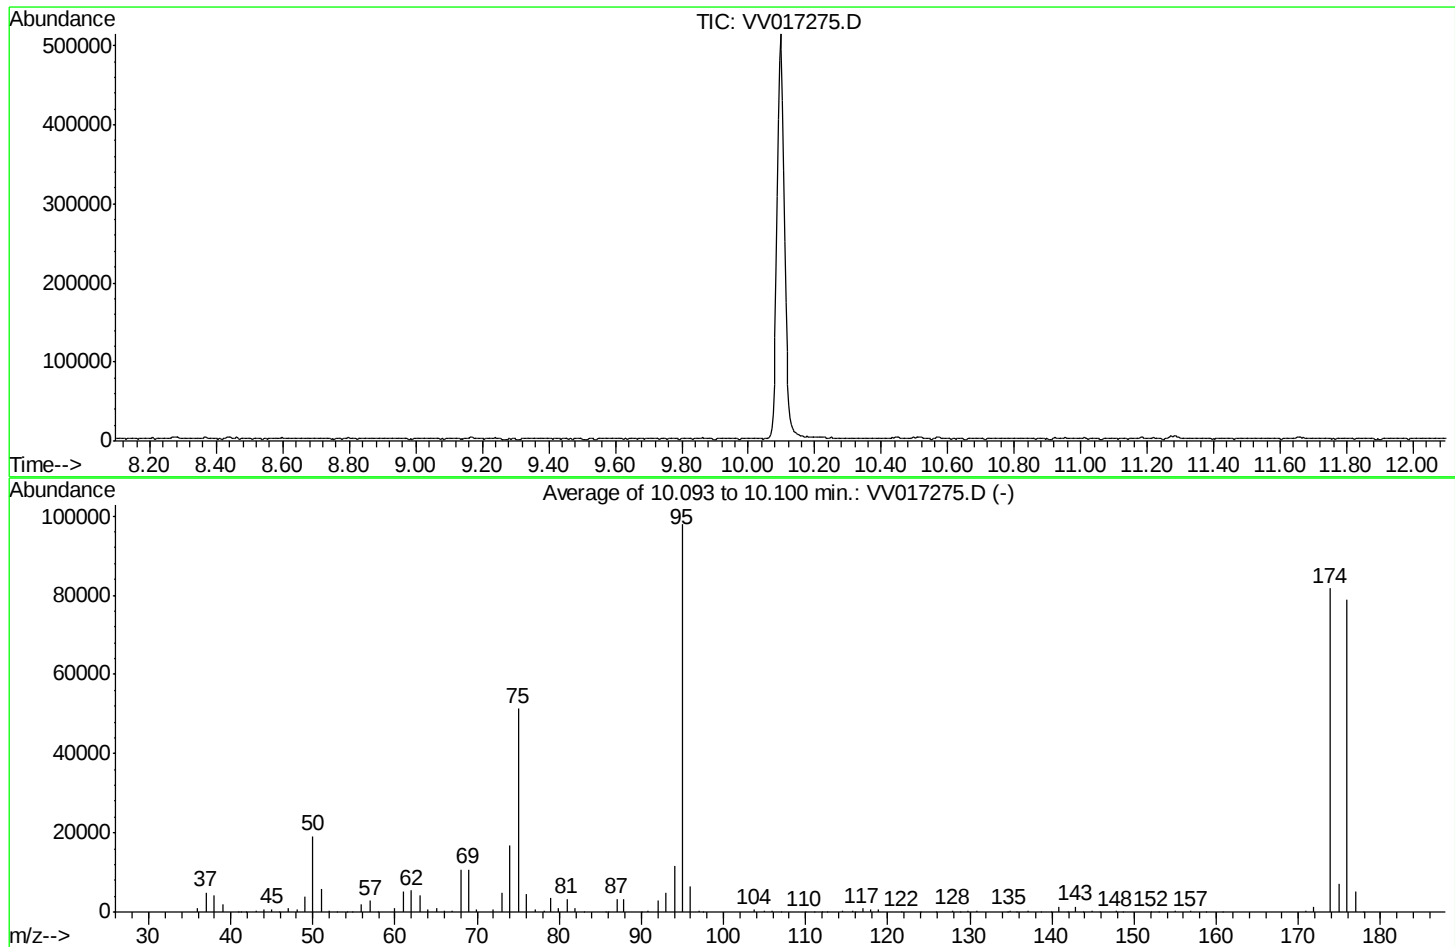

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	19090	PASS
75	95	30	80	52.4	51258	PASS
95	95	100	100	100.0	97909	PASS
96	95	5	9	6.6	6472	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.5	81706	PASS
175	174	5	9	8.7	7093	PASS
176	174	95	101	96.4	78733	PASS
177	176	5	9	6.7	5254	PASS

m/z	Abundance
35.90	777.0
37.00	4891.0
38.00	4180.0
39.00	1929.0
40.00	416.0
40.90	126.0
41.10	119.0
41.80	163.0
43.10	193.0
43.90	1026.0
45.00	681.0
45.90	238.0
47.00	1134.0
48.10	849.0
49.00	3921.0
50.00	19208.0
51.00	5640.0
52.10	333.0
52.90	184.0
54.90	243.0
56.00	1916.0
57.00	2942.0
57.90	169.0
59.90	995.0
61.00	4609.0
62.00	5348.0
63.00	4000.0
63.90	659.0
65.00	999.0
66.00	131.0
67.00	329.0
68.00	10426.0
69.00	10257.0
69.90	743.0
71.00	106.0
72.10	538.0
73.00	4422.0
74.00	16400.0
75.00	50248.0
76.00	4357.0
77.00	681.0
78.10	358.0
78.90	3588.0
79.90	1037.0
80.90	3478.0
81.90	840.0
83.00	116.0
86.00	188.0
87.00	3221.0
87.90	2937.0
90.80	274.0
92.00	2970.0
93.00	4543.0
94.00	11227.0
95.00	95096.0
96.00	6538.0
97.00	305.0
97.70	105.0
103.80	512.0
104.90	201.0
105.80	452.0
106.90	159.0
109.90	149.0
111.10	143.0
112.80	109.0
114.50	181.0
115.80	357.0
116.90	859.0
117.90	469.0
118.80	694.0
121.70	121.0
125.90	156.0
128.00	423.0
128.80	134.0
129.80	359.0
130.90	237.0
134.90	236.0
135.70	120.0
137.10	170.0
138.70	127.0
139.90	126.0
140.90	1265.0
141.90	175.0
142.90	1440.0
143.70	145.0
144.90	432.0
145.70	131.0
147.80	214.0
152.00	117.0
155.00	255.0
156.90	250.0
158.80	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

160.70	128.0
170.90	307.0
171.90	1318.0
173.90	77856.0
175.00	6769.0
175.90	74744.0
177.00	5117.0
177.90	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
36.00	852.0
37.00	5256.0
38.00	4479.0
39.00	2024.0
40.00	318.0
41.20	157.0
41.80	189.0
43.10	189.0
44.00	986.0
45.00	817.0
46.00	216.0
47.00	1177.0
48.10	873.0
49.00	4104.0
50.00	19728.0
51.00	6137.0
52.10	369.0
52.90	169.0
54.10	133.0
54.80	271.0
56.00	1870.0
57.00	2873.0
58.00	125.0
59.90	1092.0
61.00	5319.0
62.00	5723.0
63.00	4191.0
63.90	619.0
65.10	1081.0
66.00	199.0
67.00	372.0
68.00	10957.0
69.00	11342.0
70.00	819.0
71.00	104.0
71.90	535.0
73.00	4892.0
74.00	17464.0
75.00	53256.0
76.00	4598.0
77.00	666.0
78.10	317.0
78.90	3824.0
79.90	1005.0
80.90	3428.0
81.90	918.0
83.00	127.0
86.00	158.0
87.00	3459.0
87.90	3193.0
90.00	109.0
90.80	328.0
92.00	3012.0
93.00	4861.0
94.00	12156.0
95.00	101384.0
96.00	6717.0
96.90	253.0
97.50	129.0
103.80	541.0
105.00	176.0
105.80	489.0
107.00	138.0
109.90	194.0
111.00	156.0
112.00	134.0
112.60	130.0
114.50	238.0
115.80	391.0
116.90	935.0
117.90	601.0
118.80	653.0
125.90	149.0
127.90	457.0
128.70	152.0
129.80	356.0
130.90	236.0
134.70	246.0
135.00	257.0
135.70	129.0
137.00	187.0
138.70	162.0
139.90	131.0
140.90	1262.0
142.00	144.0
142.90	1488.0
143.70	166.0
144.90	395.0
145.80	129.0
147.80	244.0
148.60	125.0
152.10	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

153.00	101.0
155.00	272.0
156.90	281.0
158.80	144.0
160.70	118.0
171.00	327.0
171.90	1451.0
173.90	84456.0
175.00	7394.0
175.90	81632.0
177.00	5444.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
36.00	901.0
37.00	5093.0
38.00	4391.0
39.00	1891.0
40.00	263.0
40.90	110.0
41.30	146.0
41.80	187.0
42.90	166.0
44.00	894.0
45.00	938.0
46.00	258.0
47.00	1039.0
48.00	694.0
49.00	4013.0
50.00	18336.0
51.00	5966.0
52.00	331.0
52.90	164.0
54.10	153.0
54.90	326.0
55.90	1676.0
57.00	2527.0
59.90	1027.0
61.00	5251.0
62.00	5259.0
63.00	4132.0
63.90	553.0
65.10	1095.0
66.00	254.0
67.00	371.0
68.00	10230.0
69.00	11232.0
70.00	747.0
71.90	534.0
73.00	4837.0
74.00	16912.0
75.00	50272.0
76.10	4393.0
77.00	590.0
78.10	311.0
78.90	3674.0
79.90	936.0
80.90	3185.0
81.90	911.0
82.90	148.0
85.70	189.0
87.00	3270.0
87.90	3158.0
90.00	131.0
90.80	374.0
92.00	2763.0
93.00	4811.0
94.00	11962.0
95.00	97248.0
96.00	6161.0
96.90	208.0
97.50	128.0
103.80	520.0
104.80	151.0
105.00	155.0
105.90	521.0
107.00	124.0
109.90	160.0
111.00	162.0
112.00	172.0
112.60	152.0
114.50	204.0
116.00	413.0
116.90	787.0
117.90	635.0
118.80	569.0
124.00	122.0
127.80	505.0
128.70	151.0
129.80	376.0
130.90	224.0
134.60	238.0
135.00	234.0
135.80	109.0
137.00	192.0
138.70	127.0
139.90	178.0
140.90	1127.0
142.00	157.0
142.90	1393.0
143.80	172.0
144.80	350.0
145.90	157.0
147.80	294.0
148.70	182.0
153.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

154.90	246.0
156.90	284.0
158.80	153.0
171.00	296.0
171.80	1375.0
173.90	82808.0
175.00	7116.0
175.90	79824.0
177.00	5201.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.00	195.0
35.40	194.0
36.70	126.0
37.20	171.0
39.10	112.0
39.90	352.0
40.50	139.0
42.00	166.0
44.10	385.0
45.10	117.0
45.80	117.0
47.10	139.0
48.10	108.0
49.00	133.0
52.80	122.0
54.80	167.0
62.40	110.0
64.90	112.0
68.80	109.0
71.00	104.0
75.40	120.0
82.40	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45