




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026619.D
 Acq On : 01 Jul 2022 10:43
 Operator : SY/MD
 Sample : N3555-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA9

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:02:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

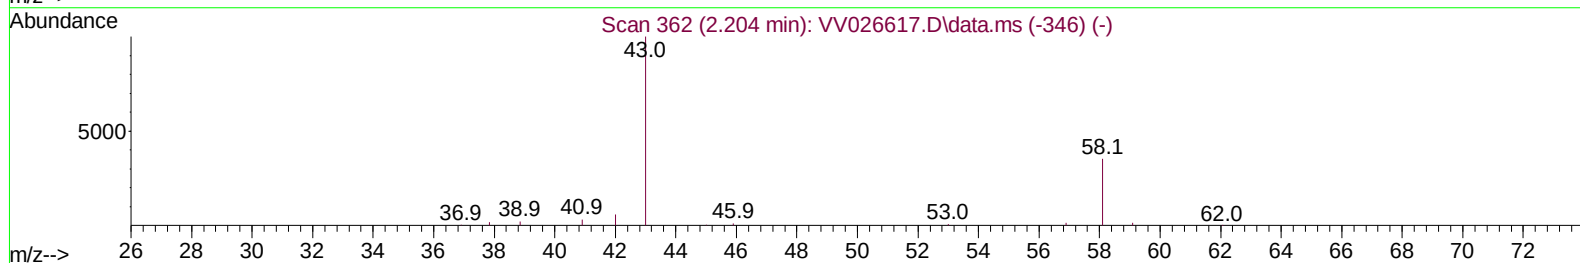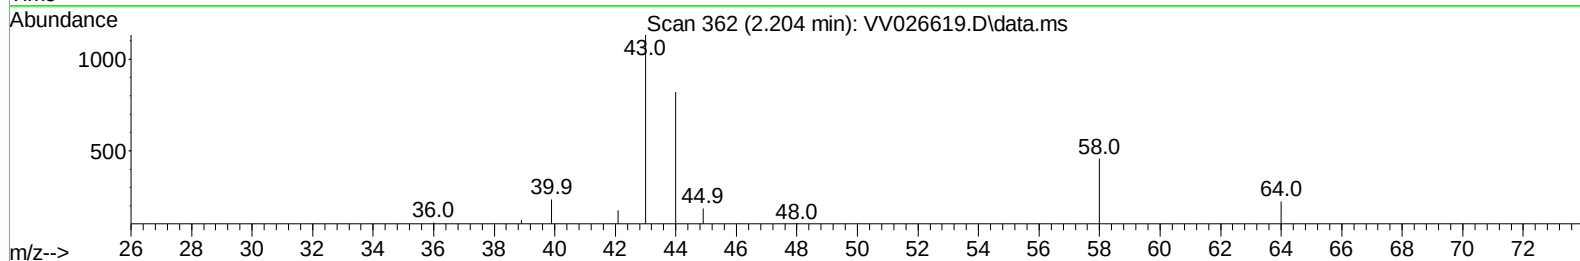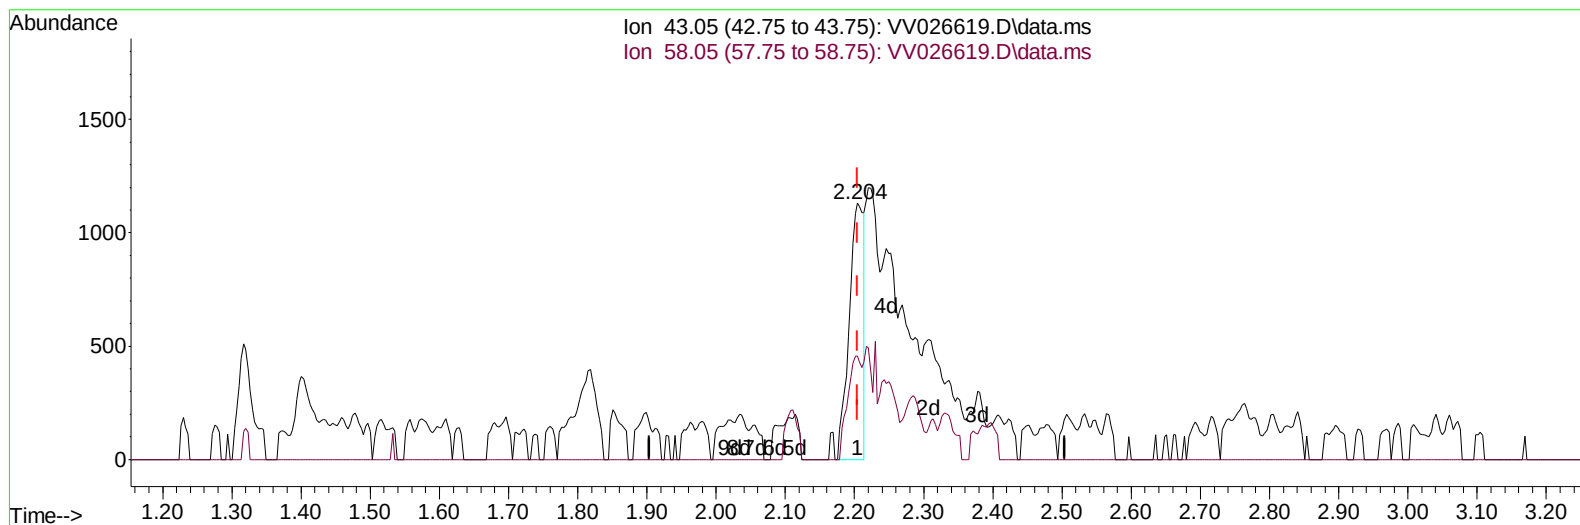

TIC: VV026619.D\data.ms

(13) Acetone (T)

2.204min (0.000) 1.68 ug/L

response 1694

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	38.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026619.D
 Acq On : 01 Jul 2022 10:43
 Operator : SY/MD
 Sample : N3555-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA9

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:02:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

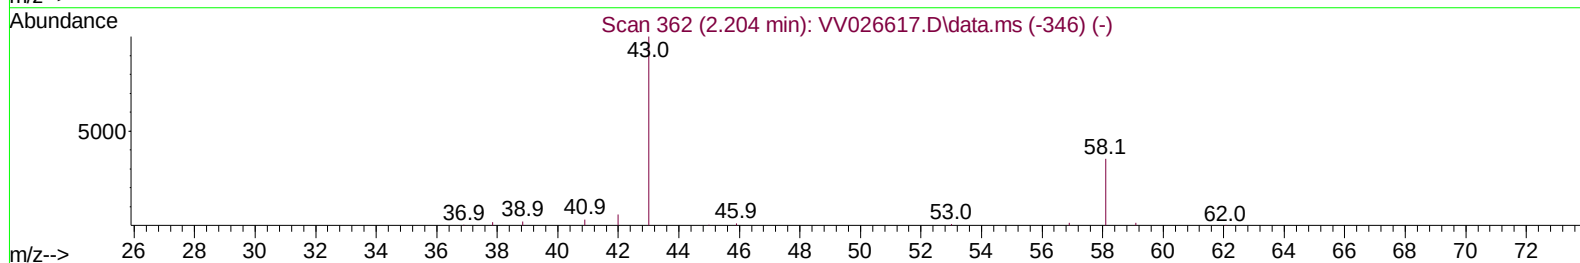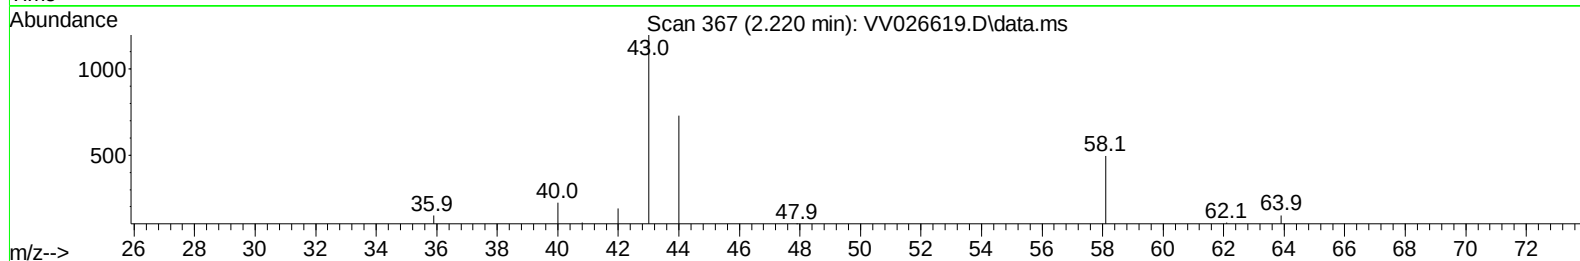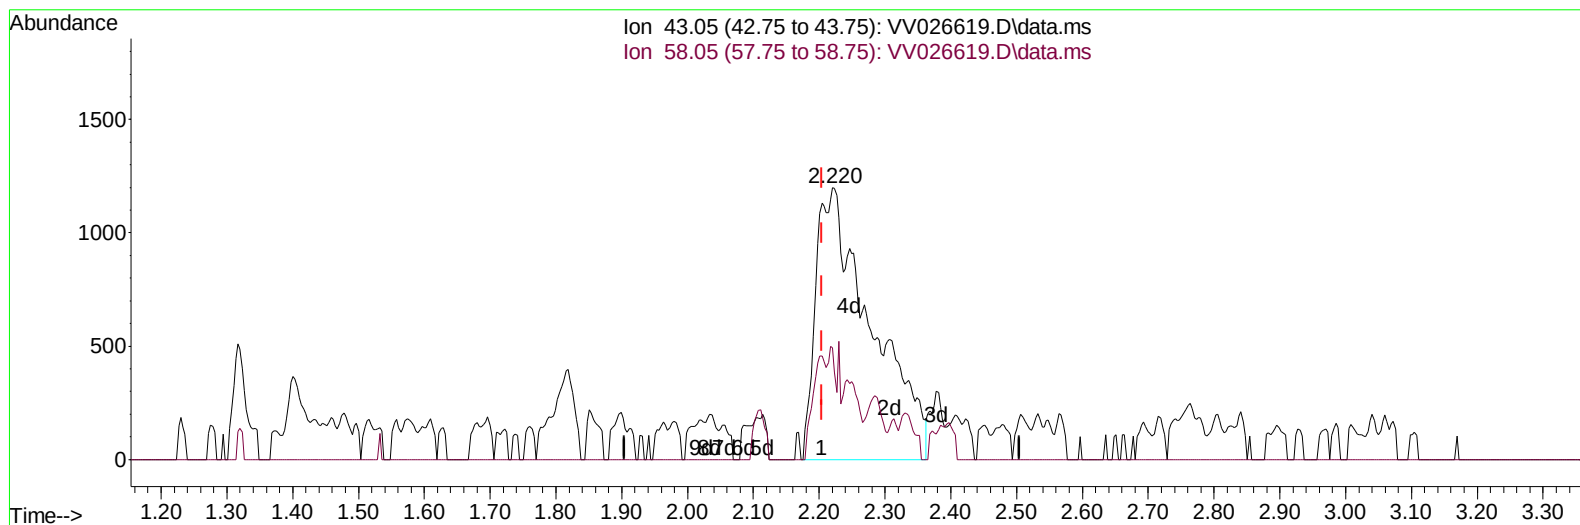

TIC: VV026619.D\data.ms

(13) Acetone (T)

2.220min (+ 0.016) 6.96 ug/L m

response 7005

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	9.31
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026619.D
 Acq On : 01 Jul 2022 10:43
 Operator : SY/MD
 Sample : N3555-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA9

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:02:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	198507	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	194193	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	78508	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	65440	4.099	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	82.000%	
7) Chloroethane-d5	1.577	69	57256	4.464	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	89.200%	
11) 1,1-Dichloroethene-d2	2.117	63	91053	3.210	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	64.200%	
20) 2-Butanone-d5	3.924	46	73497	46.307	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	92.620%	
24) Chloroform-d	4.355	84	126714	4.856	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	97.200%	
26) 1,2-Dichloroethane-d4	5.040	65	52647	5.238	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	104.800%	
32) Benzene-d6	5.056	84	229956	4.123	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	82.400%	
36) 1,2-Dichloropropane-d6	6.072	67	72992	4.759	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.200%	
41) Toluene-d8	7.316	98	182061	3.630	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	72.600%	
43) trans-1,3-Dichloroprop...	7.625	79	18318	4.620	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	92.400%	
46) 2-Hexanone-d5	8.091	63	69407	45.960	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	91.920%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49810	4.964	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	63608	4.896	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	98.000%	
Target Compounds						
13) Acetone	2.220	43	7005m	6.957	ug/L	
16) Methylene chloride	2.516	84	9862	0.693	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026619.D
Acq On : 01 Jul 2022 10:43
Operator : SY/MD
Sample : N3555-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:02:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jul 04 02:01:03 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
Supervised By :Mahesh Dadoda 07/05/2022

