




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026628.D
 Acq On : 01 Jul 2022 14:40
 Operator : SY/MD
 Sample : N3553-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COANO

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:04:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

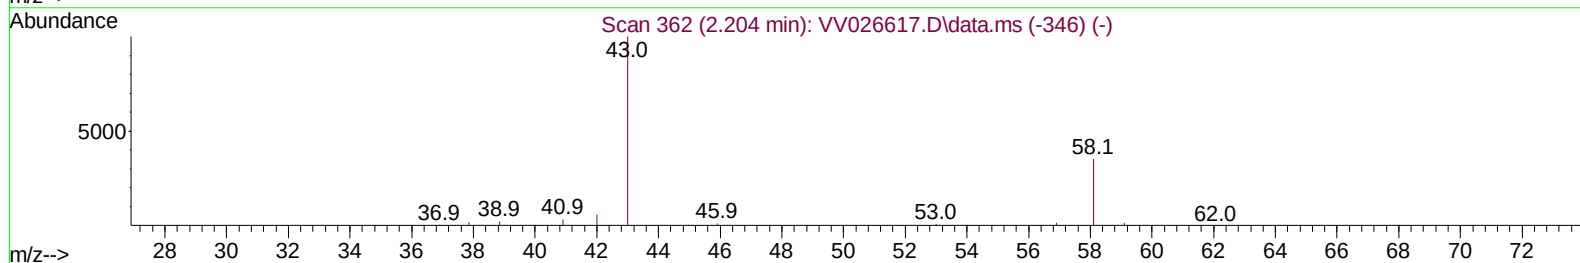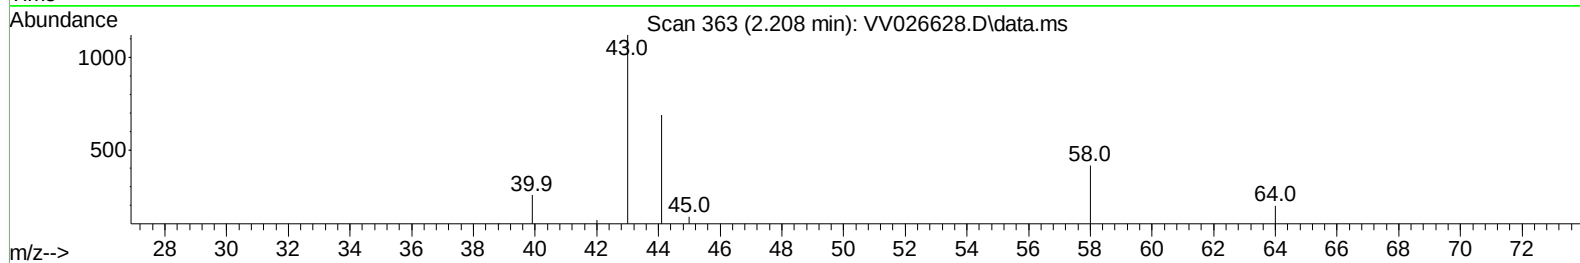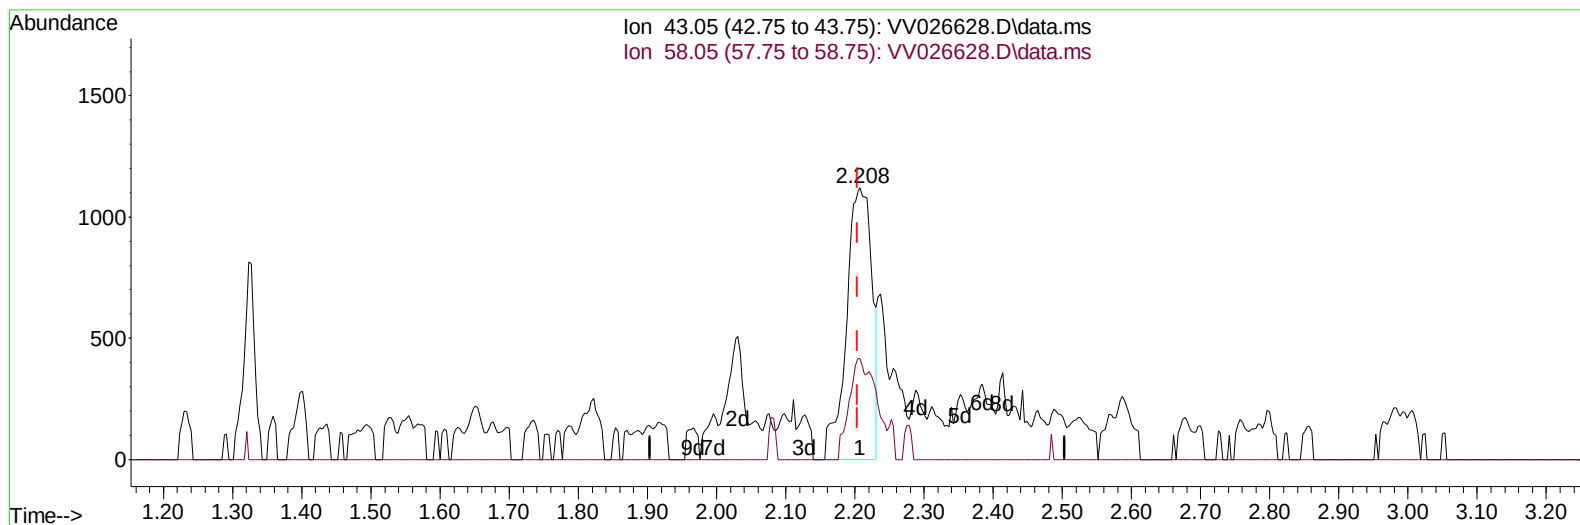

TIC: VV026628.D\data.ms

(13) Acetone (T)

2.208min (+ 0.003) 3.01 ug/L

response 2864

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	39.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026628.D
 Acq On : 01 Jul 2022 14:40
 Operator : SY/MD
 Sample : N3553-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COANO

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:04:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

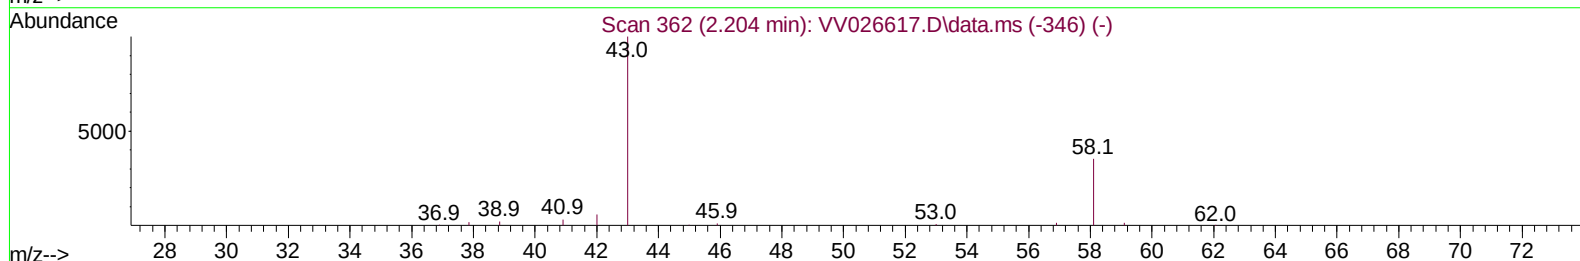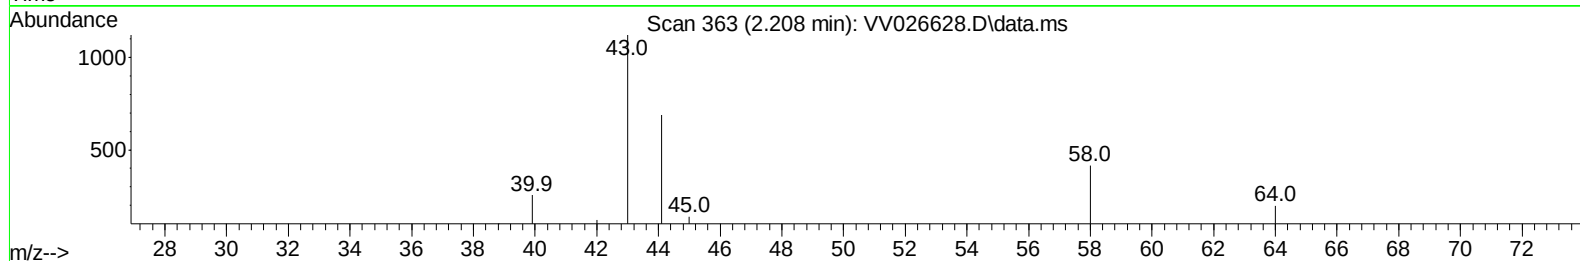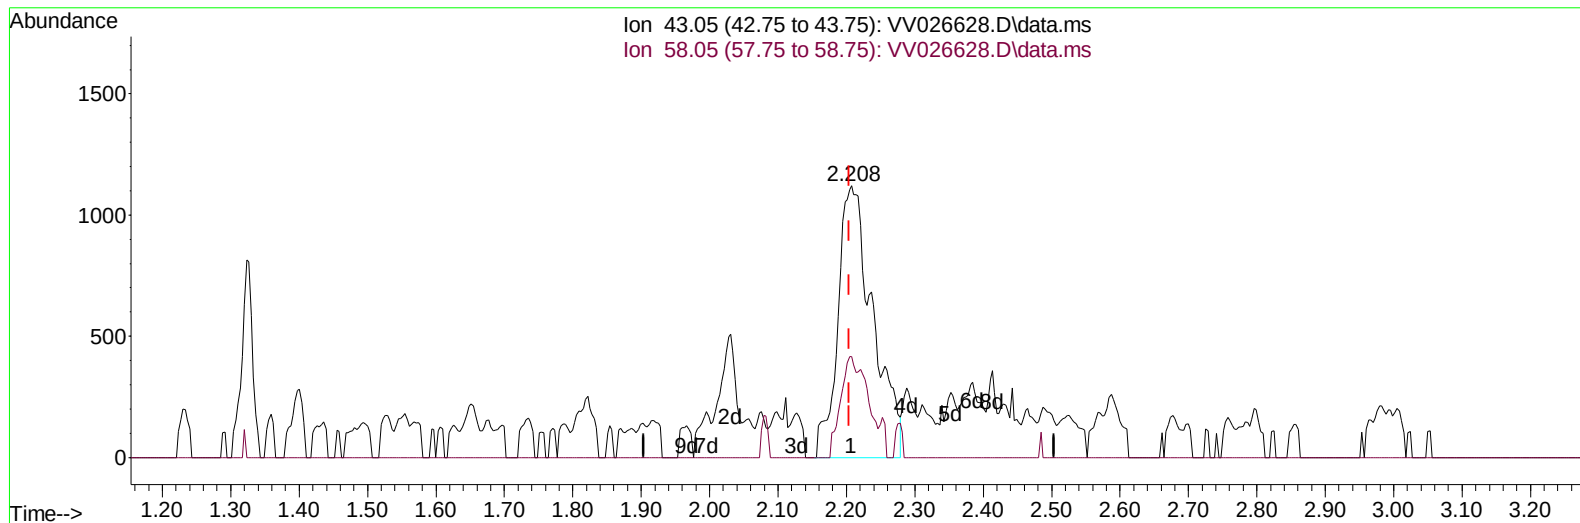

TIC: VV026628.D\data.ms

(13) Acetone (T)

2.208min (+ 0.003) 4.18 ug/L m

response 3977

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	28.29
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026628.D
 Acq On : 01 Jul 2022 14:40
 Operator : SY/MD
 Sample : N3553-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COANO

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:04:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	187791	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	181875	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75838	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	54867	3.633	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	72.600%		
7) Chloroethane-d5	1.584	69	51913	4.279	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	85.600%		
11) 1,1-Dichloroethene-d2	2.121	63	77487	2.887	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	57.800%#		
20) 2-Butanone-d5	3.918	46	98025	65.286	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	130.580%#		
24) Chloroform-d	4.365	84	127578	5.168	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	103.400%		
26) 1,2-Dichloroethane-d4	5.047	65	48910	5.144	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	102.800%		
32) Benzene-d6	5.060	84	216350	4.141	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	82.800%		
36) 1,2-Dichloropropane-d6	6.079	67	69852	4.862	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	97.200%		
41) Toluene-d8	7.320	98	166230	3.538	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	70.800%		
43) trans-1,3-Dichloroprop...	7.632	79	16707	4.499	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	90.000%		
46) 2-Hexanone-d5	8.092	63	70169	49.612	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	99.220%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49971	5.317	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	106.400%		
66) 1,2-Dichlorobenzene-d4	11.622	152	61639	4.911	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	98.200%		
Target Compounds						
						Qvalue
13) Acetone	2.208	43	3977m	4.175	ug/L	
14) Carbon disulfide	2.311	76	16991	0.508	ug/L	99
16) Methylene chloride	2.523	84	5965	0.443	ug/L	95
25) Chloroform	4.391	83	125172	5.036	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026628.D
Acq On : 01 Jul 2022 14:40
Operator : SY/MD
Sample : N3553-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
COANO

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/05/2022
Supervised By :Mahesh Dadoda 07/05/2022

Quant Time: Jul 04 02:04:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jul 04 02:01:03 2022
Response via : Initial Calibration

