




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026631.D
 Acq On : 01 Jul 2022 16:17
 Operator : SY/MD
 Sample : N3506-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

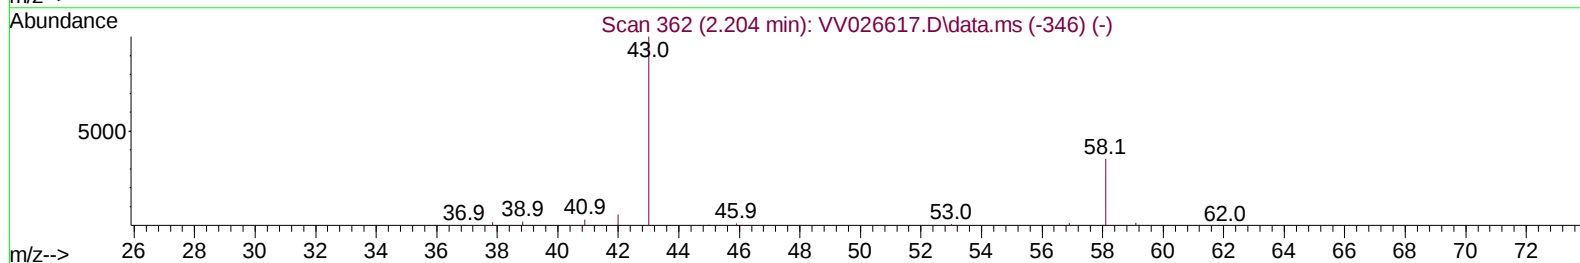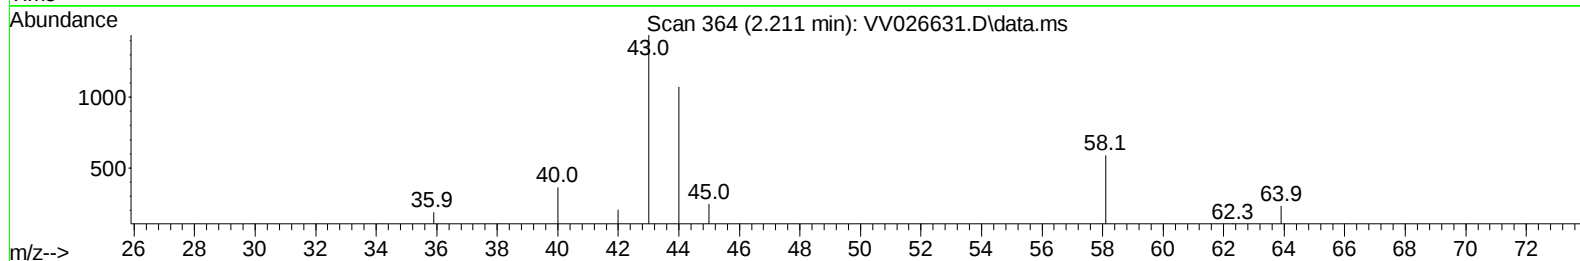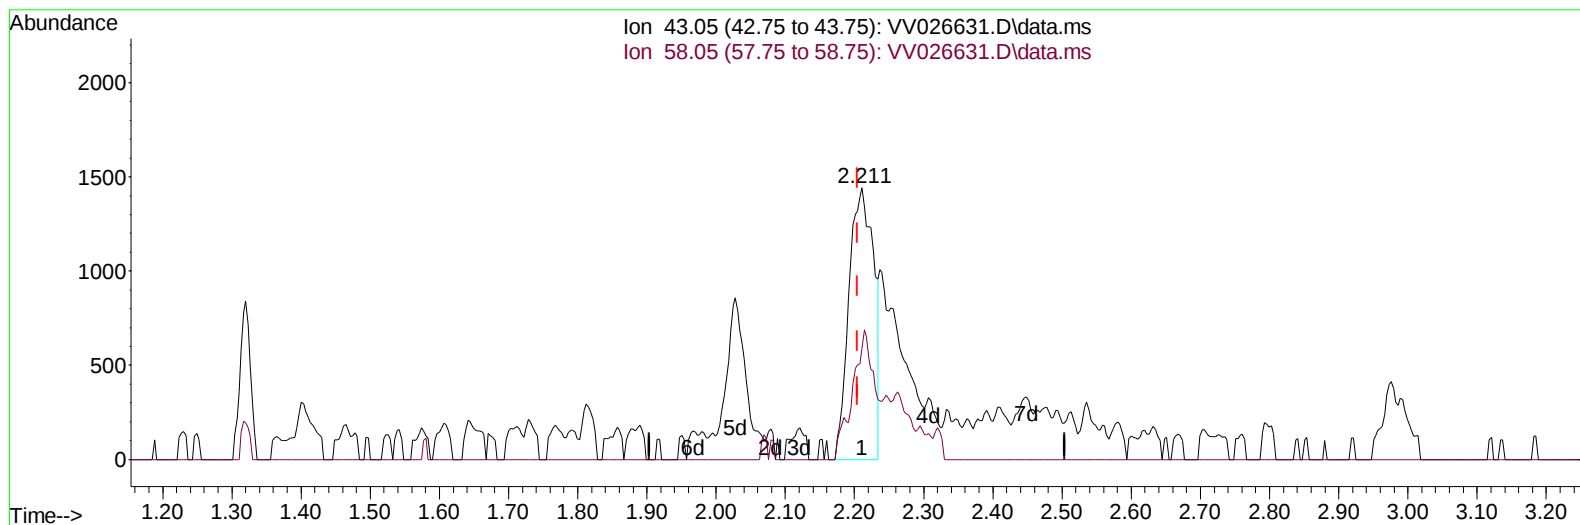

TIC: VV026631.D\data.ms

(13) Acetone (T)

2.211min (+ 0.007) 3.56 ug/L

response 3545

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	43.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026631.D
 Acq On : 01 Jul 2022 16:17
 Operator : SY/MD
 Sample : N3506-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

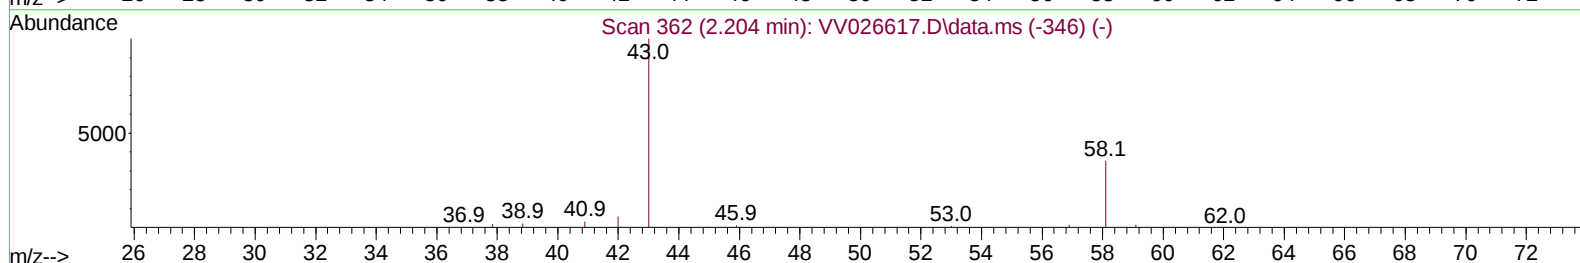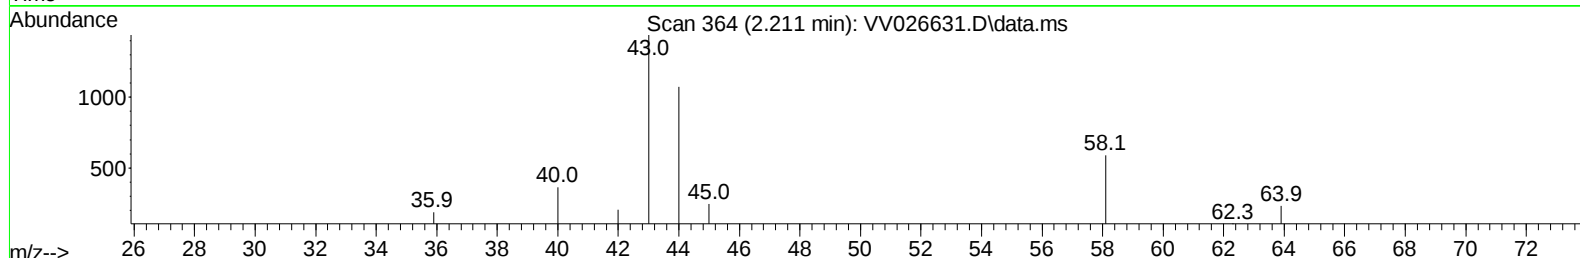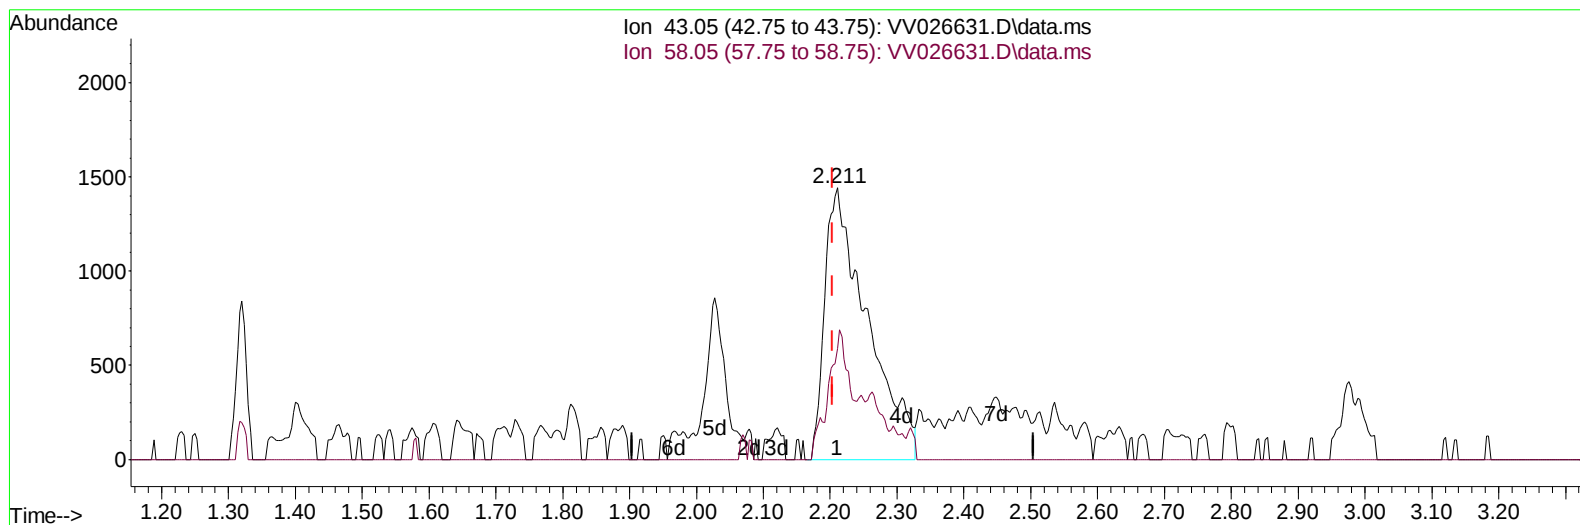

TIC: VV026631.D\data.ms

(13) Acetone (T)

2.211min (+ 0.007) 6.39 ug/L m

response 6352

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	24.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026631.D
 Acq On : 01 Jul 2022 16:17
 Operator : SY/MD
 Sample : N3506-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	196125	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	187741	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79376	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	55193	3.499	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	70.000%	
7) Chloroethane-d5	1.581	69	54653	4.313	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	86.200%	
11) 1,1-Dichloroethene-d2	2.121	63	80234	2.863	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	57.200%#	
20) 2-Butanone-d5	3.921	46	103754	66.165	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	132.320%#	
24) Chloroform-d	4.362	84	125319	4.860	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	97.200%	
26) 1,2-Dichloroethane-d4	5.047	65	51001	5.136	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	102.800%	
32) Benzene-d6	5.060	84	224070	4.155	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	83.200%	
36) 1,2-Dichloropropane-d6	6.076	67	73425	4.951	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	99.000%	
41) Toluene-d8	7.320	98	178992	3.691	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	73.800%	
43) trans-1,3-Dichloroprop...	7.629	79	18020	4.701	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	94.000%	
46) 2-Hexanone-d5	8.092	63	74229	50.842	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	101.680%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	51319	5.290	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	105.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	65592	4.993	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	99.800%	
Target Compounds						
					Qvalue	
13) Acetone	2.211	43	6352m	6.385	ug/L	
14) Carbon disulfide	2.307	76	5769	0.165	ug/L	97
25) Chloroform	4.391	83	43782	1.686	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026631.D
Acq On : 01 Jul 2022 16:17
Operator : SY/MD
Sample : N3506-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0AM5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jul 04 02:01:03 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
Supervised By :Mahesh Dadoda 07/05/2022

