




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026633.D
 Acq On : 01 Jul 2022 17:05
 Operator : SY/MD
 Sample : N3506-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM6

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

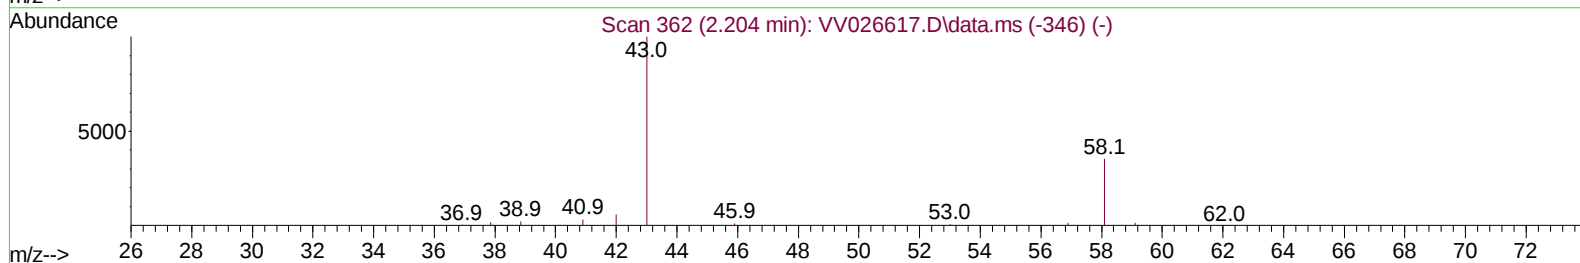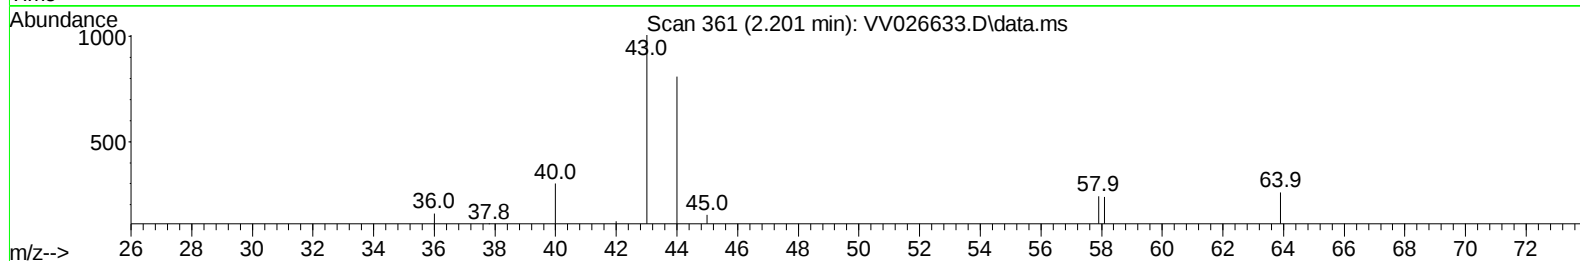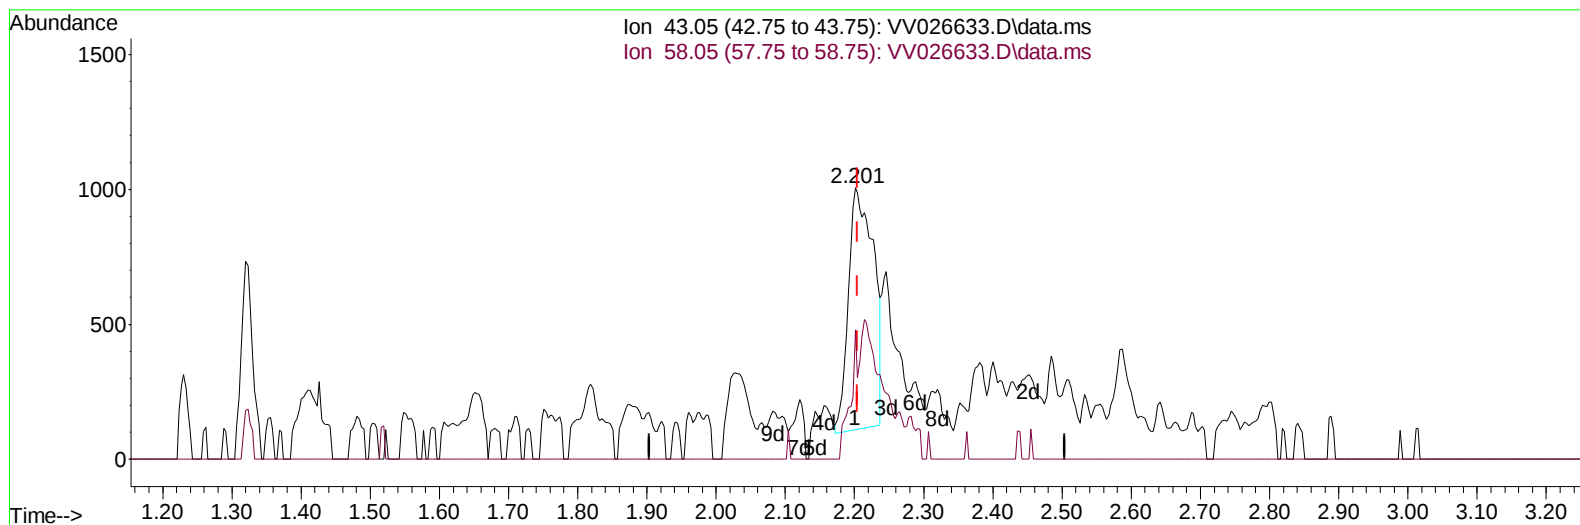

TIC: VV026633.D\data.ms

(13) Acetone (T)

2.201min (-0.003) 2.33 ug/L

response 2232

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	15.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026633.D
 Acq On : 01 Jul 2022 17:05
 Operator : SY/MD
 Sample : N3506-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM6

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

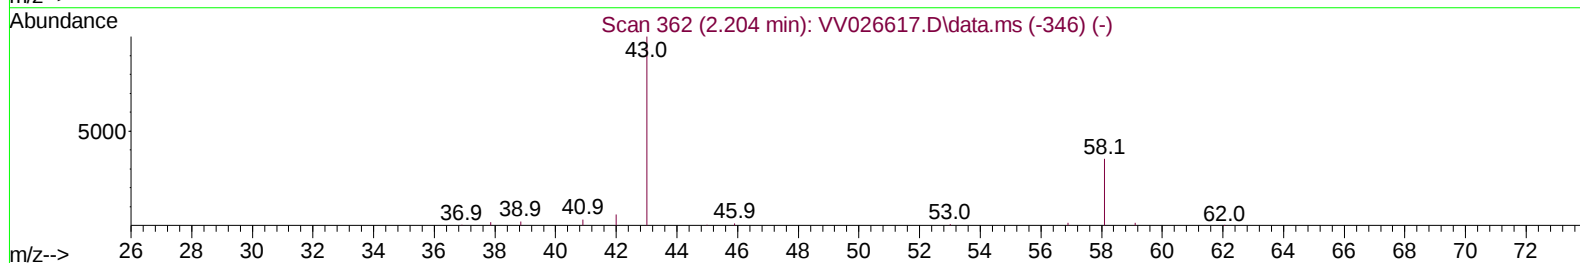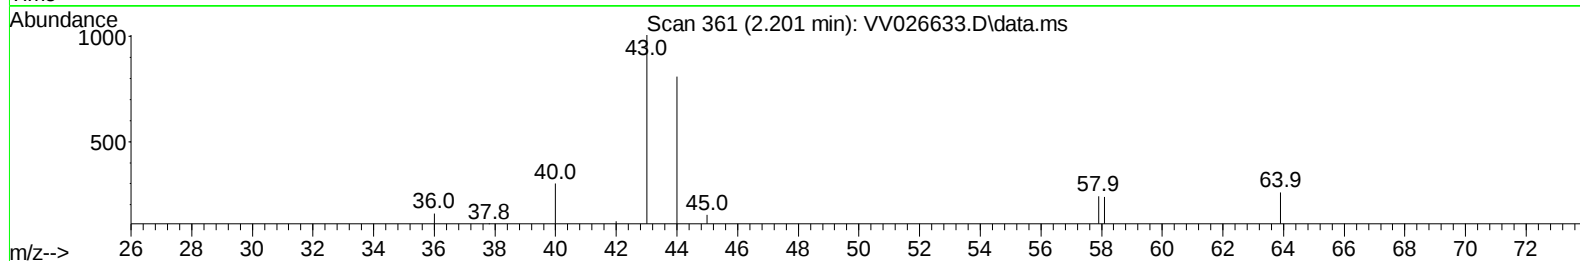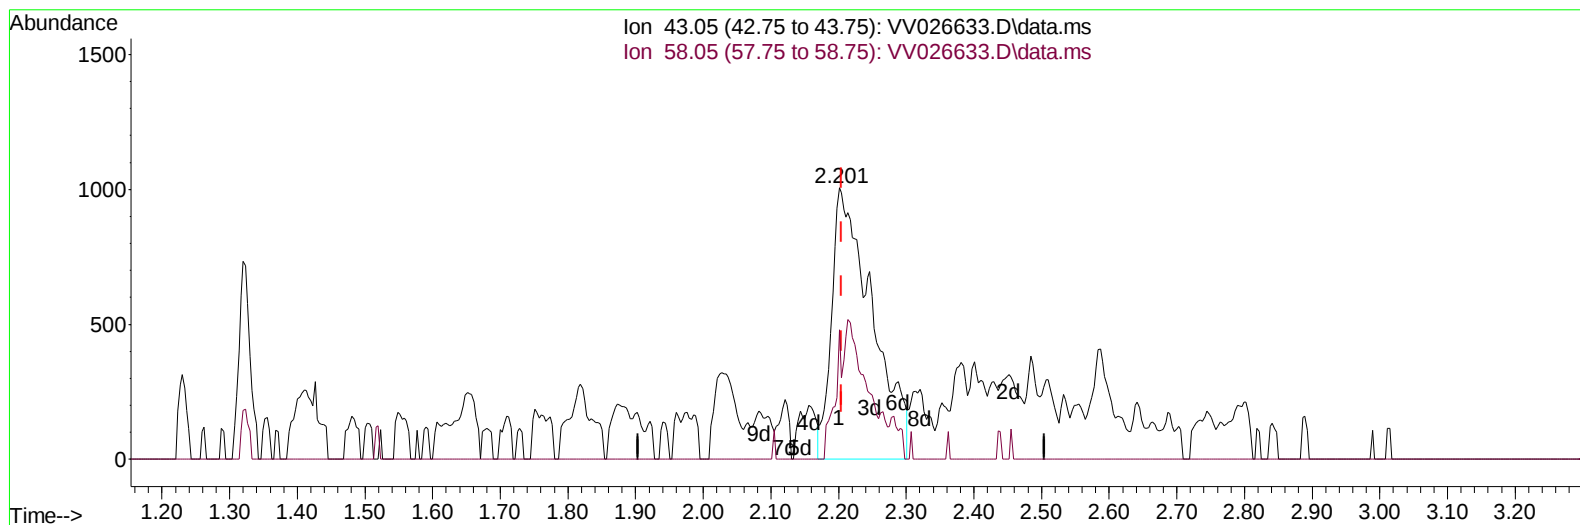

TIC: VV026633.D\data.ms

(13) Acetone (T)

2.201min (-0.003) 4.33 ug/L m

response 4150

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	8.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026633.D
 Acq On : 01 Jul 2022 17:05
 Operator : SY/MD
 Sample : N3506-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAM6

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
 Supervised By :Mahesh Dadoda 07/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	188802	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	182538	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76392	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	52763	3.475	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	69.600%	
7) Chloroethane-d5	1.584	69	49952	4.095	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	82.000%	
11) 1,1-Dichloroethene-d2	2.121	63	76952	2.852	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	57.000%#	
20) 2-Butanone-d5	3.921	46	103088	68.290	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	136.580%#	
24) Chloroform-d	4.365	84	122496	4.935	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	98.800%	
26) 1,2-Dichloroethane-d4	5.047	65	48429	5.066	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	101.400%	
32) Benzene-d6	5.063	84	209617	3.998	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	80.000%	
36) 1,2-Dichloropropane-d6	6.079	67	68988	4.785	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.600%	
41) Toluene-d8	7.323	98	161119	3.417	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	68.400%#	
43) trans-1,3-Dichloroprop...	7.632	79	16068	4.311	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	86.200%	
46) 2-Hexanone-d5	8.095	63	71154	50.125	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	100.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49404	5.238	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	104.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	61024	4.827	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	96.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.201	43	4150m	4.333	ug/L	
14) Carbon disulfide	2.310	76	19236	0.572	ug/L	98
16) Methylene chloride	2.523	84	6217	0.459	ug/L	91
25) Chloroform	4.391	83	134137	5.367	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026633.D
Acq On : 01 Jul 2022 17:05
Operator : SY/MD
Sample : N3506-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM6

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:05:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jul 04 02:01:03 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/05/2022
Supervised By :Mahesh Dadoda 07/05/2022

