

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026618.D
 Acq On : 01 Jul 2022 10:10
 Operator : SY/MD
 Sample : VV0701WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK387

Quant Time: Jul 04 02:02:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jul 04 02:01:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	192209	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	189256	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76086	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	64329	4.162	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	83.200%	
7) Chloroethane-d5	1.580	69	57703	4.647	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	2.121	63	89532	3.260	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.200%	
20) 2-Butanone-d5	3.912	46	61134	39.780	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	79.560%	
24) Chloroform-d	4.359	84	125830	4.980	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.600%	
26) 1,2-Dichloroethane-d4	5.040	65	52573	5.402	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.000%	
32) Benzene-d6	5.056	84	231337	4.256	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.200%	
36) 1,2-Dichloropropane-d6	6.072	67	72911	4.877	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.600%	
41) Toluene-d8	7.317	98	177194	3.625	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	72.400%	
43) trans-1,3-Dichloroprop...	7.628	79	17935	4.642	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.800%	
46) 2-Hexanone-d5	8.091	63	72403	49.195	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.380%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	52726	5.392	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	107.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	63057	5.008	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.523	84	3568	0.259	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026618.D
Acq On : 01 Jul 2022 10:10
Operator : SY/MD
Sample : VV0701WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK387


Quant Time: Jul 04 02:02:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jul 04 02:01:03 2022
Response via : Initial Calibration

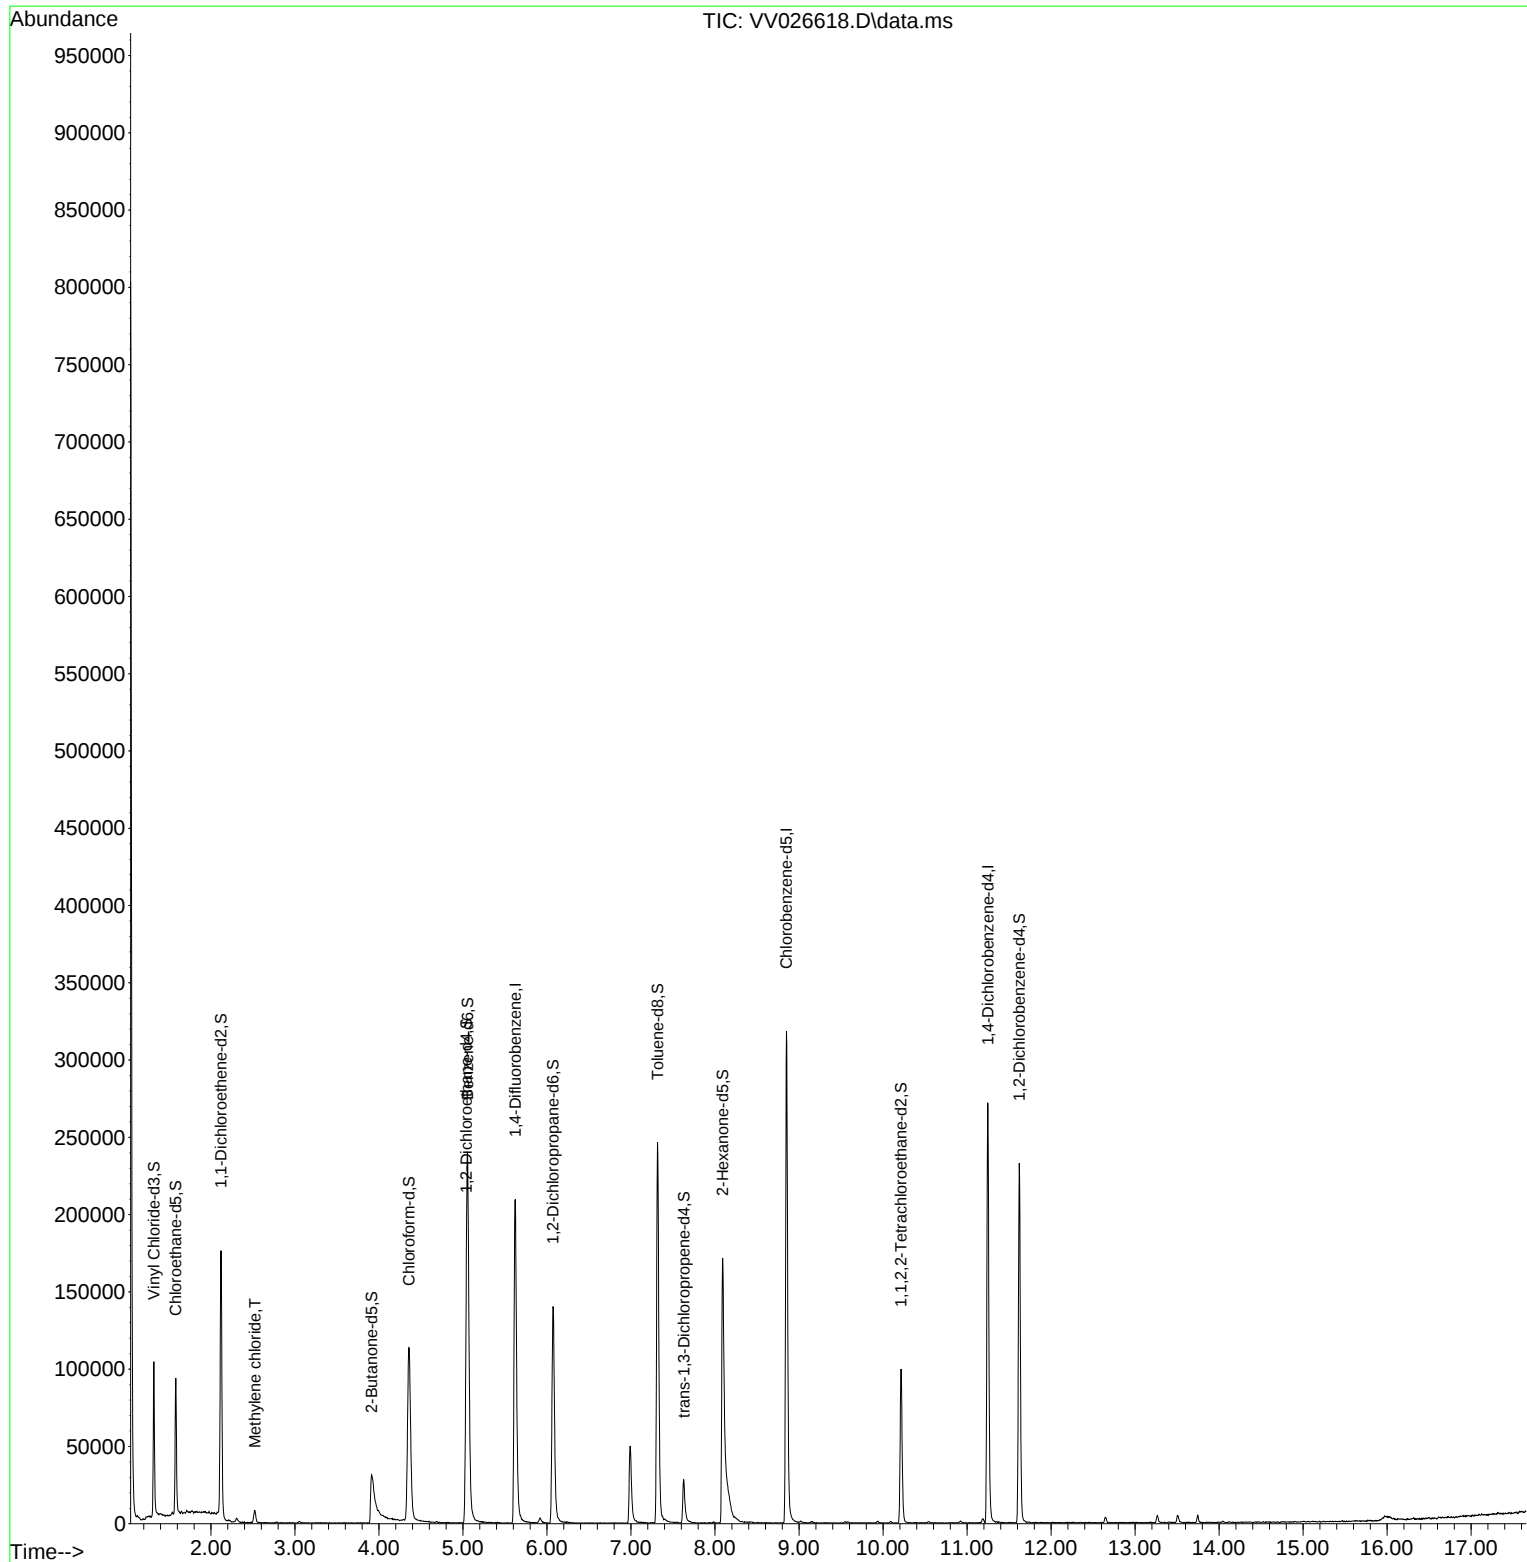

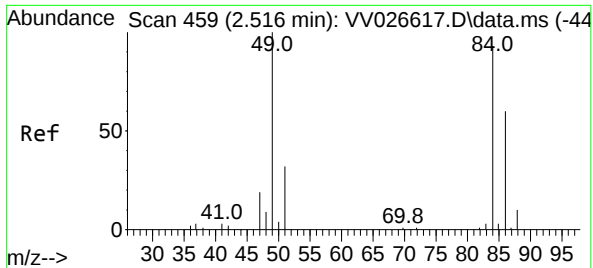

#16
Methylene chloride
Concen: 0.259 ug/L
RT: 2.523 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV026618.D
Acq: 01 Jul 2022 10:10

Instrument :
MSVOA_V
ClientSampleId :
VBLK387

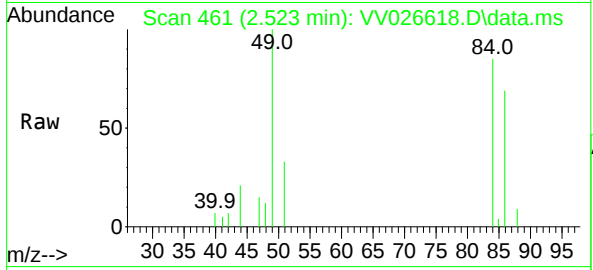

Tgt Ion: 84 Resp: 3568

Ion	Ratio	Lower	Upper
84	100		
86	81.5	46.0	85.4
49	117.3	77.7	144.3

