

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026618.D
 Acq On : 01 Jul 2022 10:10
 Operator : SY/MD
 Sample : VV0701WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK387

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	99	rBV	100193	104237	17.48%	2.202%
2	1.580	160	168	185	rBV	88261	103721	17.39%	2.192%
3	2.121	326	336	354	rVB	174560	258027	43.27%	5.452%
4	2.523	450	461	472	rBV3	8082	14227	2.39%	0.301%
5	3.912	884	893	917	rBV	31134	107230	17.98%	2.266%
6	4.355	1015	1031	1057	rBV	111628	284925	47.78%	6.020%
7	5.053	1230	1248	1282	rBV2	240170	596361	100.00%	12.601%
8	5.622	1412	1425	1453	rBV	209503	434070	72.79%	9.171%
9	6.072	1552	1565	1596	rBV	140240	294620	49.40%	6.225%
10	6.989	1839	1850	1871	rBV	50015	97622	16.37%	2.063%
11	7.317	1941	1952	1969	rBV	246356	440484	73.86%	9.307%
12	7.625	2039	2048	2070	rBV2	27781	52171	8.75%	1.102%
13	8.091	2183	2193	2234	rBV2	171526	431765	72.40%	9.123%
14	8.850	2418	2429	2462	rBV	317958	530589	88.97%	11.211%
15	10.214	2842	2853	2872	rBV	99543	164730	27.62%	3.481%
16	11.246	3164	3174	3195	rBV	271720	433808	72.74%	9.166%
17	11.622	3279	3291	3318	rBV	232806	376309	63.10%	7.951%
18	13.509	3866	3878	3886	rBV	4643	7935	1.33%	0.168%




Sum of corrected areas: 4732831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026618.D
Acq On : 01 Jul 2022 10:10
Operator : SY/MD
Sample : VV0701WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

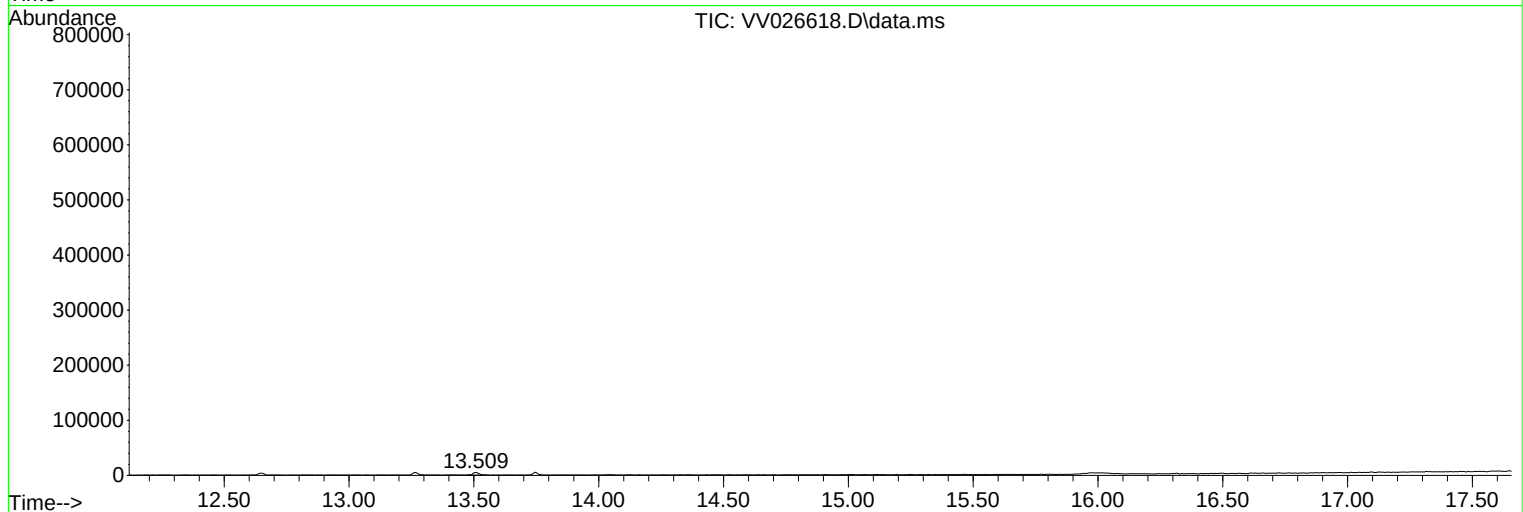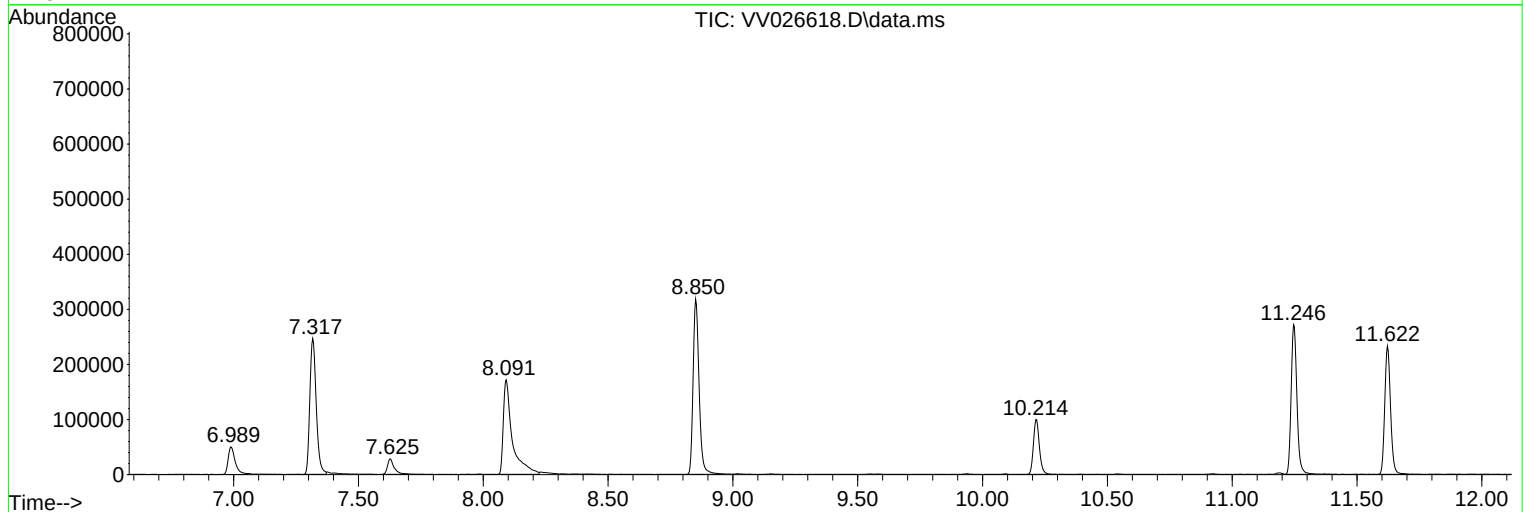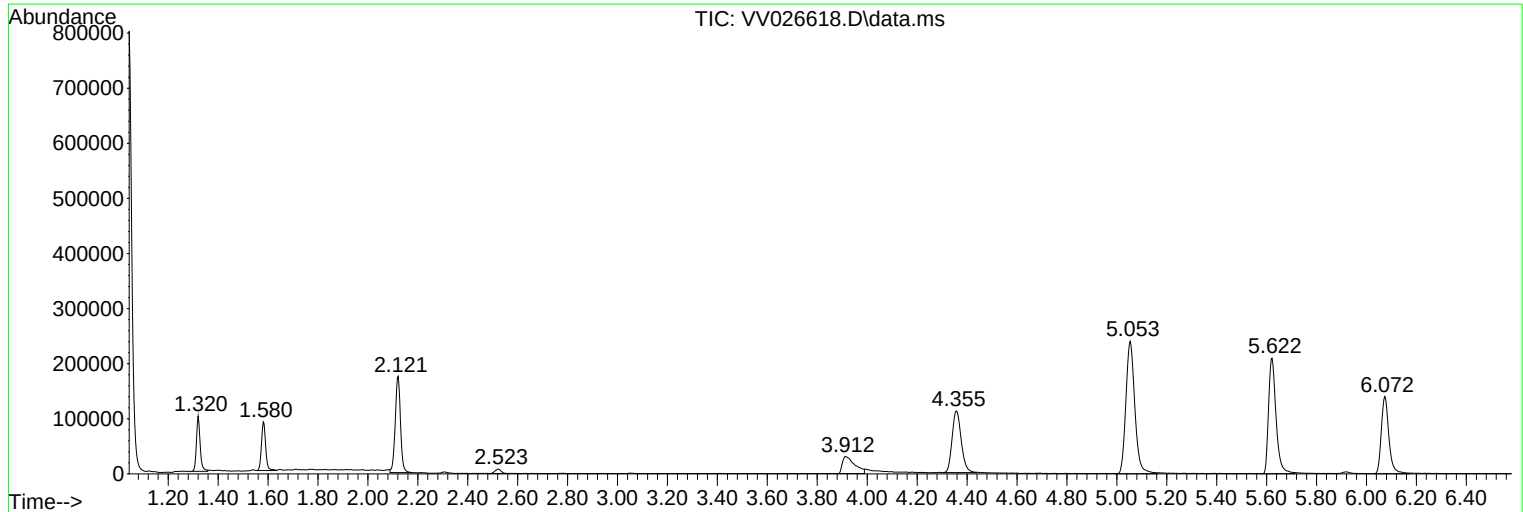

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026618.D
Acq On : 01 Jul 2022 10:10
Operator : SY/MD
Sample : VV0701WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026618.D
Acq On : 01 Jul 2022 10:10
Operator : SY/MD
Sample : VV0701WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc