

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026619.D
 Acq On : 01 Jul 2022 10:43
 Operator : SY/MD
 Sample : N3555-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	35	rVB2	21872	19911	3.36%	0.413%
2	1.317	79	86	99	rBV	97339	104419	17.61%	2.168%
3	1.577	160	167	181	rVB	88092	101946	17.19%	2.117%
4	2.117	325	335	349	rVB	175684	258265	43.56%	5.363%
5	2.516	449	459	472	rBV	21927	36652	6.18%	0.761%
6	3.924	886	897	936	rBV2	27565	135591	22.87%	2.816%
7	4.355	1015	1031	1056	rBV	116574	293411	49.49%	6.093%
8	5.053	1232	1248	1283	rBV2	239138	592901	100.00%	12.312%
9	5.622	1413	1425	1456	rBV	216662	445270	75.10%	9.246%
10	6.072	1552	1565	1591	rBV	139869	295173	49.78%	6.129%
11	6.989	1840	1850	1879	rBV	49842	97669	16.47%	2.028%
12	7.317	1940	1952	1974	rBV	255338	450353	75.96%	9.352%
13	7.628	2039	2049	2070	rBV	27005	51494	8.69%	1.069%
14	8.091	2180	2193	2230	rBV2	174717	415465	70.07%	8.627%
15	8.850	2418	2429	2454	rBV	324713	544567	91.85%	11.308%
16	10.217	2842	2854	2874	rBV	100415	160503	27.07%	3.333%
17	10.384	2896	2906	2921	rVB4	4090	6834	1.15%	0.142%
18	11.249	3164	3175	3193	rBV	276615	441220	74.42%	9.162%
19	11.622	3280	3291	3309	rBV	228253	364042	61.40%	7.560%




Sum of corrected areas: 4815686

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026619.D
Acq On : 01 Jul 2022 10:43
Operator : SY/MD
Sample : N3555-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

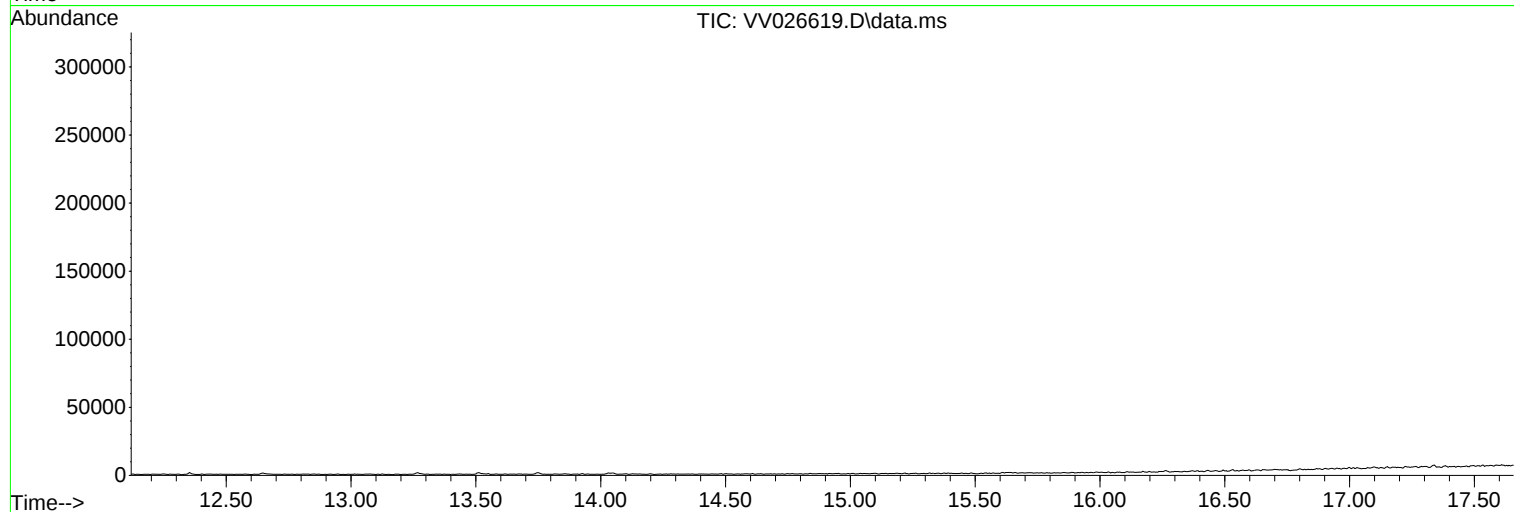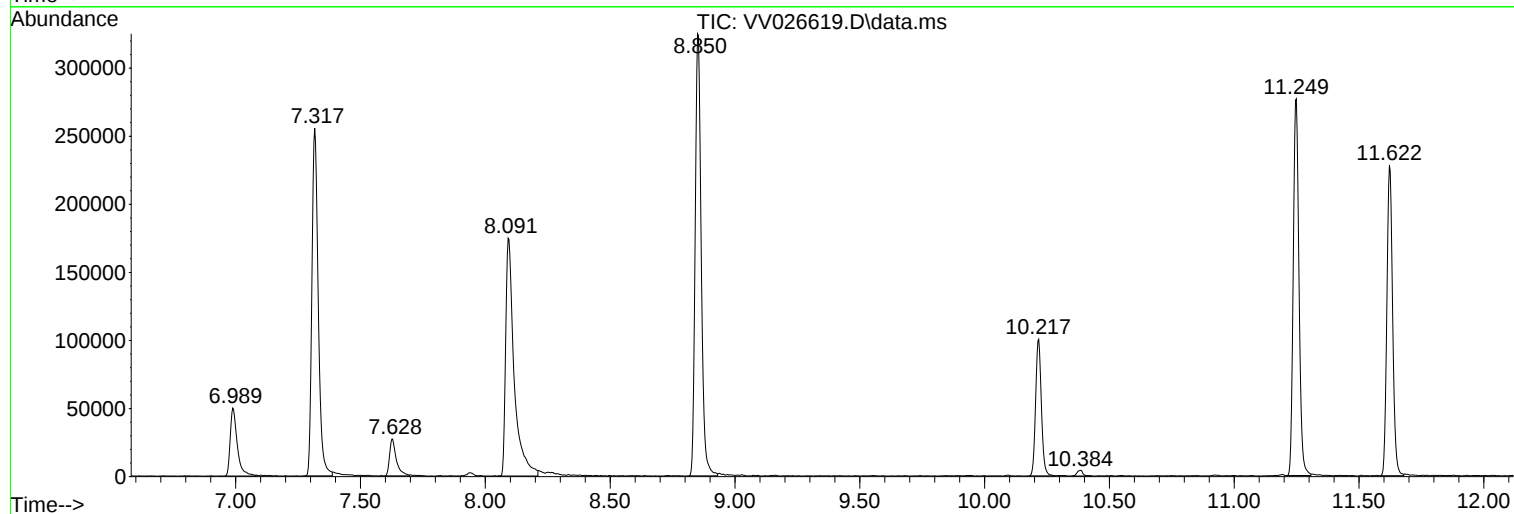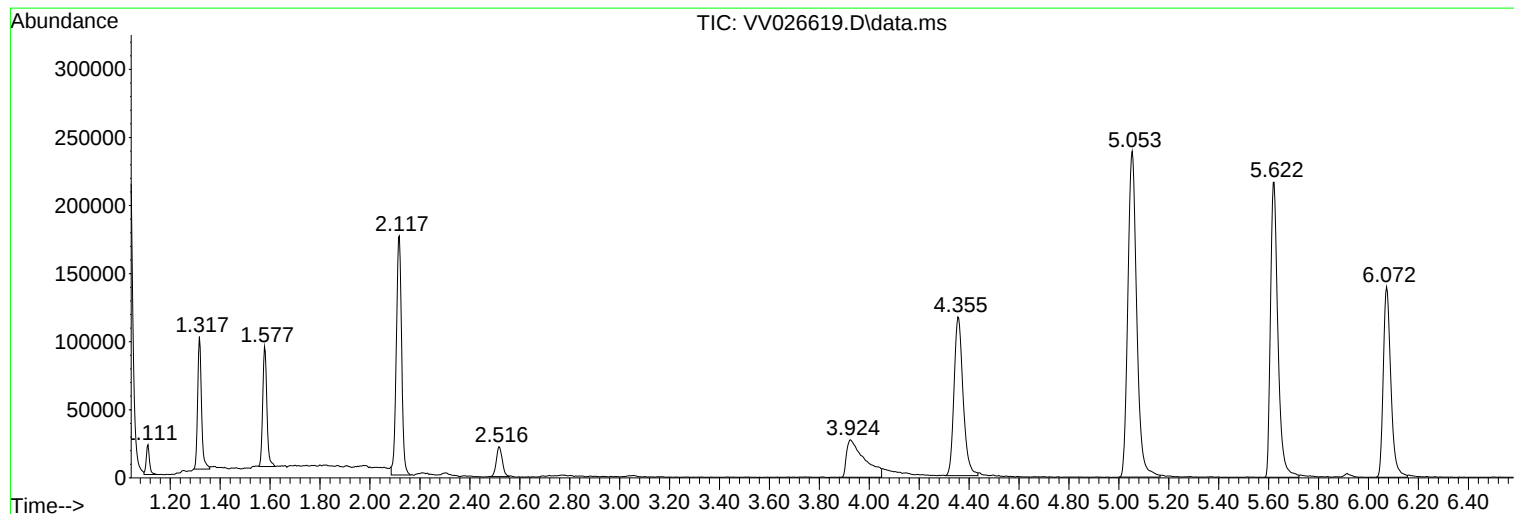

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026619.D
Acq On : 01 Jul 2022 10:43
Operator : SY/MD
Sample : N3555-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026619.D
Acq On : 01 Jul 2022 10:43
Operator : SY/MD
Sample : N3555-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
