

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026628.D
 Acq On : 01 Jul 2022 14:40
 Operator : SY/MD
 Sample : N3553-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COANO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	78	87	104	rBV	80580	98858	17.24%	2.010%
2	1.584	162	169	180	rBV	79288	92976	16.22%	1.891%
3	2.121	327	336	350	rVB	148884	217321	37.91%	4.419%
4	2.307	386	394	405	rBV	14022	20661	3.60%	0.420%
5	2.523	450	461	472	rBV2	13276	22434	3.91%	0.456%
6	2.593	472	483	496	rVB2	14718	26783	4.67%	0.545%
7	3.918	885	895	940	rBV	45048	172011	30.00%	3.498%
8	4.375	1016	1037	1073	rBV4	164640	573297	100.00%	11.657%
9	5.060	1234	1250	1279	rBV3	224486	556397	97.05%	11.314%
10	5.625	1415	1426	1454	rBV	205690	418845	73.06%	8.517%
11	6.079	1554	1567	1593	rBV	134502	281211	49.05%	5.718%
12	6.587	1713	1725	1738	rBV6	5020	12384	2.16%	0.252%
13	6.995	1839	1852	1873	rBV	47023	89419	15.60%	1.818%
14	7.143	1888	1898	1912	rVB5	4606	9288	1.62%	0.189%
15	7.320	1940	1953	1973	rBV	237293	417003	72.74%	8.479%
16	7.632	2039	2050	2067	rBV2	25546	46848	8.17%	0.953%
17	8.095	2183	2194	2235	rBV2	202503	427582	74.58%	8.694%
18	8.854	2419	2430	2454	rBV	305393	502282	87.61%	10.213%
19	10.217	2842	2854	2870	rBV	99161	158308	27.61%	3.219%
20	11.249	3164	3175	3193	rBV	273601	419210	73.12%	8.524%
21	11.622	3279	3291	3313	rBV	224907	354807	61.89%	7.215%




Sum of corrected areas: 4917925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026628.D
Acq On : 01 Jul 2022 14:40
Operator : SY/MD
Sample : N3553-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COANO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

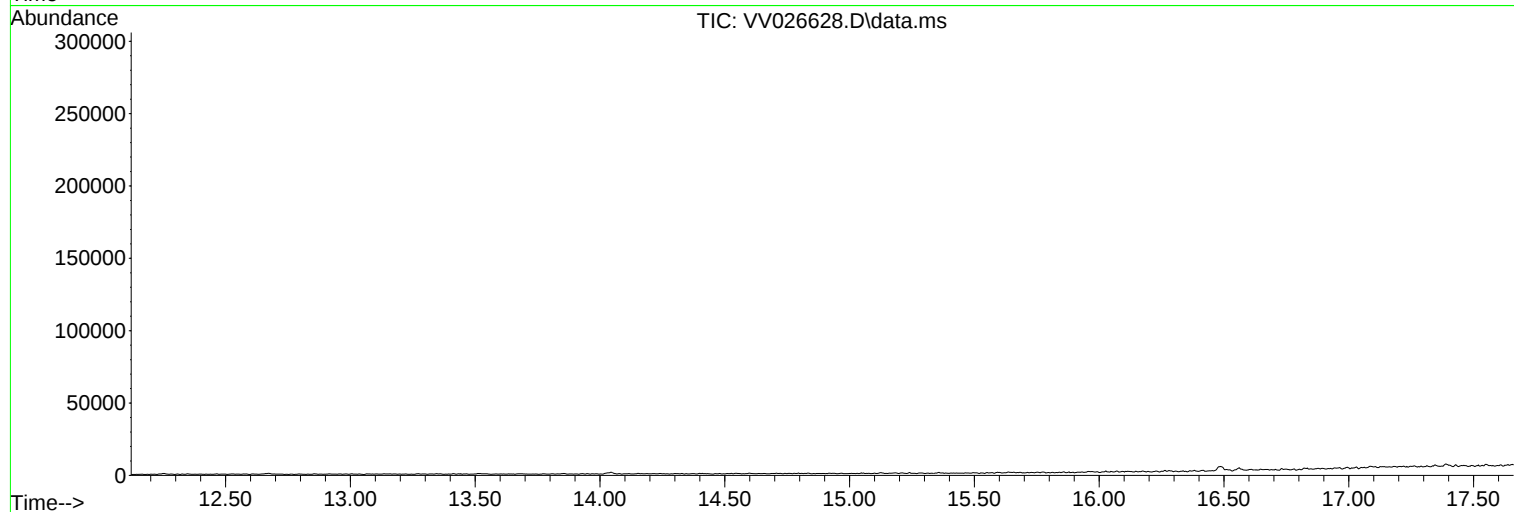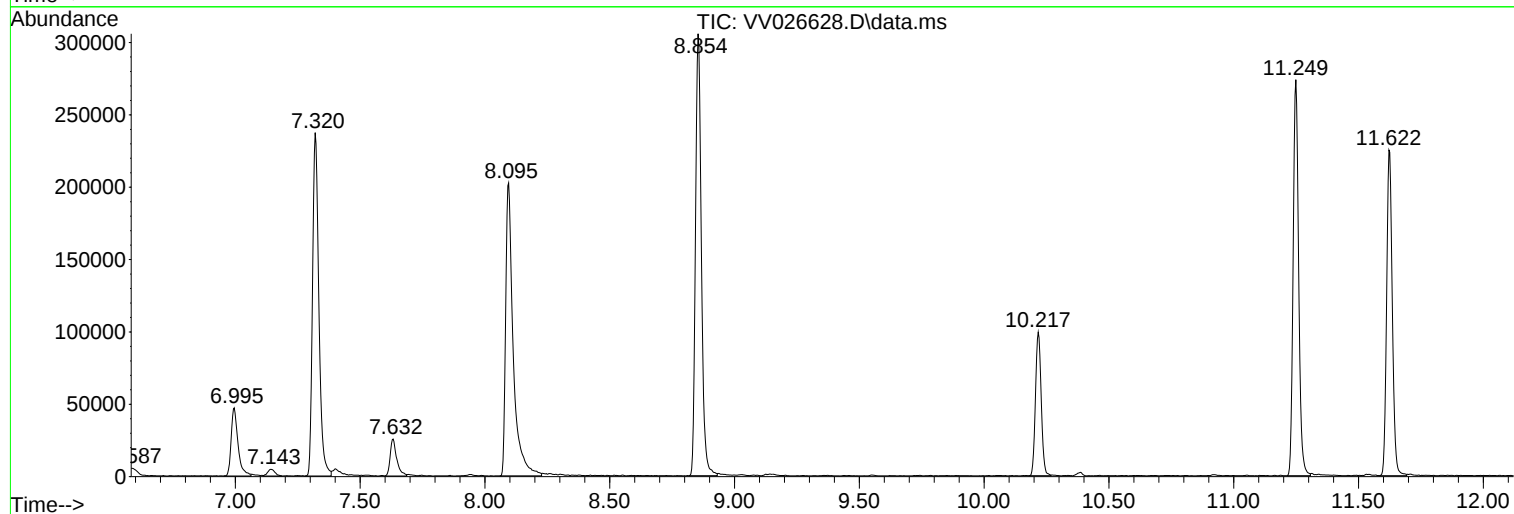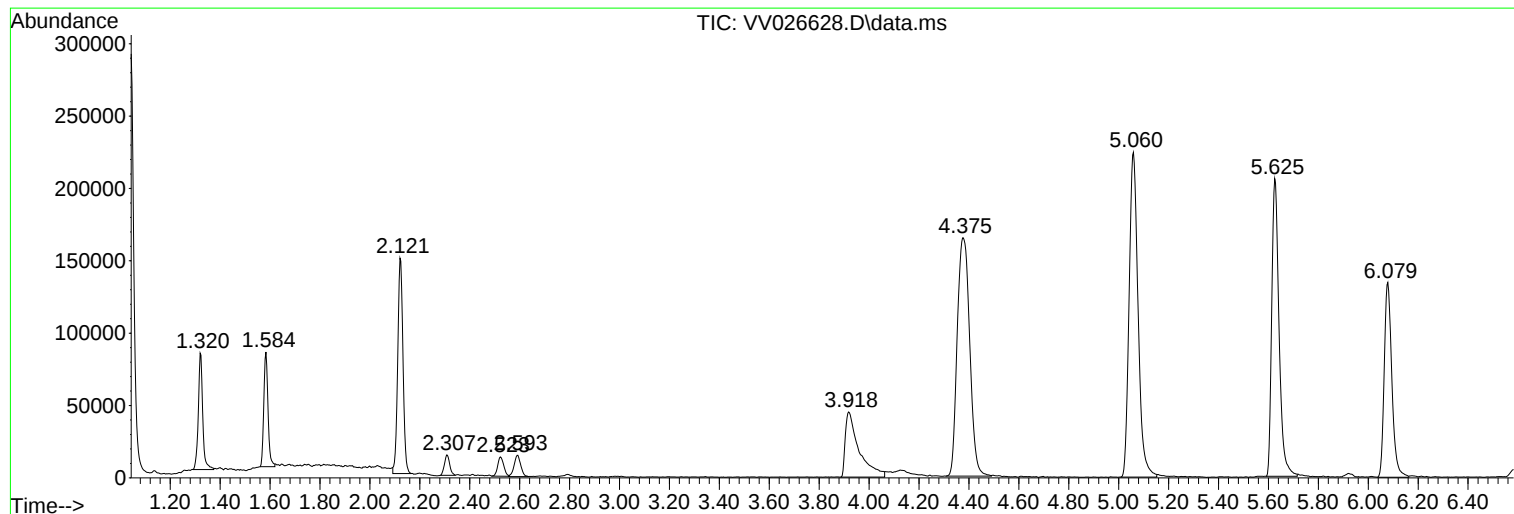

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026628.D
Acq On : 01 Jul 2022 14:40
Operator : SY/MD
Sample : N3553-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
Data File : VV026628.D
Acq On : 01 Jul 2022 14:40
Operator : SY/MD
Sample : N3553-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COANO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc