
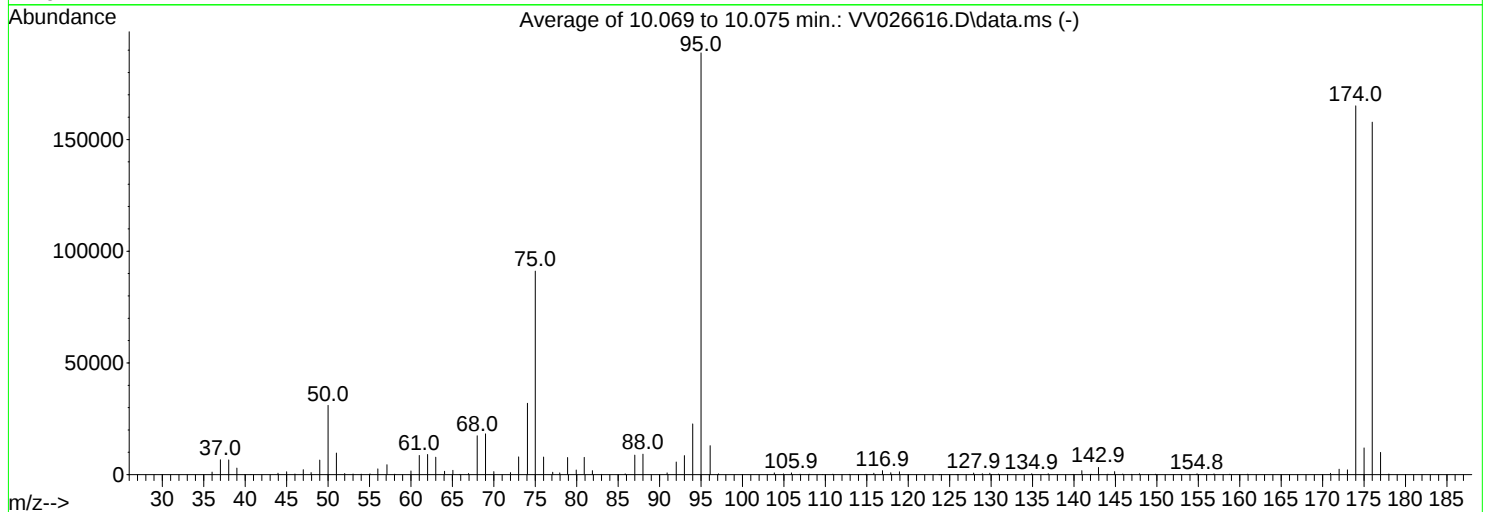


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070122\
 Data File : VV026616.D
 Acq On : 01 Jul 2022 08:51
 Operator : SY/MD
 Sample : BFB337
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB337

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jul 04 02:01:03 2022

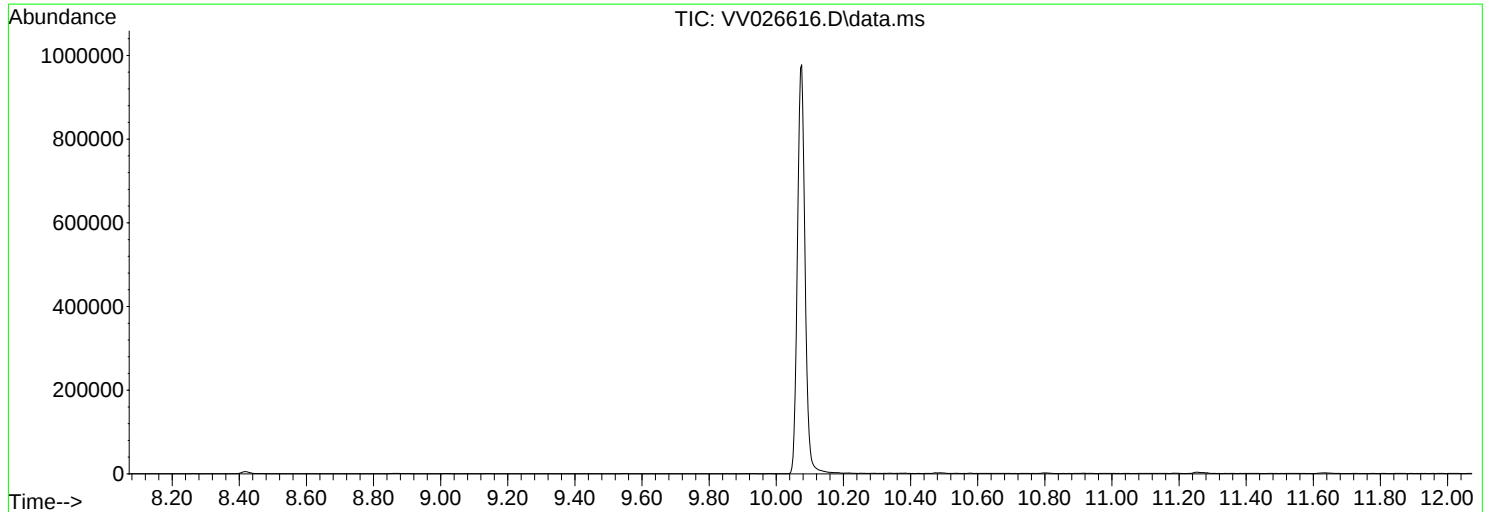

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	31008	PASS
75	95	30	80	48.3	91141	PASS
95	95	100	100	100.0	188800	PASS
96	95	5	9	6.9	12939	PASS
173	174	0.00	2	1.3	2131	PASS
174	95	50	120	87.4	165099	PASS
175	174	5	9	7.3	11977	PASS
176	174	95	105	95.6	157803	PASS
177	176	5	10	6.3	9984	PASS

m/z	Abundance
40.00	184.0
43.90	453.0

Instrument :
MSVOA_V
ClientSampleId :
BFB337

m/z	Abundance
36.00	1104.0
37.00	6111.0
38.00	6104.0
39.00	2786.0
39.90	282.0
40.70	144.0
44.00	948.0
45.00	1213.0
46.00	271.0
47.00	2079.0
47.90	933.0
49.00	6064.0
50.00	29360.0
51.00	9228.0
52.00	503.0
53.00	294.0
54.00	210.0
55.10	414.0
56.00	2394.0
57.10	4304.0
58.00	199.0
60.00	1730.0
61.00	8013.0
62.00	8555.0
63.00	7314.0
64.00	1568.0
65.00	1910.0
65.90	160.0
67.00	480.0
68.00	16432.0
69.00	16992.0
70.00	1210.0
72.00	954.0
73.00	7230.0
74.00	29576.0
75.00	84648.0
76.00	7517.0
77.10	1024.0
78.00	654.0
78.90	7069.0
79.90	1874.0
80.90	7314.0
81.90	1675.0
82.90	116.0
85.90	323.0
87.00	8149.0
88.00	8523.0
90.90	718.0
92.00	5420.0
93.00	7972.0
94.00	21064.0
95.00	176000.0
96.10	12416.0
97.10	385.0
103.80	789.0
104.90	316.0
105.90	777.0
106.90	242.0
108.00	233.0
110.90	185.0
113.00	166.0
114.90	175.0
115.80	656.0
116.90	1801.0
117.90	836.0
119.00	1299.0
124.00	118.0
127.90	654.0
128.90	424.0
129.80	579.0
130.90	278.0
134.90	395.0
136.90	336.0
139.90	133.0
141.00	1615.0
142.10	244.0
142.90	2875.0
144.10	258.0
144.90	1248.0
146.00	256.0
147.00	106.0
147.90	455.0
149.90	156.0
152.10	112.0
152.90	120.0
153.90	125.0
154.80	341.0
156.90	318.0
158.80	211.0
161.00	236.0
171.00	597.0
172.00	2064.0

Instrument :
MSVOA_V
ClientSampleId :
BFB337

173.00	1869.0
174.00	149824.0
175.00	11066.0
176.00	142080.0
177.00	9140.0
178.00	267.0

Instrument :
MSVOA_V
ClientSampleId :
BFB337

m/z	Abundance
36.00	1189.0
37.00	6898.0
38.00	6763.0
39.00	3072.0
40.00	286.0
40.70	132.0
44.00	1081.0
45.00	1329.0
46.00	330.0
47.00	2323.0
47.90	935.0
49.00	6743.0
50.00	32128.0
51.00	9967.0
52.00	540.0
53.00	291.0
54.00	281.0
55.00	392.0
56.00	2679.0
57.10	4569.0
58.10	246.0
60.00	1682.0
61.00	8917.0
62.00	9361.0
63.00	8121.0
64.10	1555.0
65.00	2016.0
65.90	188.0
67.00	520.0
68.00	17992.0
69.00	18920.0
70.00	1407.0
72.00	988.0
73.00	8172.0
74.00	33304.0
75.00	94408.0
76.00	8214.0
77.10	1109.0
77.90	840.0
78.90	7863.0
79.90	2101.0
80.90	7996.0
81.90	1811.0
83.00	136.0
85.80	358.0
87.00	8967.0
88.00	9459.0
90.90	822.0
92.00	5817.0
93.00	8785.0
94.00	23576.0
95.00	195456.0
96.10	13367.0
97.10	391.0
103.80	841.0
104.90	326.0
105.90	838.0
107.00	252.0
108.10	236.0
109.70	117.0
110.90	202.0
112.90	183.0
114.90	246.0
115.90	676.0
116.90	1833.0
117.90	863.0
119.00	1383.0
124.00	112.0
127.90	751.0
128.90	481.0
129.90	621.0
130.90	321.0
134.90	446.0
136.90	430.0
139.90	174.0
140.90	1869.0
142.00	218.0
143.00	3341.0
144.10	211.0
144.90	1411.0
145.90	246.0
147.00	154.0
147.90	457.0
149.80	196.0
152.00	112.0
152.80	178.0
153.90	167.0
154.90	460.0
155.80	106.0
156.90	385.0
158.80	251.0
160.90	261.0

Instrument :
MSVOA_V
ClientSampleId :
BFB337

170.90	618.0
172.00	2490.0
173.00	2204.0
174.00	170368.0
175.00	12504.0
176.00	162752.0
177.00	10387.0
178.00	299.0

Instrument :
MSVOA_V
ClientSampleId :
BFB337

m/z	Abundance
36.00	1202.0
37.00	6955.0
38.00	6848.0
39.00	2965.0
40.00	284.0
44.00	1185.0
45.00	1290.0
46.00	357.0
47.00	2241.0
48.00	926.0
49.00	6702.0
50.00	31536.0
51.00	9800.0
52.00	520.0
53.00	270.0
54.00	266.0
55.00	379.0
56.00	2639.0
57.10	4457.0
58.10	254.0
60.00	1496.0
61.00	8874.0
62.00	9070.0
63.00	8082.0
64.10	1417.0
65.10	1814.0
65.90	186.0
66.90	544.0
68.00	17816.0
69.00	18840.0
70.00	1475.0
72.00	975.0
73.00	8401.0
74.10	32992.0
75.00	94368.0
76.00	8014.0
77.10	1088.0
77.90	910.0
78.90	8004.0
80.00	2201.0
80.90	7931.0
81.90	1804.0
83.10	160.0
85.90	365.0
87.00	9127.0
88.00	9632.0
90.90	833.0
92.00	5761.0
93.00	8805.0
94.00	23560.0
95.00	194944.0
96.10	13035.0
97.10	330.0
103.90	815.0
105.00	379.0
105.90	871.0
107.00	235.0
108.00	204.0
109.70	126.0
110.90	173.0
112.80	190.0
114.90	267.0
115.90	635.0
116.90	1671.0
117.90	823.0
118.90	1281.0
123.70	108.0
125.90	110.0
127.90	763.0
129.00	452.0
129.90	678.0
130.90	331.0
134.90	438.0
136.90	467.0
139.90	156.0
140.90	2005.0
142.00	195.0
143.00	3557.0
144.10	154.0
144.90	1405.0
145.80	282.0
146.90	188.0
147.90	453.0
149.80	216.0
152.80	185.0
153.90	183.0
154.90	566.0
155.80	103.0
156.90	380.0
158.80	255.0
160.90	251.0
170.90	551.0

Instrument :
MSVOA_V
ClientSampleId :
BFB337

172.00	2742.0
173.00	2320.0
174.00	175104.0
175.00	12361.0
176.00	168576.0
177.00	10425.0
178.00	301.0

Instrument :
MSVOA_V
ClientSampleId :
BFB337