

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070218\
 Data File : VV006523.D
 Acq On : 02 Jul 2018 11:09
 Operator : SY/MD
 Sample : VV0702WBL01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK68

Quant Time: Jul 02 23:36:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 30 02:15:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	327359	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	296720	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	131067	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	101954	4.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.80%
7) Chloroethane-d5	1.59	69	81672	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.20%
11) 1,1-Dichloroethene-d2	2.13	63	133526	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.97	46	179102	44.40	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.80%
24) Chloroform-d	4.41	84	153958	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.00%
26) 1,2-Dichloroethane-d4	5.09	65	74461	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
32) Benzene-d6	5.10	84	348930	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	101810	4.42	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.40%
41) Toluene-d8	7.36	98	311170	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.00%
43) trans-1,3-Dichloropropene-	7.67	79	33292	3.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.60%
46) 2-Hexanone-d5	8.14	63	126274	37.59	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.18%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	52971	3.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	106315	4.37	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.40%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	5567	0.24 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070218\
Data File : VV006523.D
Acq On : 02 Jul 2018 11:09
Operator : SY/MD
Sample : VV0702WBL01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK68

Quant Time: Jul 02 23:36:12 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 30 02:15:06 2018
Response via : Initial Calibration

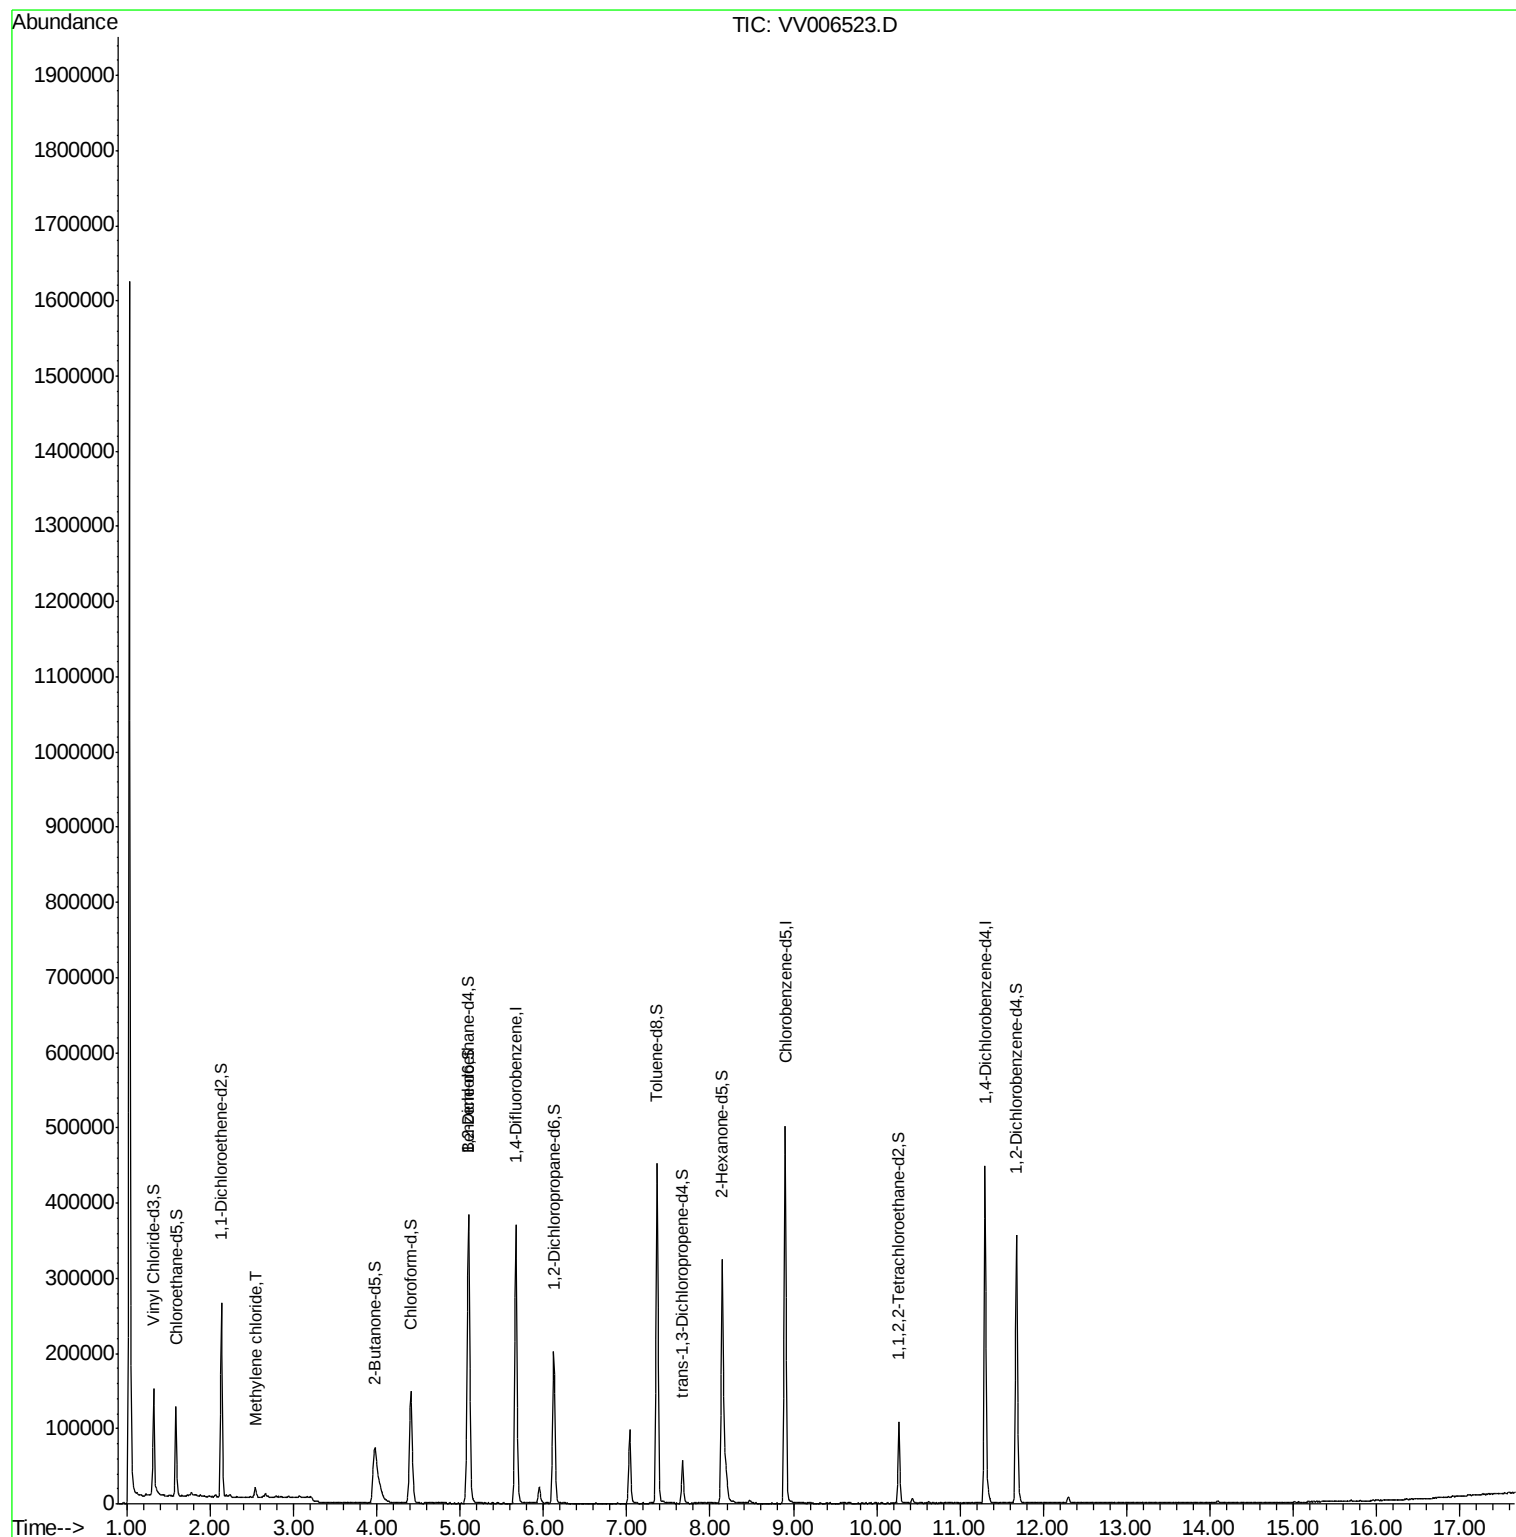

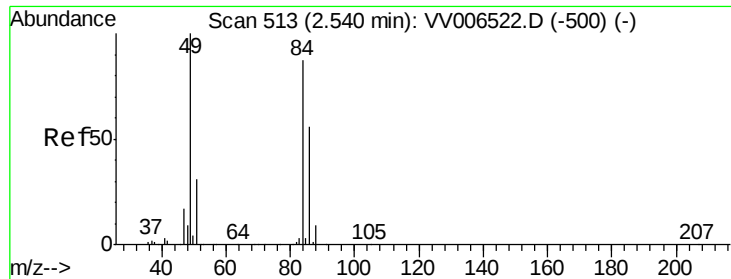

#16
 Methvlene chloride
 Concen: 0.24 ug/L
 RT: 2.54 min Scan# 513
 Delta R.T. 0.00 min
 Lab File: VV006523.D
 Acq: 02 Jul 2018 11:09

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK68

Tot Ion: 84 Resp: 5567
 Ion Ratio Lower Upper
 84 100
 86 65.5 44.2 82.2
 49 118.9 79.0 146.8

