

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070218\
 Data File : VV006538.D
 Acq On : 02 Jul 2018 18:51
 Operator : SY/MD
 Sample : J3792-16
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB0J1

Quant Time: Jul 02 23:57:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 30 02:15:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	284914	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	259779	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	113312	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	96176	5.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.60%
7) Chloroethane-d5	1.58	69	82110	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.80%
11) 1,1-Dichloroethene-d2	2.13	63	128563	3.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.40%
20) 2-Butanone-d5	3.96	46	245532	69.94	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	139.88%#
24) Chloroform-d	4.41	84	173434	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.60%
26) 1,2-Dichloroethane-d4	5.09	65	89454	5.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.80%
32) Benzene-d6	5.11	84	372852	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.40%
36) 1,2-Dichloropropane-d6	6.12	67	115636	5.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.80%
41) Toluene-d8	7.37	98	324175	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%
43) trans-1,3-Dichloropropene-	7.67	79	33885	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
46) 2-Hexanone-d5	8.14	63	184020	62.57	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	125.14%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	72500	5.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	117.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	121976	5.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	2799	1.30 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070218\
Data File : VV006538.D
Acq On : 02 Jul 2018 18:51
Operator : SY/MD
Sample : J3792-16
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB0J1

Quant Time: Jul 02 23:57:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 30 02:15:06 2018
Response via : Initial Calibration

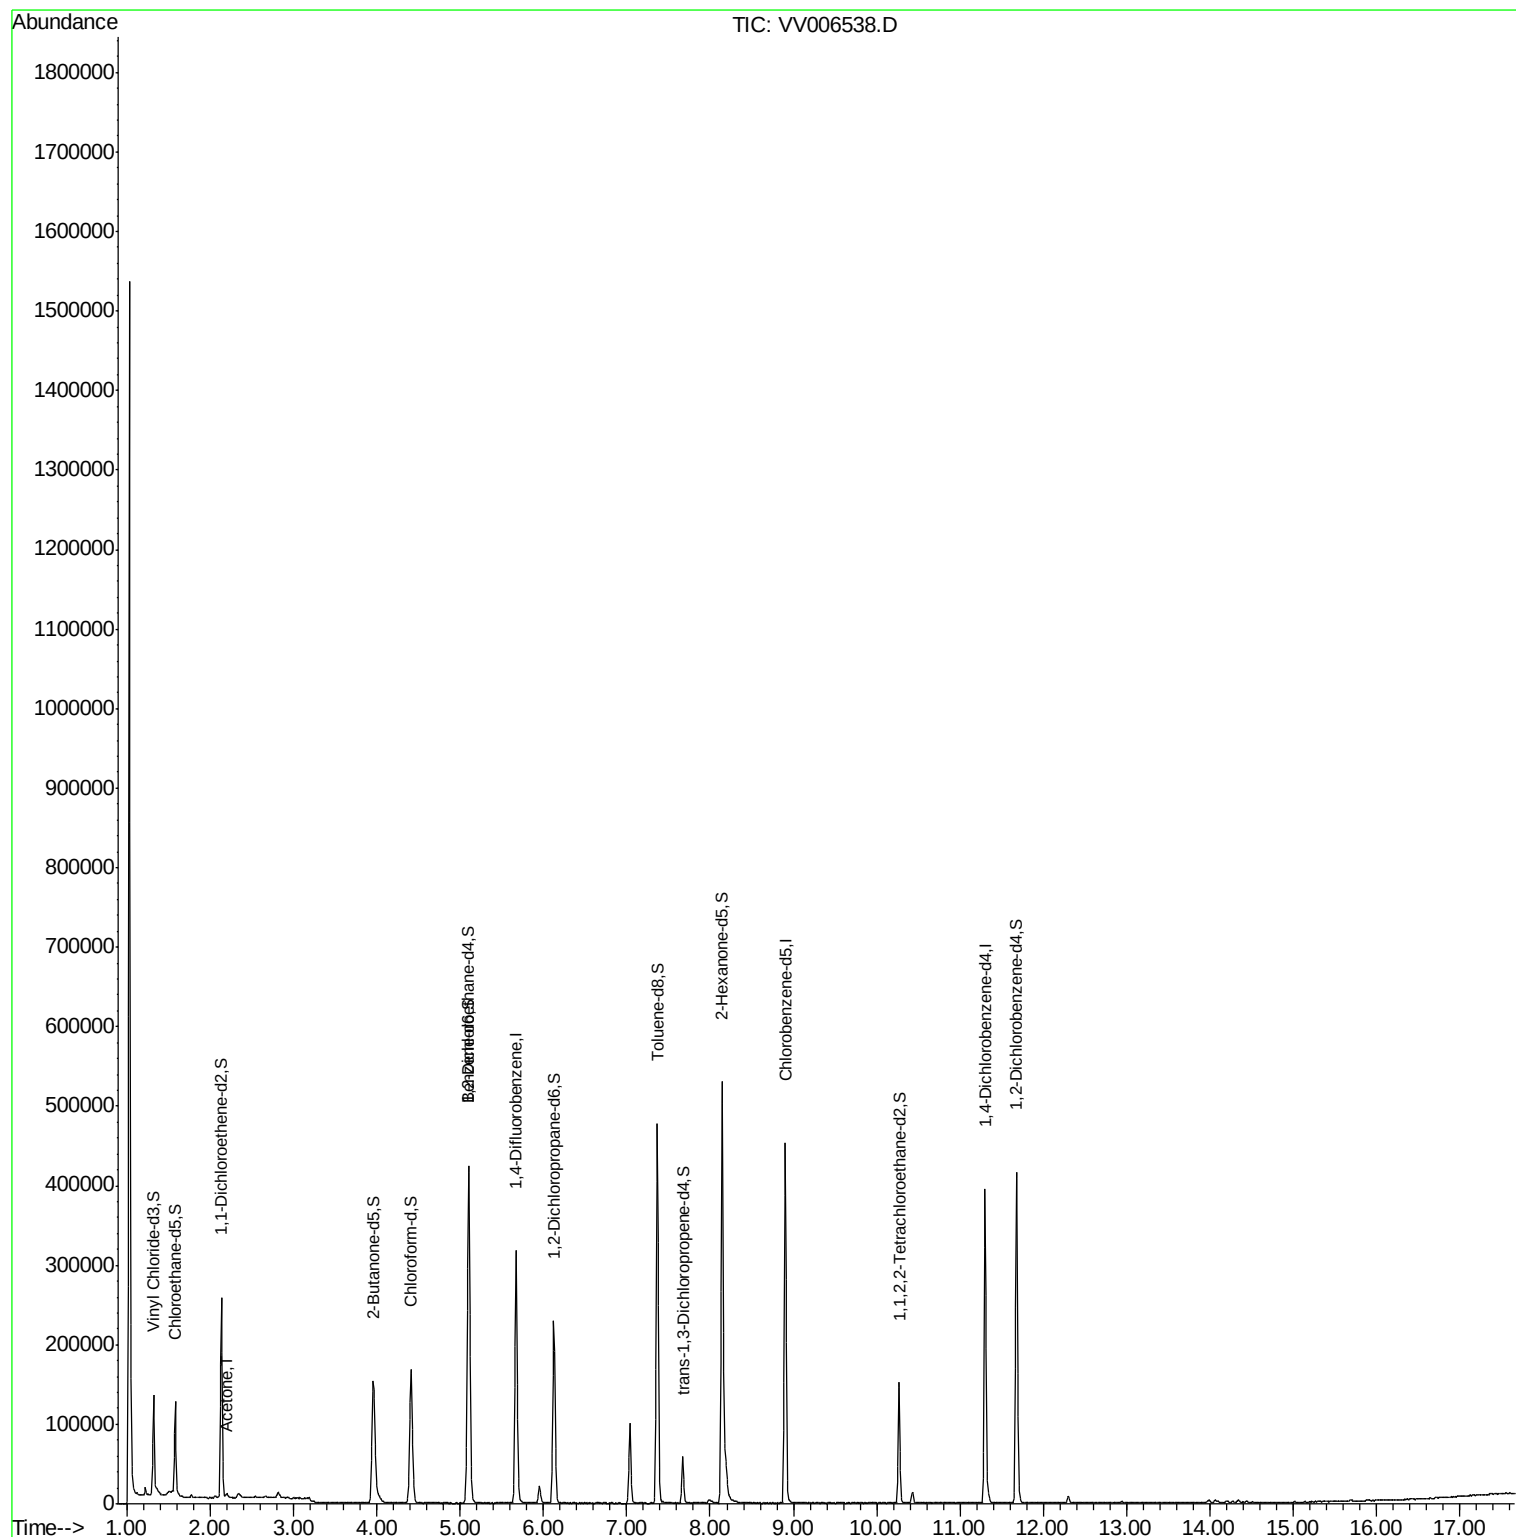

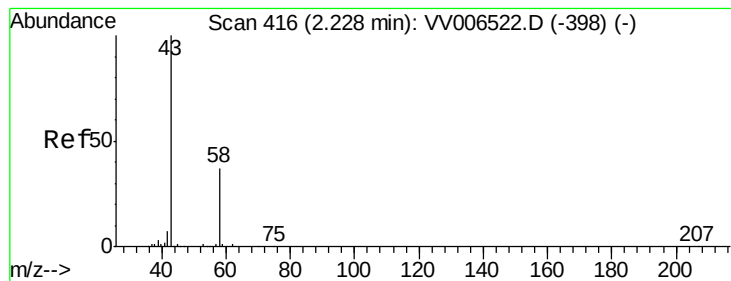

#13

Acetone

Concen: 1.30 ug/L

RT: 2.20 min Scan# 407

Delta R.T. -0.04 min

Lab File: VV006538.D

Acq: 02 Jul 2018 18:51

Instrument :

MSVOA_V

ClientSampleId :

DB0J1

Tot Ion: 43 Resp: 2799

Ion Ratio Lower Upper

43 100

58 43.3 0.0 77.4

