

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070218\
 Data File : VV006539.D
 Acq On : 02 Jul 2018 19:18
 Operator : SY/MD
 Sample : J3792-20
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB0J3

Quant Time: Jul 02 23:58:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 30 02:15:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	278714	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	255820	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	113065	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	90784	4.95	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.00%
7) Chloroethane-d5	1.58	69	78929	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.00%
11) 1,1-Dichloroethene-d2	2.13	63	122427	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.95	46	240341	69.99	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	139.98%#
24) Chloroform-d	4.41	84	166502	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.60%
26) 1,2-Dichloroethane-d4	5.09	65	85256	5.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.60%
32) Benzene-d6	5.11	84	360074	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.20%
36) 1,2-Dichloropropane-d6	6.12	67	111671	5.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.60%
41) Toluene-d8	7.37	98	310936	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
43) trans-1,3-Dichloropropene-	7.67	79	32211	4.41	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.20%
46) 2-Hexanone-d5	8.14	63	178528	61.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.28%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	69622	5.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	117281	5.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	3729	1.77 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070218\
Data File : VV006539.D
Acq On : 02 Jul 2018 19:18
Operator : SY/MD
Sample : J3792-20
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB0J3

Quant Time: Jul 02 23:58:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 30 02:15:06 2018
Response via : Initial Calibration

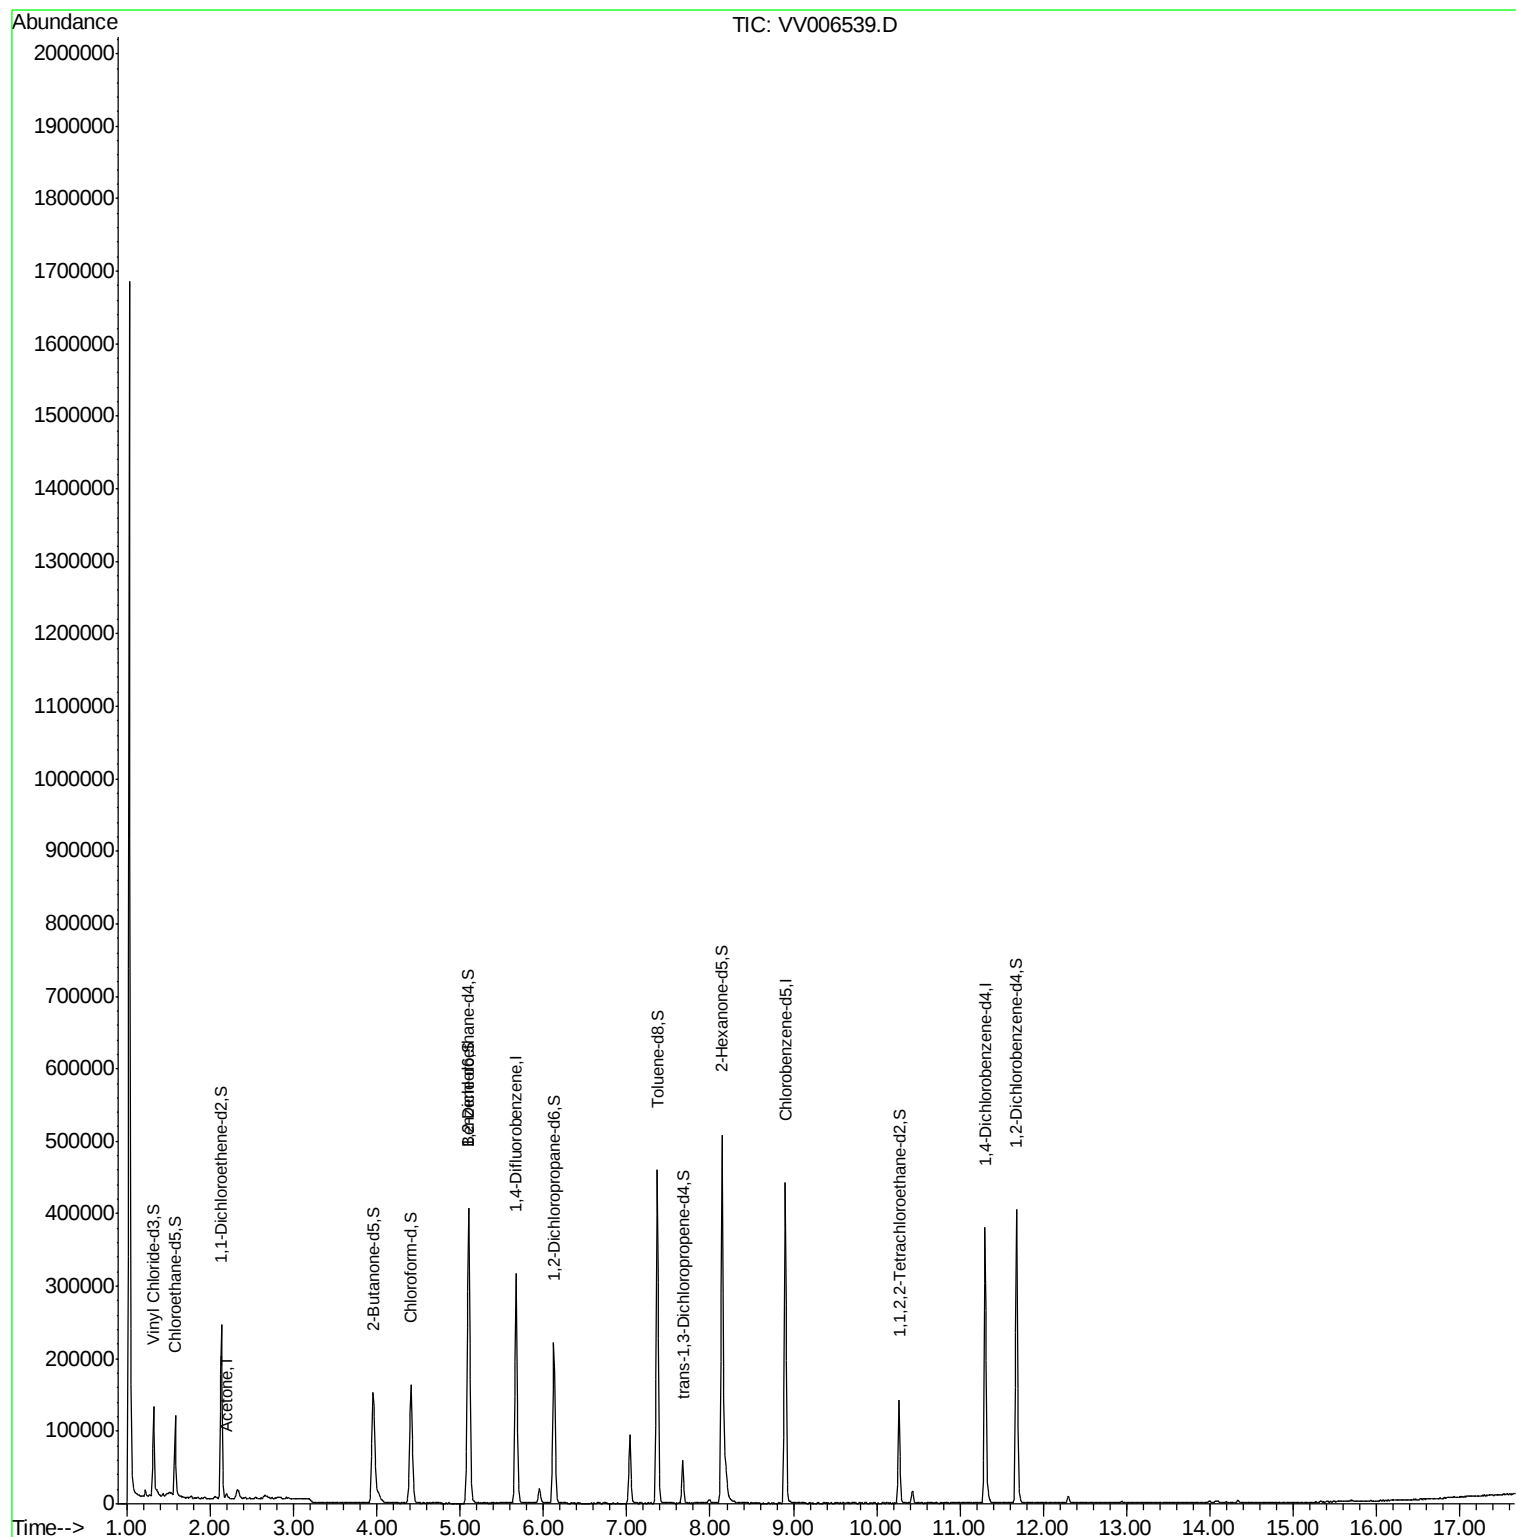

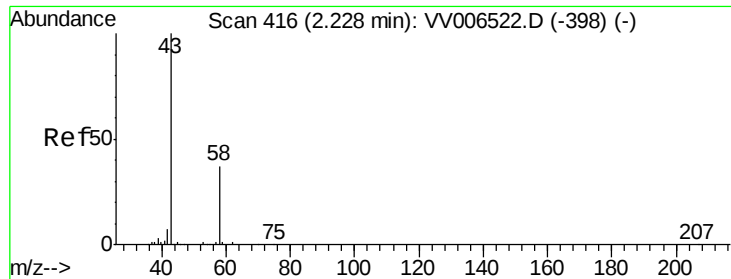

#13

Acetone

Concen: 1.77 ug/L

RT: 2.20 min Scan# 407

Delta R.T. -0.04 min

Lab File: VV006539.D

Acq: 02 Jul 2018 19:18

Instrument :

MSVOA_V

ClientSampleId :

DB0J3

Tot Ion: 43 Resp: 3729

Ion Ratio Lower Upper

43 100

58 41.2 0.0 77.4

