


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070218\
Data File : VV006521.D
Acq On : 02 Jul 2018 08:54
Operator : SY/MD
Sample : BFB64
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB64

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 05 12:04:44 2018

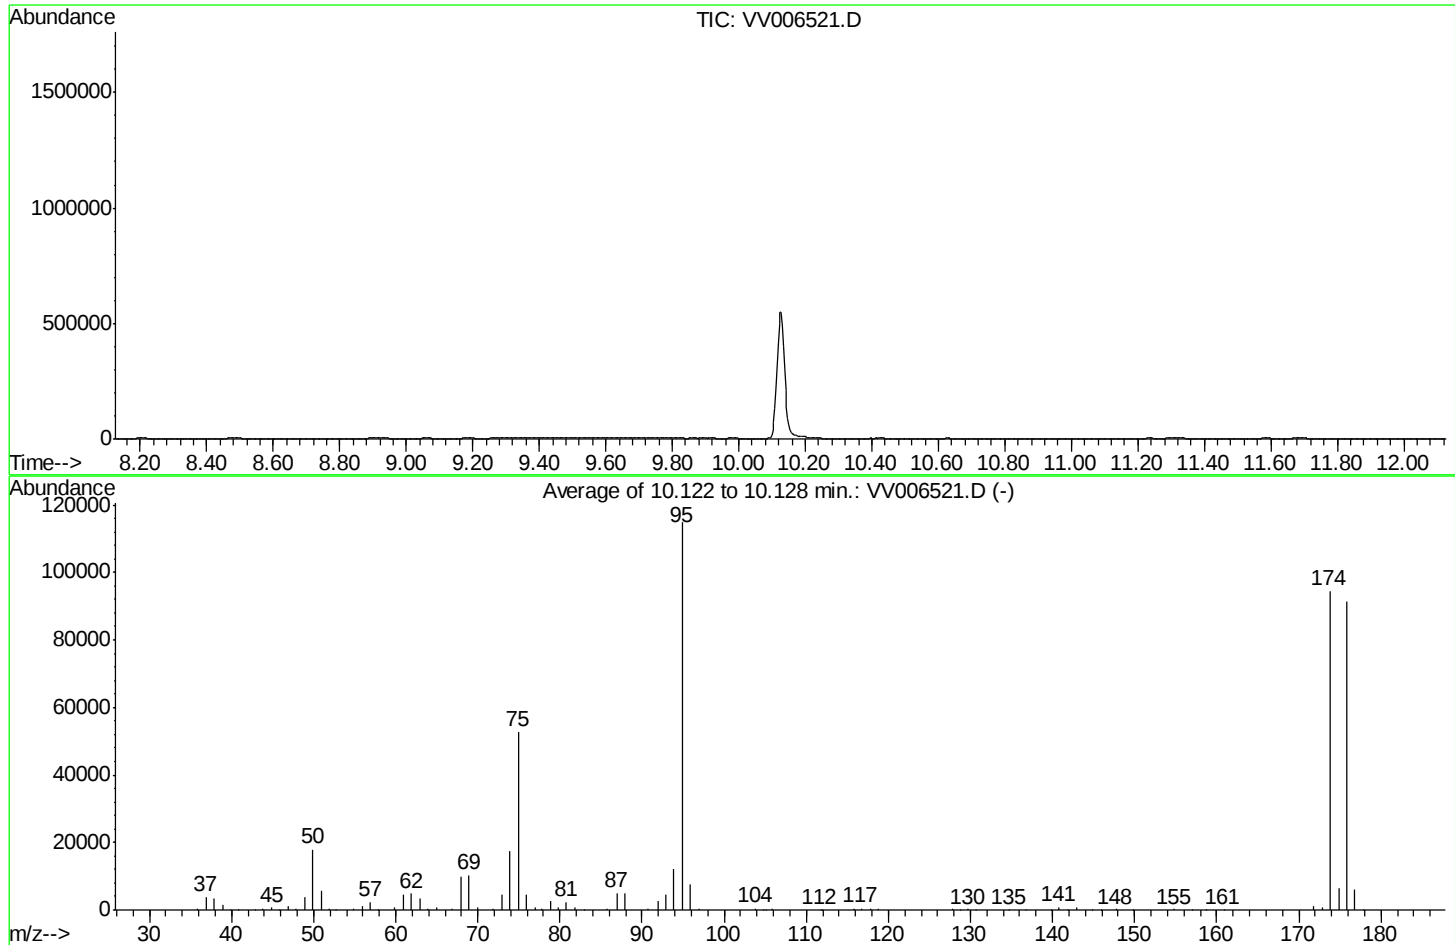

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	18021	PASS
75	95	30	80	46.0	52794	PASS
95	95	100	100	100.0	114821	PASS
96	95	5	9	6.6	7565	PASS
173	174	0.00	2	0.8	715	PASS
174	95	50	120	82.4	94589	PASS
175	174	5	9	6.8	6448	PASS
176	174	95	101	96.8	91517	PASS
177	176	5	9	6.5	5924	PASS

Scan 2858 (10.080 min): VV006521.D
BFB64

m/z	Abundance
35.80	1330.0
37.80	454.0
38.80	106.0
39.80	192.0
43.80	713.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	1901.0
36.90	3673.0
37.90	3841.0
38.90	1610.0
39.90	261.0
42.80	122.0
43.90	1060.0
44.90	664.0
45.80	143.0
46.90	1188.0
47.80	497.0
48.90	3566.0
49.90	17064.0
50.90	5472.0
51.90	252.0
54.90	365.0
55.90	1198.0
56.90	2294.0
57.90	130.0
59.90	796.0
60.90	4104.0
61.90	4570.0
62.90	3448.0
63.90	500.0
65.00	764.0
66.90	251.0
67.90	9266.0
68.90	9892.0
69.90	769.0
71.80	565.0
72.90	4331.0
73.90	16488.0
74.90	50248.0
76.00	4582.0
77.00	672.0
77.80	385.0
78.80	2359.0
79.80	729.0
80.80	2246.0
81.80	601.0
82.90	102.0
85.70	233.0
86.90	4656.0
87.80	4581.0
90.80	377.0
91.90	2676.0
92.90	4104.0
93.90	11514.0
94.90	108712.0
95.90	7364.0
96.90	227.0
103.80	386.0
104.70	153.0
105.80	358.0
111.70	113.0
115.80	370.0
116.70	530.0
117.80	379.0
118.80	448.0
127.70	337.0
128.80	178.0
129.70	364.0
130.60	102.0
134.70	168.0
136.70	166.0
140.80	858.0
142.90	849.0
144.70	157.0
145.90	132.0
147.70	292.0
149.70	103.0
154.90	216.0
156.90	138.0
171.90	992.0
172.80	670.0
173.80	87152.0
174.90	6151.0
175.80	84352.0
176.90	5333.0
177.90	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	1897.0
36.90	3951.0
37.90	4020.0
38.90	1703.0
39.90	281.0
40.80	112.0
42.80	128.0
43.80	1085.0
44.90	720.0
45.80	132.0
46.80	1309.0
47.90	553.0
48.90	3834.0
49.90	18664.0
50.90	5969.0
51.90	236.0
54.90	373.0
55.90	1316.0
56.90	2478.0
57.80	118.0
59.80	832.0
60.90	4566.0
61.90	4977.0
62.90	3686.0
63.90	567.0
64.90	829.0
66.90	295.0
67.90	10024.0
68.90	10583.0
69.90	789.0
71.80	581.0
72.90	4667.0
73.90	18112.0
74.90	54392.0
75.90	4800.0
77.00	659.0
77.80	397.0
78.80	2582.0
79.80	808.0
80.80	2415.0
81.80	695.0
82.90	117.0
85.70	238.0
86.90	5191.0
87.90	5010.0
90.80	374.0
91.90	2886.0
92.90	4574.0
93.90	12408.0
94.90	118520.0
95.90	7813.0
96.90	279.0
103.90	417.0
104.70	151.0
105.80	365.0
111.70	102.0
115.80	378.0
116.70	598.0
117.80	408.0
118.80	502.0
127.80	332.0
128.80	194.0
129.70	381.0
130.70	107.0
134.70	178.0
136.70	186.0
140.80	940.0
141.80	120.0
142.90	884.0
144.70	172.0
145.80	148.0
147.70	291.0
149.80	107.0
154.80	260.0
156.90	181.0
158.70	113.0
160.80	110.0
171.80	1153.0
172.90	737.0
173.80	97648.0
174.90	6660.0
175.80	94328.0
176.90	6144.0
177.90	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	1854.0
36.90	3883.0
37.90	3877.0
39.00	1665.0
39.90	282.0
40.80	106.0
42.80	123.0
43.80	1102.0
44.90	704.0
45.80	112.0
46.80	1272.0
47.90	570.0
48.90	3709.0
49.90	18336.0
50.90	5852.0
51.90	223.0
52.70	136.0
54.90	343.0
55.90	1326.0
56.90	2508.0
57.80	102.0
59.80	777.0
60.90	4620.0
61.90	4840.0
62.90	3638.0
63.90	551.0
64.90	827.0
66.90	309.0
67.90	10013.0
68.90	10372.0
69.90	772.0
71.90	565.0
72.90	4587.0
73.90	17704.0
74.90	53744.0
75.90	4541.0
77.00	649.0
77.80	384.0
78.80	2552.0
79.80	822.0
80.80	2372.0
81.80	740.0
82.90	130.0
85.80	195.0
86.90	5165.0
87.80	4912.0
90.70	360.0
91.90	2831.0
92.90	4446.0
93.90	12299.0
94.90	117232.0
95.90	7518.0
96.90	280.0
103.90	376.0
105.00	148.0
105.80	356.0
111.90	116.0
115.80	349.0
116.80	593.0
117.80	375.0
118.80	514.0
127.70	317.0
128.70	172.0
129.80	361.0
130.70	123.0
134.70	193.0
136.80	195.0
139.80	102.0
140.80	946.0
141.90	124.0
142.90	908.0
144.80	194.0
145.80	140.0
147.70	255.0
149.90	133.0
154.80	283.0
156.90	221.0
158.70	129.0
160.80	124.0
171.80	1203.0
172.90	739.0
173.80	98968.0
174.90	6534.0
175.80	95872.0
176.80	6297.0
177.80	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64