

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070219\
 Data File : VV011807.D
 Acq On : 02 Jul 2019 17:07
 Operator : SY/MD
 Sample : VIBLK40
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK40

Quant Time: Jul 03 08:40:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 03 08:28:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	171286	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	157325	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	62585	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	57650	5.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.00%
7) Chloroethane-d5	1.58	69	44670	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.80%
11) 1,1-Dichloroethene-d2	2.12	63	83974	3.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.40%
20) 2-Butanone-d5	3.97	46	146512	51.47	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.94%
24) Chloroform-d	4.40	84	108103	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.08	65	60432	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.09	84	218099	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
36) 1,2-Dichloropropane-d6	6.12	67	68971	5.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.00%
41) Toluene-d8	7.36	98	187874	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
43) trans-1,3-Dichloropropene-	7.66	79	20815	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.14	63	112763	54.33	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.66%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	45044	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	62323	5.64	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.80%


Target Compounds					Ovalue
47) Tetrachloroethene	8.01	164	1693	0.177 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070219\
Data File : VV011807.D
Acq On : 02 Jul 2019 17:07
Operator : SY/MD
Sample : VIBLK40
Misc : 25ML/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK40

Quant Time: Jul 03 08:40:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 08:28:44 2019
Response via : Initial Calibration

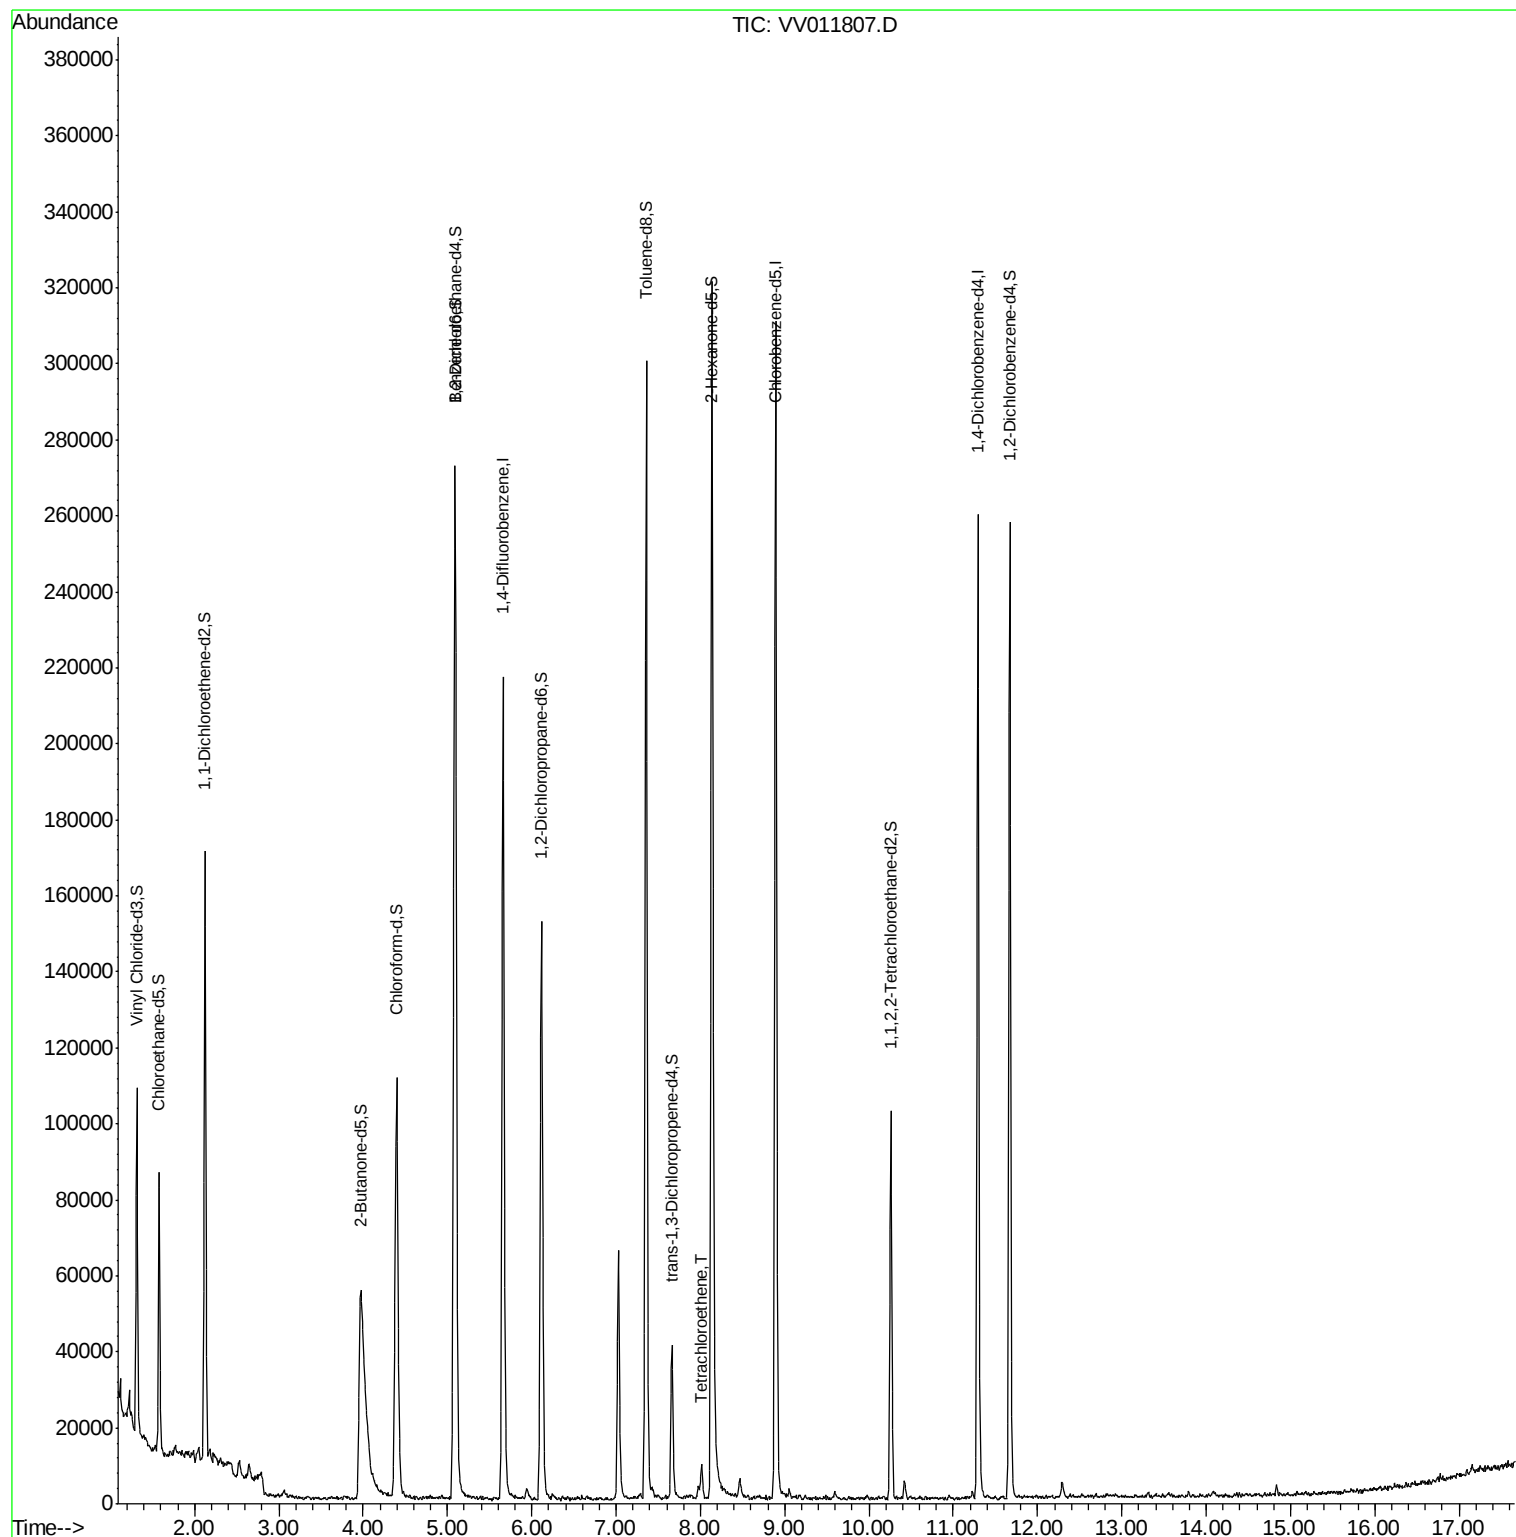

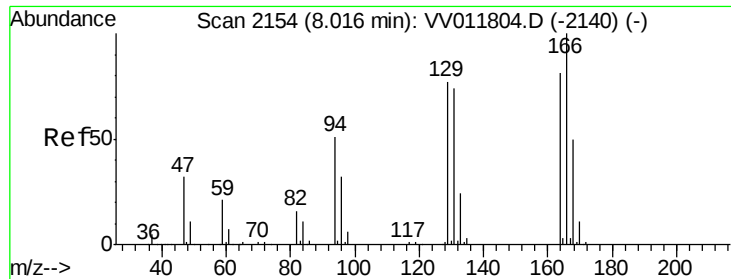

#47
Tetrachloroethene
Concen: 0.177 ug/L
RT: 8.01 min Scan# 2153
Delta R.T. -0.00 min
Lab File: VV011807.D
Acq: 02 Jul 2019 17:07

Instrument :
MSVOA_V
ClientSampleId :
VIBLK40

Tot Ion:	164	Resp:	1693
Ion	Ratio	Lower	Upper
164	100		
129	102.7	65.7	121.9
131	87.0	63.2	117.4
166	113.7	85.8	159.3

