

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070219\
 Data File : VV011814.D
 Acq On : 02 Jul 2019 19:58
 Operator : SY/MD
 Sample : K3608-15
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAMM4

Quant Time: Jul 03 09:03:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 03 08:28:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	178335	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	174330	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	78073	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65806	5.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.60%
7) Chloroethane-d5	1.58	69	51892	5.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.40%
11) 1,1-Dichloroethene-d2	2.13	63	96772	4.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.40%
20) 2-Butanone-d5	3.95	46	158481	53.47	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.94%
24) Chloroform-d	4.40	84	119755	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.08	65	64937	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.10	84	244319	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
36) 1,2-Dichloropropane-d6	6.12	67	74158	5.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.80%
41) Toluene-d8	7.36	98	211572	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
43) trans-1,3-Dichloropropene-	7.67	79	23140	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.14	63	117844	51.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.48%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	49236	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	74405	5.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	7626	3.757 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070219\
Data File : VV011814.D
Acq On : 02 Jul 2019 19:58
Operator : SY/MD
Sample : K3608-15
Misc : 25ML/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAMM4

Quant Time: Jul 03 09:03:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 08:28:44 2019
Response via : Initial Calibration

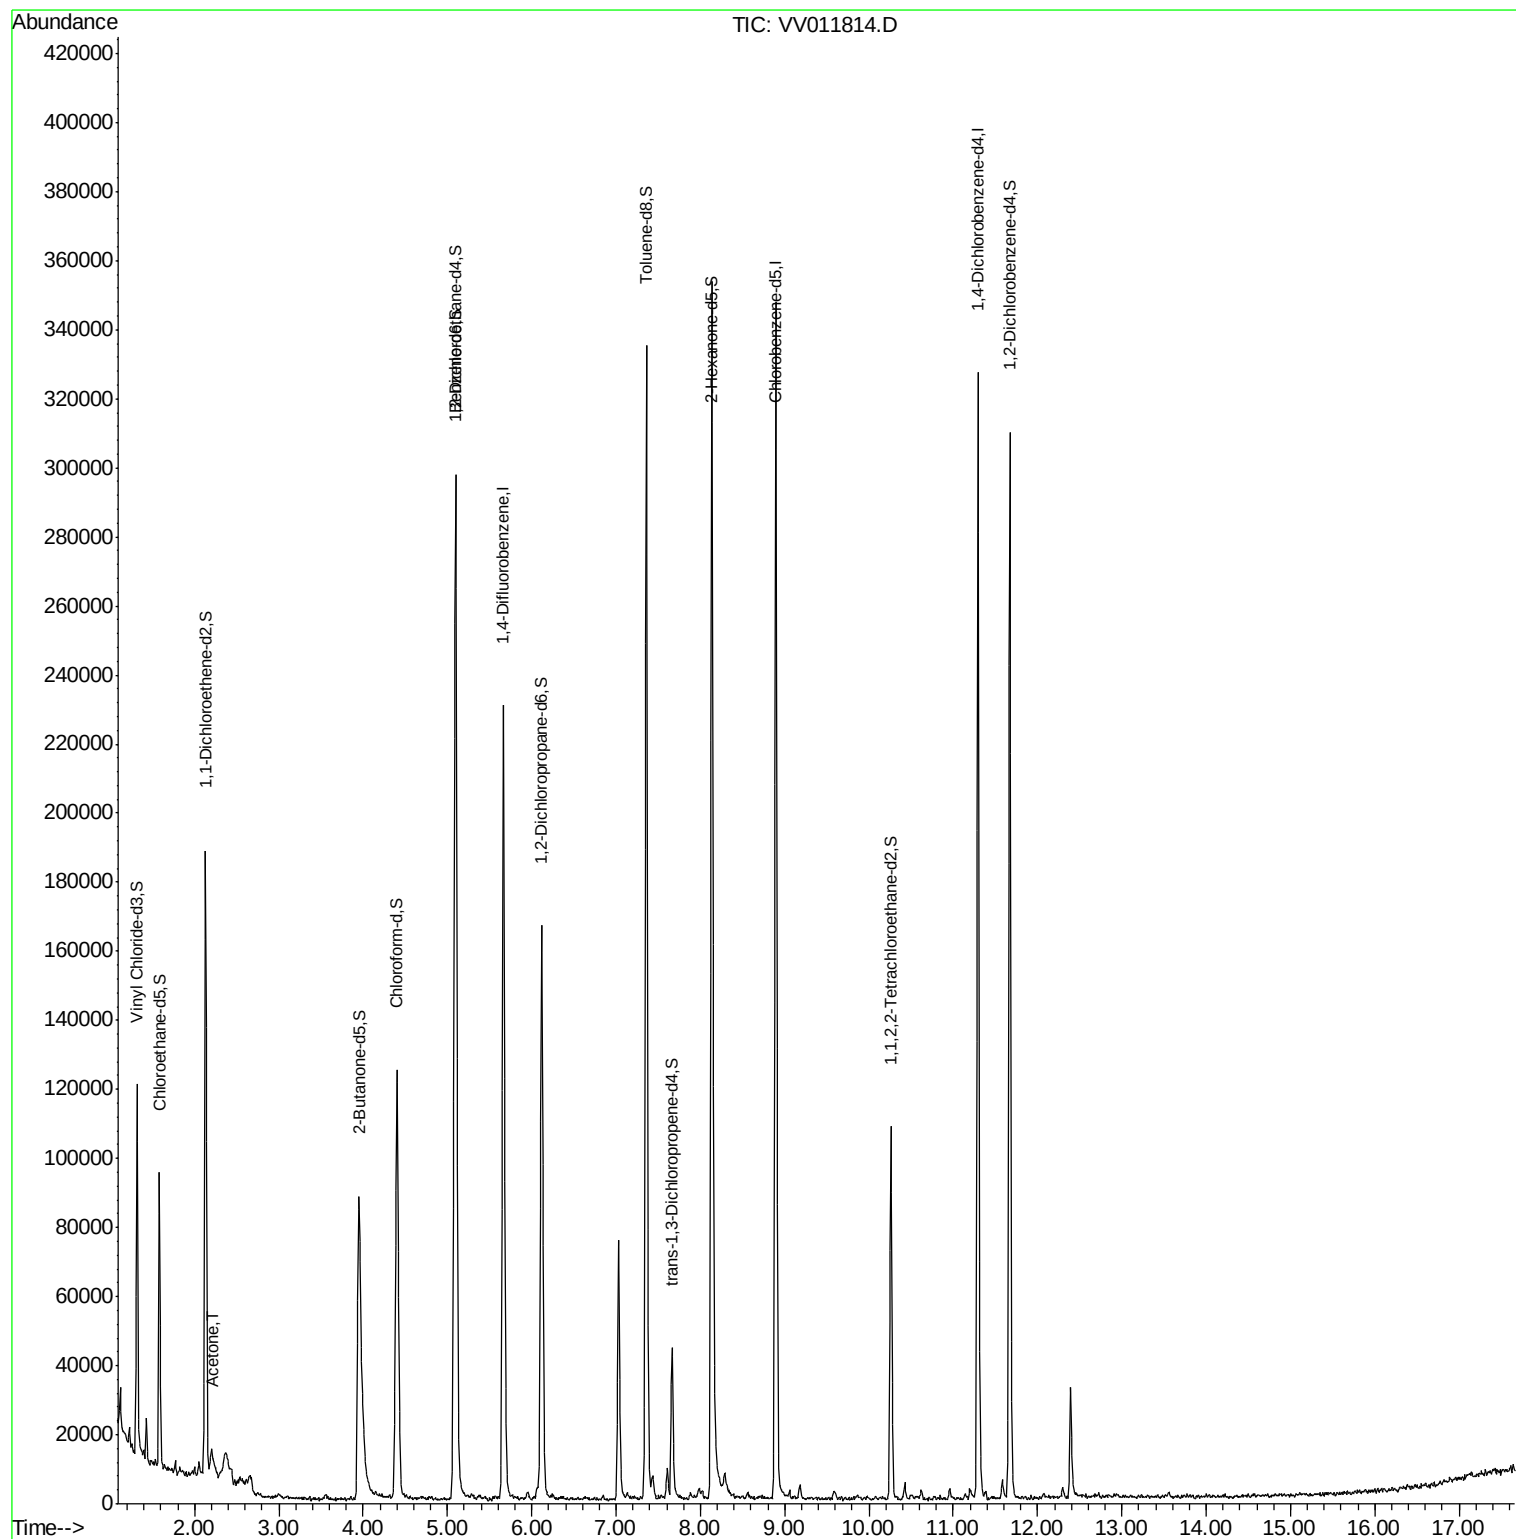

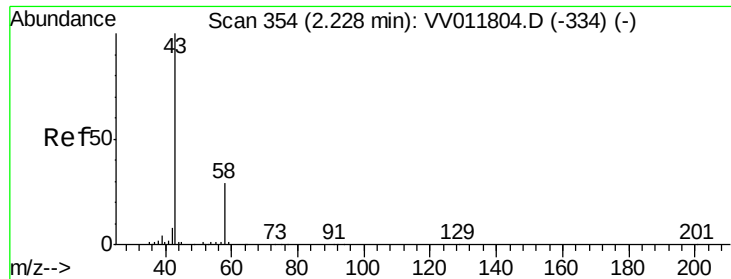

#13

Acetone

Concen: 3.757 ug/L

RT: 2.20 min Scan# 346

Delta R.T. -0.03 min

Lab File: VV011814.D

Acq: 02 Jul 2019 19:58

Instrument :
MSVOA_V
ClientSampleId :
GAMM4

Tot Ion: 43 Resp: 7626

Ion Ratio Lower Upper

43 100

58 32.8 0.0 58.0

