
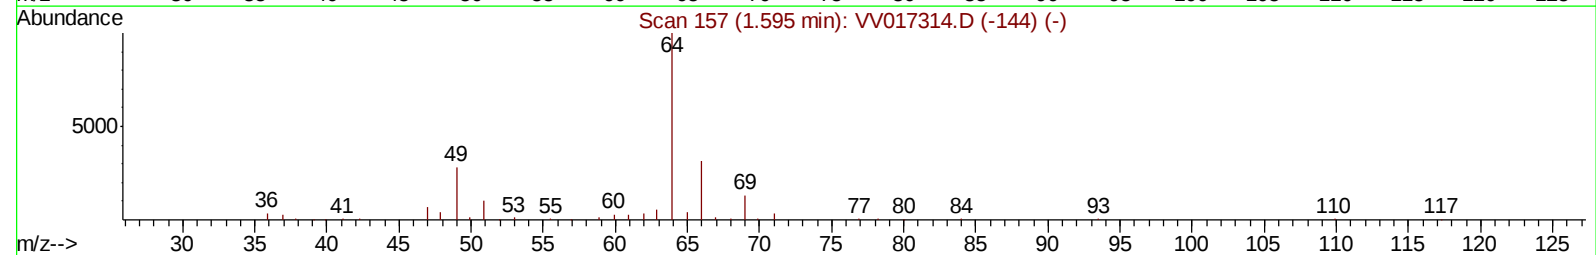
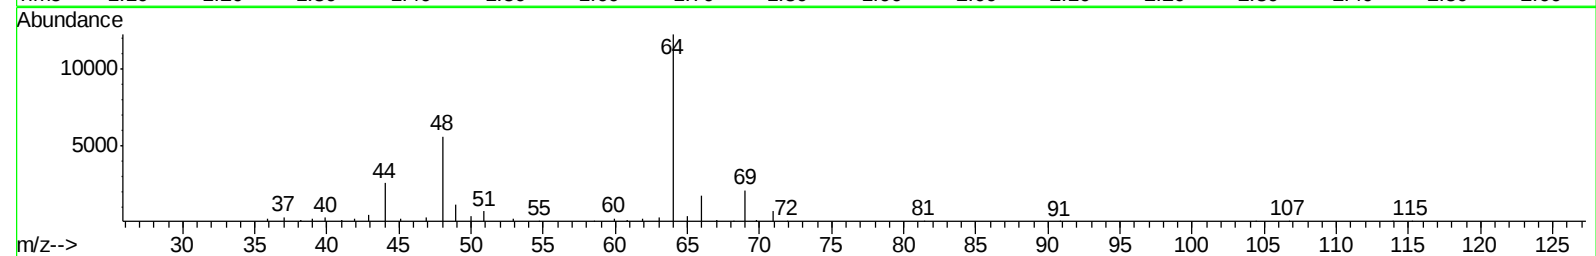


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
Data File : VV017318.D
Acq On : 02 Jul 2020 20:13
Operator : SY/MD
Sample : L3154-03DL 10X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Jul 03 06:17:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 03 06:15:26 2020
Response via : Initial Calibration

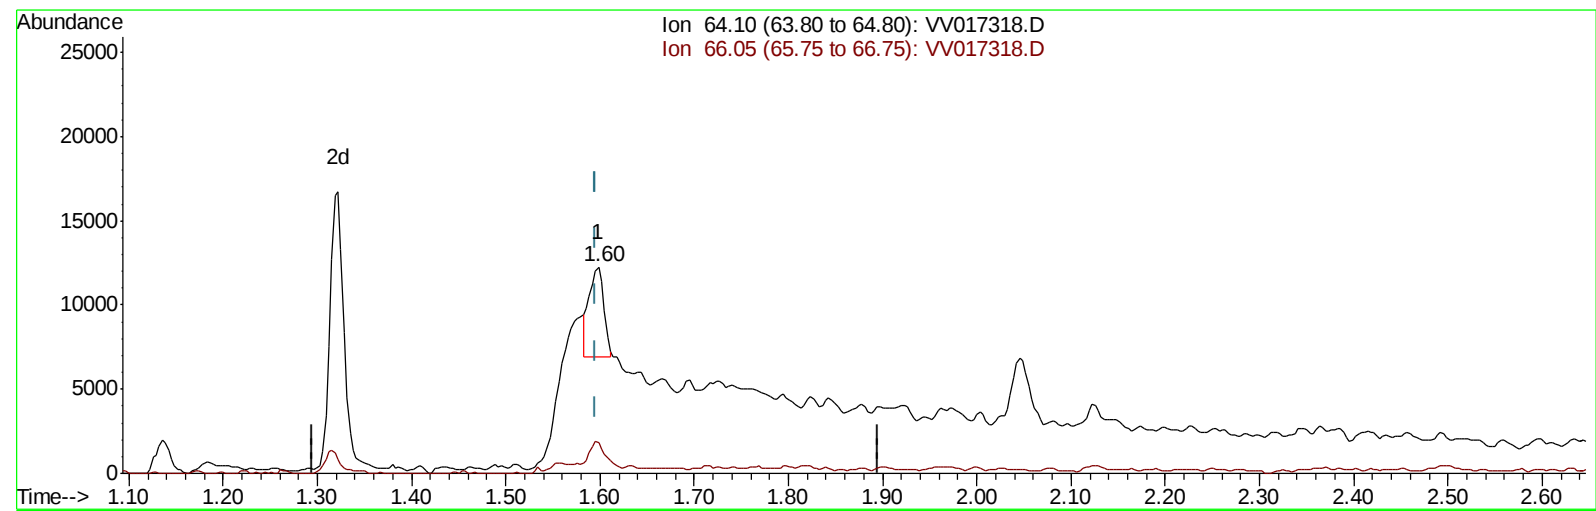

TIC: VV017318.D

(8) Chloroethane (T)

1.598min (+0.003) 0.92ug/L m

response 5708

Ion	Exp%	Act%
64.10	100	100
66.05	32.60	14.72#
0.00	0.00	0.00
0.00	0.00	0.00