

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
 Data File : VV017302.D
 Acq On : 02 Jul 2020 11:48
 Operator : SY/MD
 Sample : L3150-09DL 5X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETYJ4DL

Quant Time: Jul 03 04:19:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 03 01:13:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	167374	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	163000	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	75391	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46866	4.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.20%
7) Chloroethane-d5	1.58	69	35894	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.13	63	74547	3.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.00%
20) 2-Butanone-d5	3.92	46	104163	40.69	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.38%
24) Chloroform-d	4.38	84	100186	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.06	65	53076	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
32) Benzene-d6	5.08	84	187716	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
36) 1,2-Dichloropropane-d6	6.10	67	53446	4.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.40%
41) Toluene-d8	7.34	98	164759	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
45) trans-1,3-Dichloropropene-	7.64	79	20379	3.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.40%
48) 2-Hexanone-d5	8.11	63	64973	32.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	64.68%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	35193	4.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	62161	4.46	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.20%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	4114	0.478 ug/L	90
22) cis-1,2-Dichloroethene	3.95	96	3698	0.318 ug/L	99
34) Trichloroethene	5.94	95	93984	7.519 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070220\
Data File : VV017302.D
Acq On : 02 Jul 2020 11:48
Operator : SY/MD
Sample : L3150-09DL 5X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETYJ4DL

Quant Time: Jul 03 04:19:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 03 01:13:36 2020
Response via : Initial Calibration

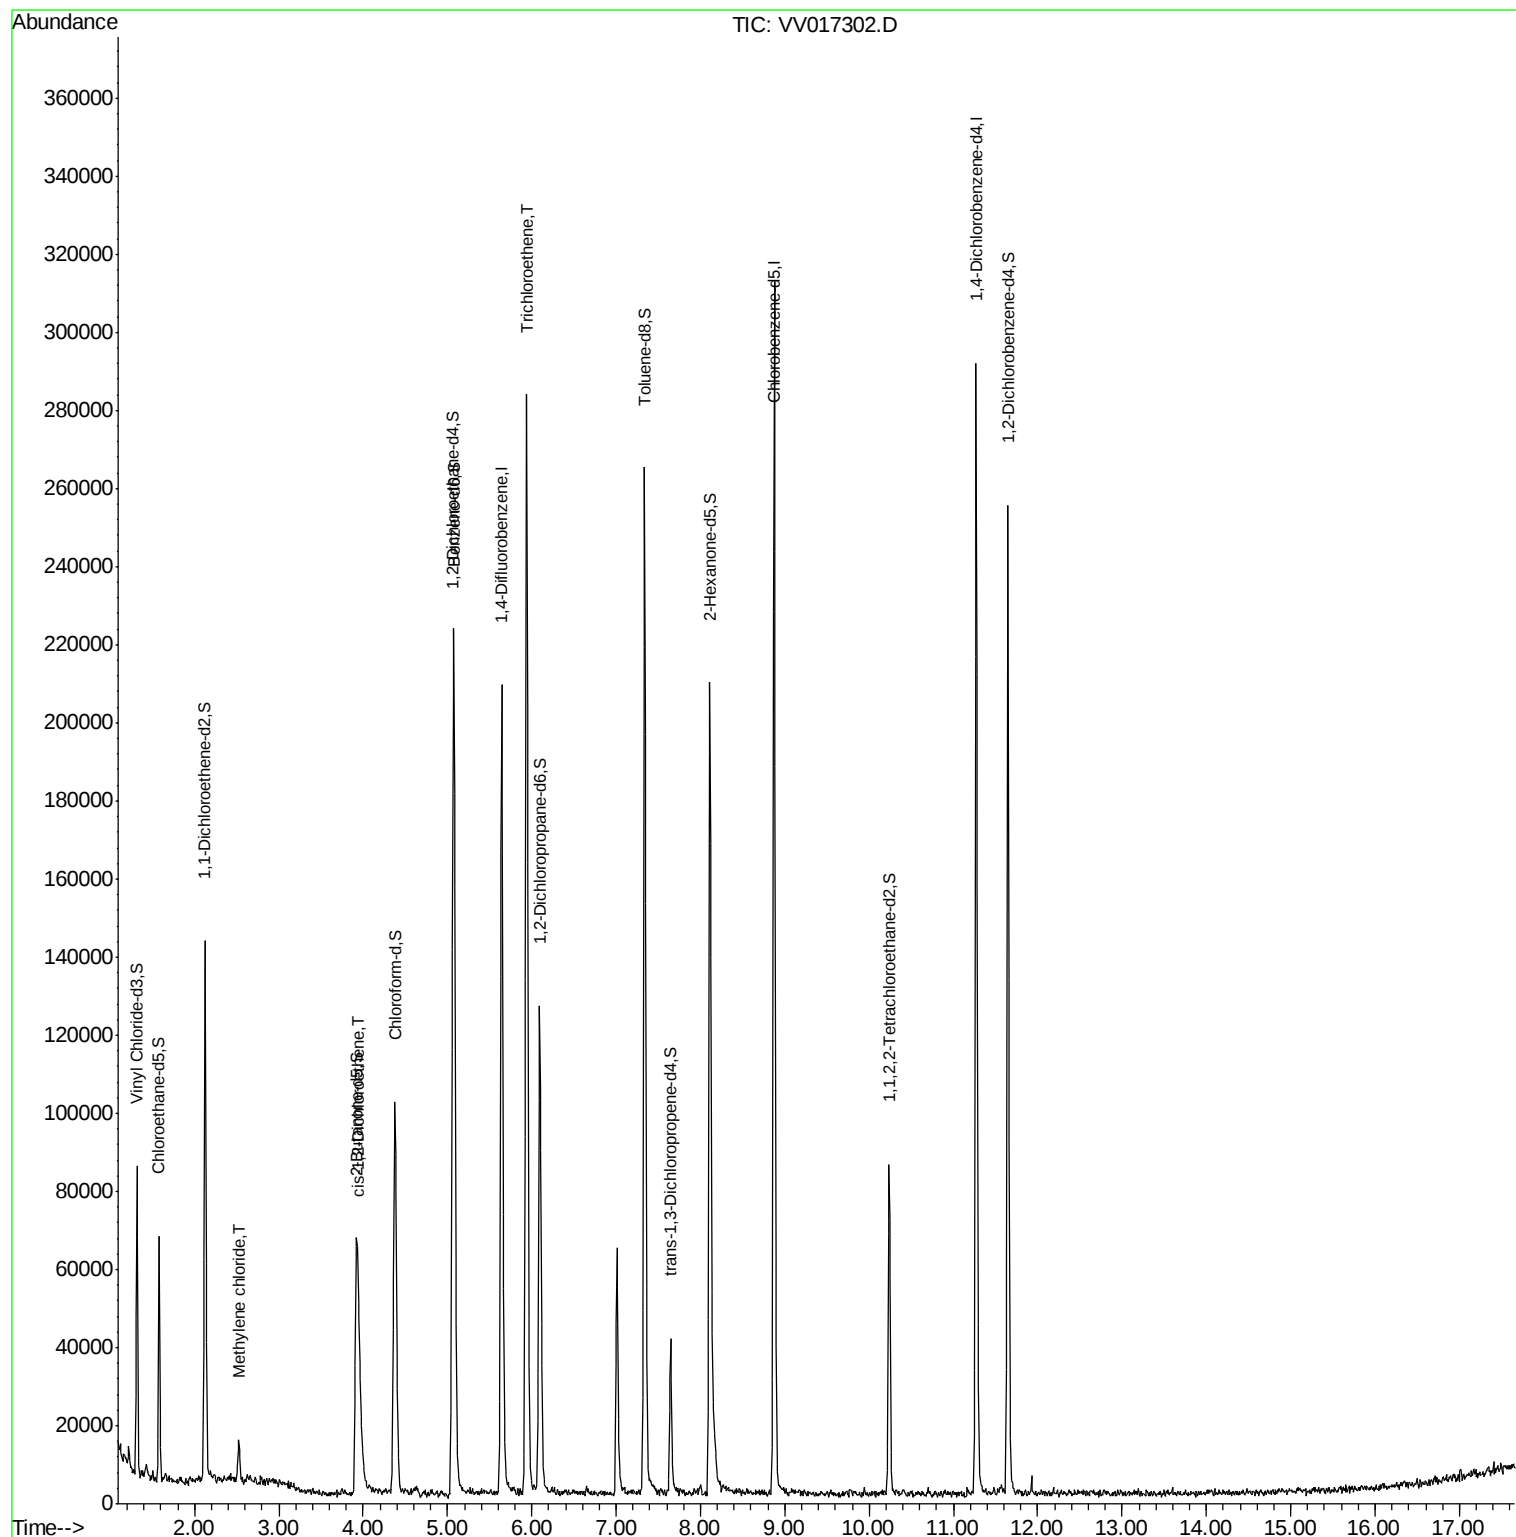


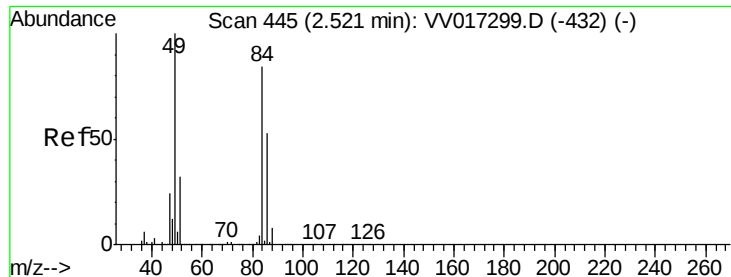




#16
Methvlene chloride
Concen: 0.478 ug/L
RT: 2.53 min Scan# 447
Delta R.T. 0.01 min
Lab File: VV017302.D
Acq: 02 Jul 2020 11:48

Instrument :
MSVOA_V
ClientSampleId :
ETYJ4DL

Tot Ion: 84 Resp: 4114
Ion Ratio Lower Upper
84 100
86 55.4 45.8 85.0
49 117.6 89.6 166.4

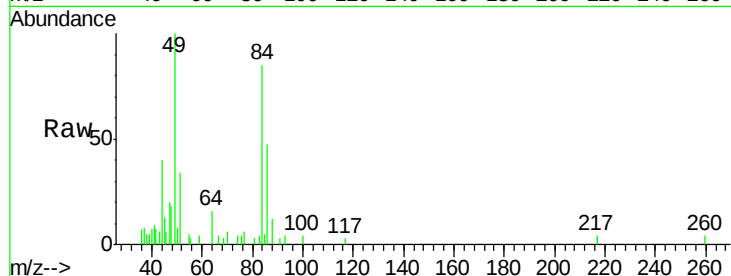


Abundance Ion 84.05 (83.75 to 84.75): VV0
Ion 86.00 (85.70 to 86.70): VV0
Ion 49.10 (48.80 to 49.80): VV0

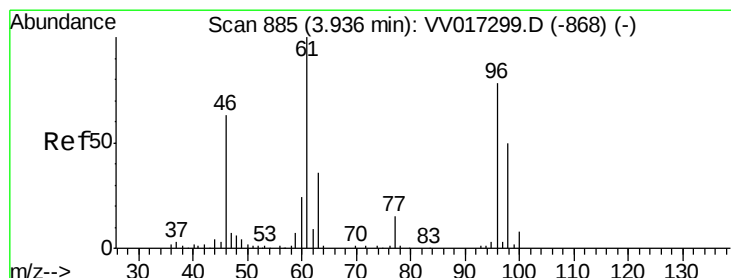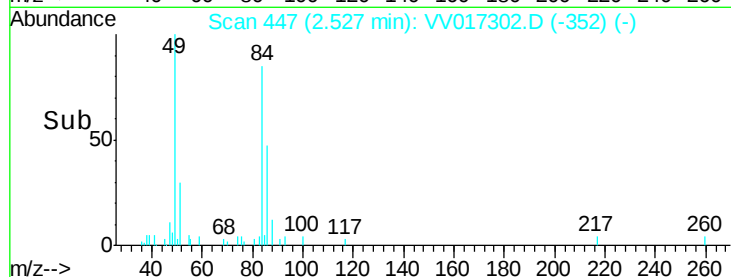
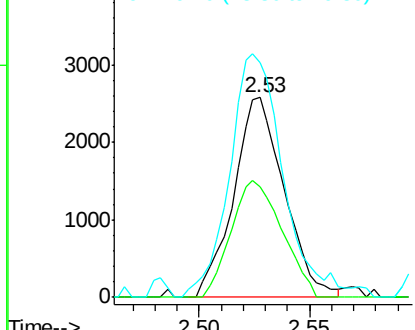





#22
cis-1,2-Dichloroethene
Concen: 0.318 ug/L
RT: 3.95 min Scan# 888
Delta R.T. 0.01 min
Lab File: VV017302.D
Acq: 02 Jul 2020 11:48

Tgt Ion: 96 Resp: 3698
Ion Ratio Lower Upper
96 100
61 130.6 91.0 169.0
68 0.0 0.0 0.0

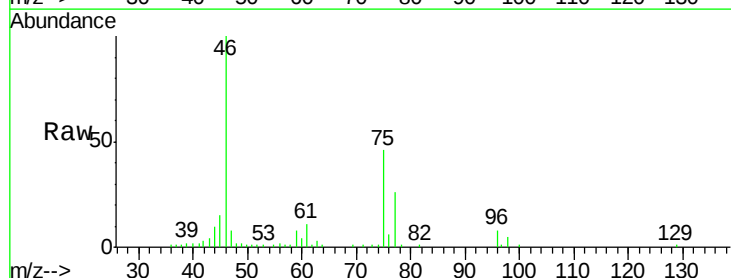

Abundance Ion 96.00 (95.70 to 96.70): VV0
Ion 61.05 (60.75 to 61.75): VV0
Ion 68.15 (67.85 to 68.85): VV0

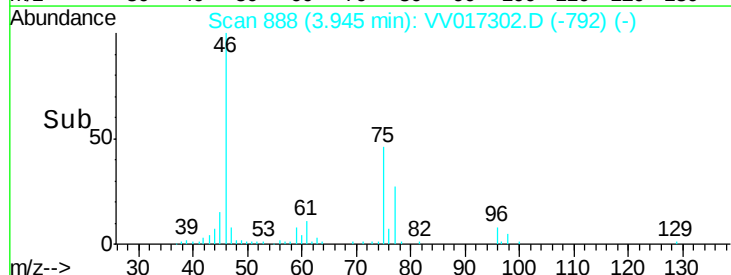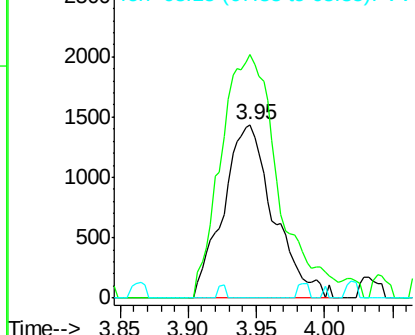

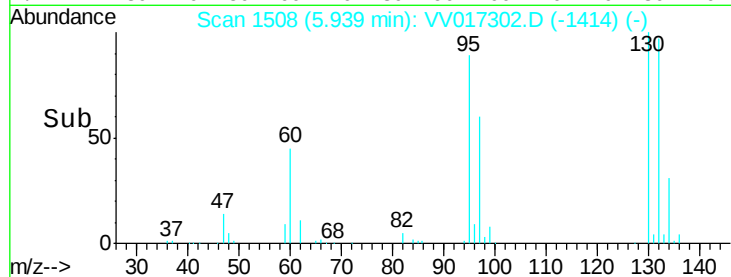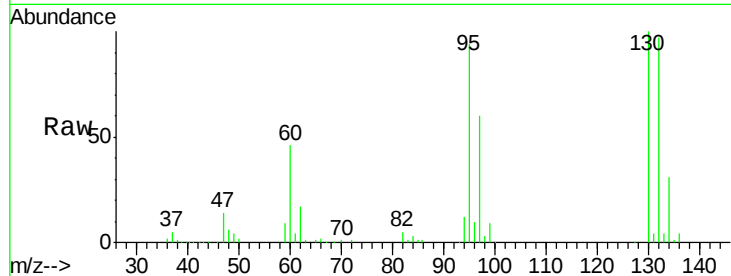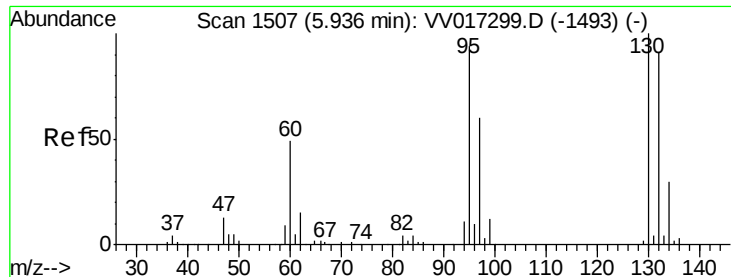

#34

Trichloroethene

Concen: 7.519 ug/L

RT: 5.94 min Scan# 1508

Delta R.T. 0.00 min

Lab File: VV017302.D

Acq: 02 Jul 2020 11:48

Instrument :

MSVOA_V

ClientSampleId :

ETYJ4DL

Tot Ion: 95 Resp: 93984

Ion Ratio Lower Upper

95 100

97 63.7 45.3 84.1

132 103.2 68.8 127.8

130 106.8 70.2 130.4

Abundance Ion 95.00 (94.70 to 95.70): VV017299.D (-1493) (-)

80000

Ion 96.95 (96.65 to 97.65): VV017299.D (-1493) (-)

60000

Ion 131.95 (131.65 to 132.65): VV017299.D (-1493) (-)

40000

Ion 129.95 (129.65 to 130.65): VV017299.D (-1493) (-)

20000

0

