

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
 Data File : VV017303.D
 Acq On : 02 Jul 2020 12:13
 Operator : SY/MD
 Sample : L3150-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETYJ7

Quant Time: Jul 03 04:31:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 03 01:13:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	148446	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	144809	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	66046	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47821	5.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.40%
7) Chloroethane-d5	1.58	69	37808	5.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.80%
11) 1,1-Dichloroethene-d2	2.13	63	74388	4.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.80%
20) 2-Butanone-d5	3.93	46	101126	44.54	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.08%
24) Chloroform-d	4.38	84	102092	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
26) 1,2-Dichloroethane-d4	5.06	65	53888	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.60%
32) Benzene-d6	5.08	84	186855	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.10	67	54279	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.34	98	167182	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
45) trans-1,3-Dichloropropene-	7.64	79	21349	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
48) 2-Hexanone-d5	8.11	63	63409	35.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	71.06%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	35214	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	63283	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
34) Trichloroethene	5.95	95	5137	0.463 ug/L	95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070220\
Data File : VV017303.D
Acq On : 02 Jul 2020 12:13
Operator : SY/MD
Sample : L3150-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETYJ7

Quant Time: Jul 03 04:31:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 03 01:13:36 2020
Response via : Initial Calibration

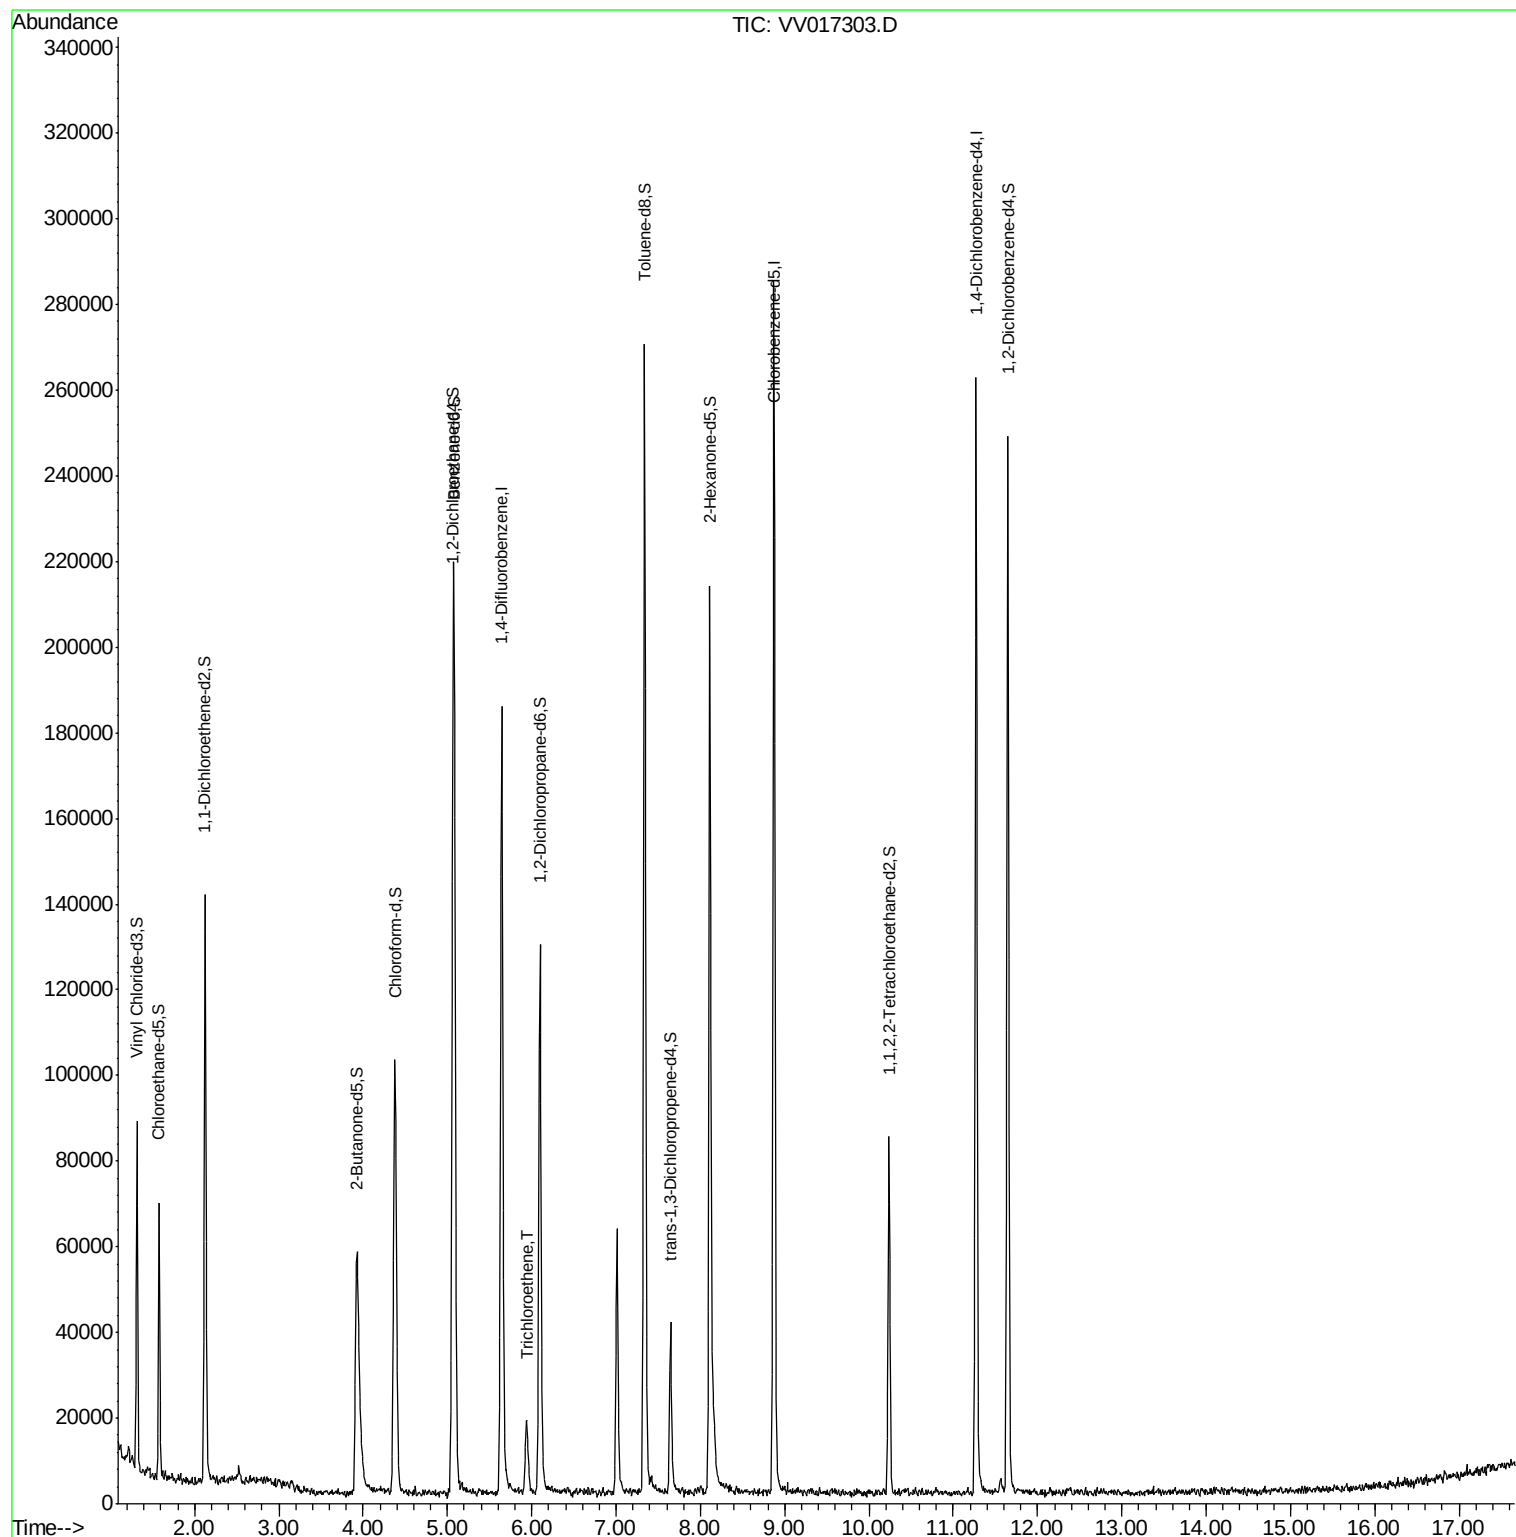

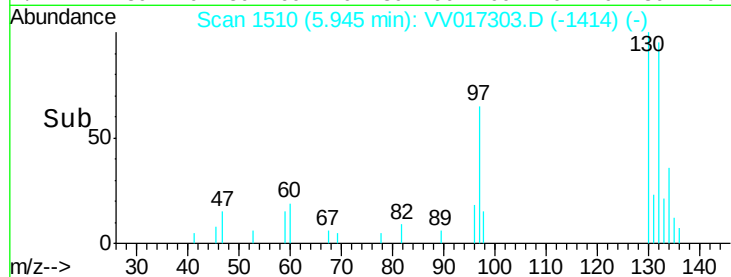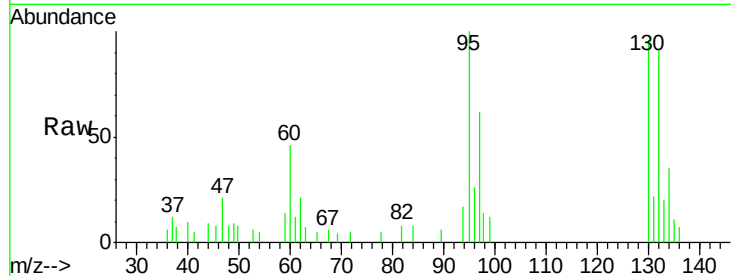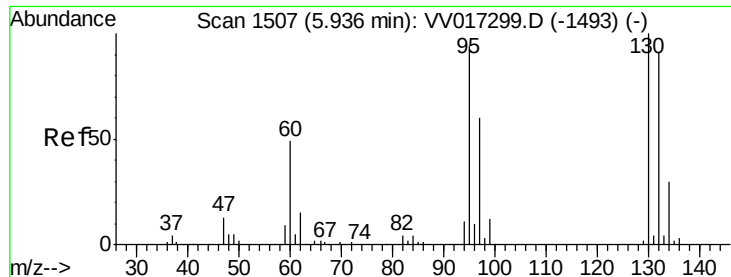

#34

Trichloroethene

Concen: 0.463 ug/L

RT: 5.95 min Scan# 1510

Delta R.T. 0.01 min

Lab File: VV017303.D

Acq: 02 Jul 2020 12:13

Instrument :

MSVOA_V

ClientSampleId :

ETYJ7

Tot Ion: 95 Resp: 5137

Ion Ratio Lower Upper

95 100

97 62.1 45.3 84.1

132 90.9 68.8 127.8

130 96.1 70.2 130.4

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

