

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
 Data File : VV017326.D
 Acq On : 02 Jul 2020 23:25
 Operator : SY/MD
 Sample : VIBLK52
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK52

Quant Time: Jul 03 07:22:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 03 06:15:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	165173	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	159260	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	79137	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	39899	4.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.40%
7) Chloroethane-d5	1.58	69	31938	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.12	63	65976	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.95	46	95392	37.76	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.52%
24) Chloroform-d	4.38	84	91774	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.60%
26) 1,2-Dichloroethane-d4	5.06	65	52108	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
32) Benzene-d6	5.08	84	169696	4.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.20%
36) 1,2-Dichloropropane-d6	6.10	67	47024	3.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.00%
41) Toluene-d8	7.34	98	152146	3.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.60%
45) trans-1,3-Dichloropropene-	7.64	79	19014	3.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.80%
48) 2-Hexanone-d5	8.11	63	64354	32.78	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	65.56%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	33441	4.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	63969	4.37	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.40%


Target Compounds					Ovalue
16) Methylene chloride	2.52	84	5619	0.662 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
Data File : VV017326.D
Acq On : 02 Jul 2020 23:25
Operator : SY/MD
Sample : VIBLK52
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK52

Quant Time: Jul 03 07:22:06 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 03 06:15:26 2020
Response via : Initial Calibration

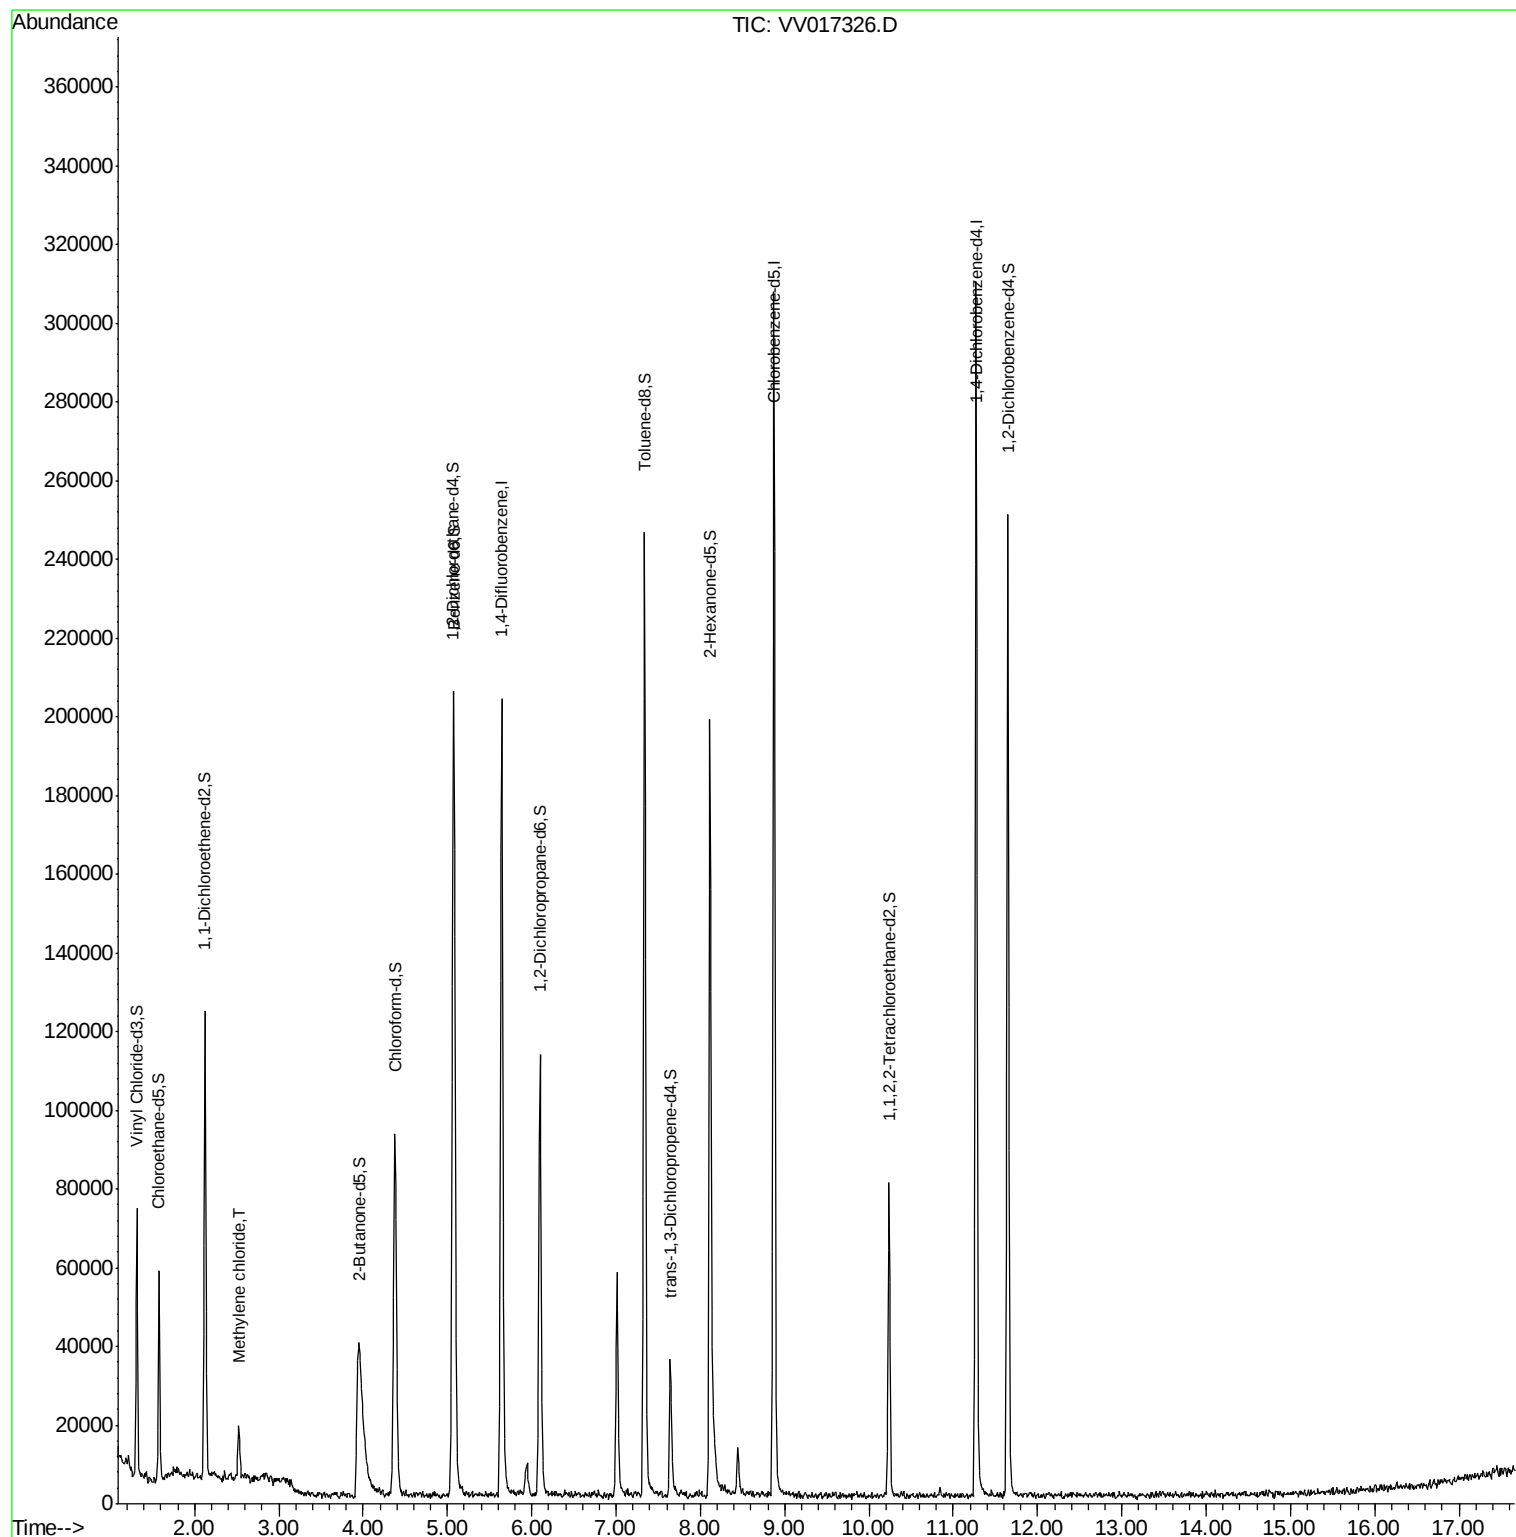

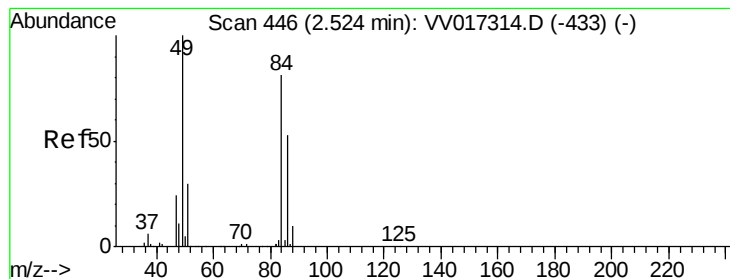

#16
 Methvlene chloride
 Concen: 0.662 ug/L
 RT: 2.52 min Scan# 445
 Delta R.T. -0.00 min
 Lab File: VV017326.D
 Acq: 02 Jul 2020 23:25

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK52

Tot Ion: 84 Resp: 5619
 Ion Ratio Lower Upper
 84 100
 86 56.2 45.8 85.0
 49 114.1 89.6 166.4

