

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
 Data File : VV017331.D
 Acq On : 03 Jul 2020 01:25
 Operator : SY/MD
 Sample : L3121-21
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 03 07:52:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 03 06:15:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	158312	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	152665	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	74265	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	41560	4.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.40%
7) Chloroethane-d5	1.58	69	32705	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.60%
11) 1,1-Dichloroethene-d2	2.12	63	67759	3.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.00%
20) 2-Butanone-d5	3.95	46	95514	39.44	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.88%
24) Chloroform-d	4.38	84	93479	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	5.06	65	53647	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.07	84	173884	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
36) 1,2-Dichloropropane-d6	6.10	67	49292	4.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.20%
41) Toluene-d8	7.34	98	158233	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.20%
45) trans-1,3-Dichloropropene-	7.65	79	19809	4.01	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.20%
48) 2-Hexanone-d5	8.11	63	63708	33.86	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.72%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	34334	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	62802	4.57	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.40%


Target Compounds					Ovalue
16) Methylene chloride	2.52	84	5471	0.672 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
Data File : VV017331.D
Acq On : 03 Jul 2020 01:25
Operator : SY/MD
Sample : L3121-21
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 03 07:52:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 03 06:15:26 2020
Response via : Initial Calibration

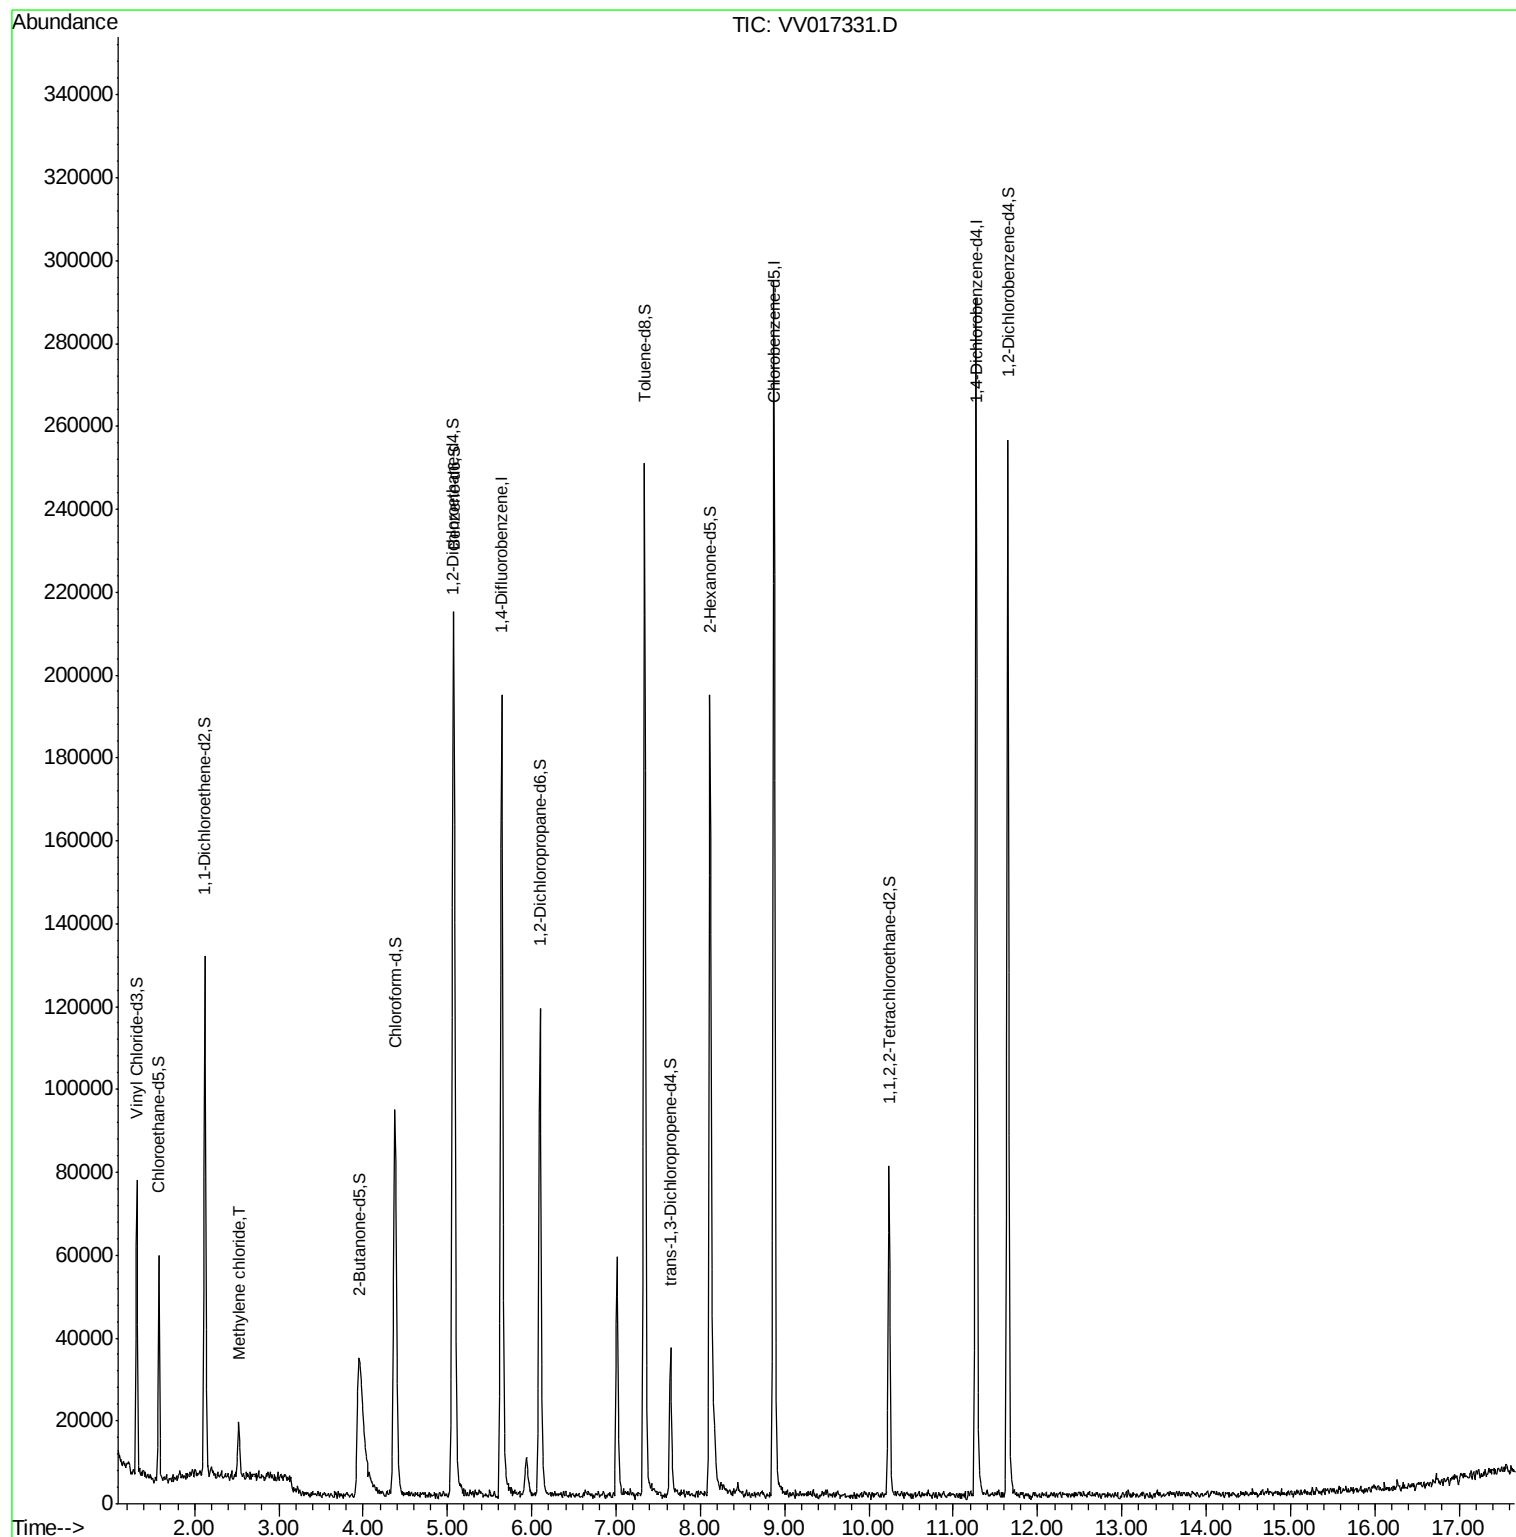

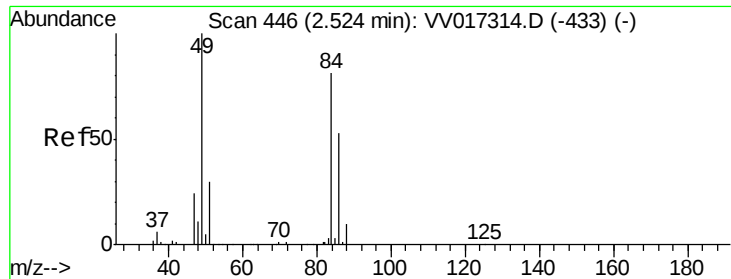

#16
 Methvlene chloride
 Concen: 0.672 ug/L
 RT: 2.52 min Scan# 446
 Delta R.T. 0.00 min
 Lab File: VV017331.D
 Acq: 03 Jul 2020 01:25

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 5471
 Ion Ratio Lower Upper
 84 100
 86 68.0 45.8 85.0
 49 130.3 89.6 166.4

