

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
 Data File : VV017332.D
 Acq On : 03 Jul 2020 01:49
 Operator : SY/MD
 Sample : L3132-11
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 03 07:54:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 03 06:15:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	156727	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	151193	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	72113	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45794	4.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.40%
7) Chloroethane-d5	1.58	69	36729	5.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.40%
11) 1,1-Dichloroethene-d2	2.12	63	73327	4.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.00%
20) 2-Butanone-d5	3.96	46	102266	42.66	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.32%
24) Chloroform-d	4.38	84	100915	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
26) 1,2-Dichloroethane-d4	5.06	65	57930	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.60%
32) Benzene-d6	5.07	84	187036	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
36) 1,2-Dichloropropane-d6	6.10	67	52399	4.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.20%
41) Toluene-d8	7.34	98	172359	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
45) trans-1,3-Dichloropropene-	7.65	79	22009	4.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.00%
48) 2-Hexanone-d5	8.12	63	70086	37.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.22%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	36369	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	67088	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	5335	0.662 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV070220\
Data File : VV017332.D
Acq On : 03 Jul 2020 01:49
Operator : SY/MD
Sample : L3132-11
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 03 07:54:58 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 03 06:15:26 2020
Response via : Initial Calibration

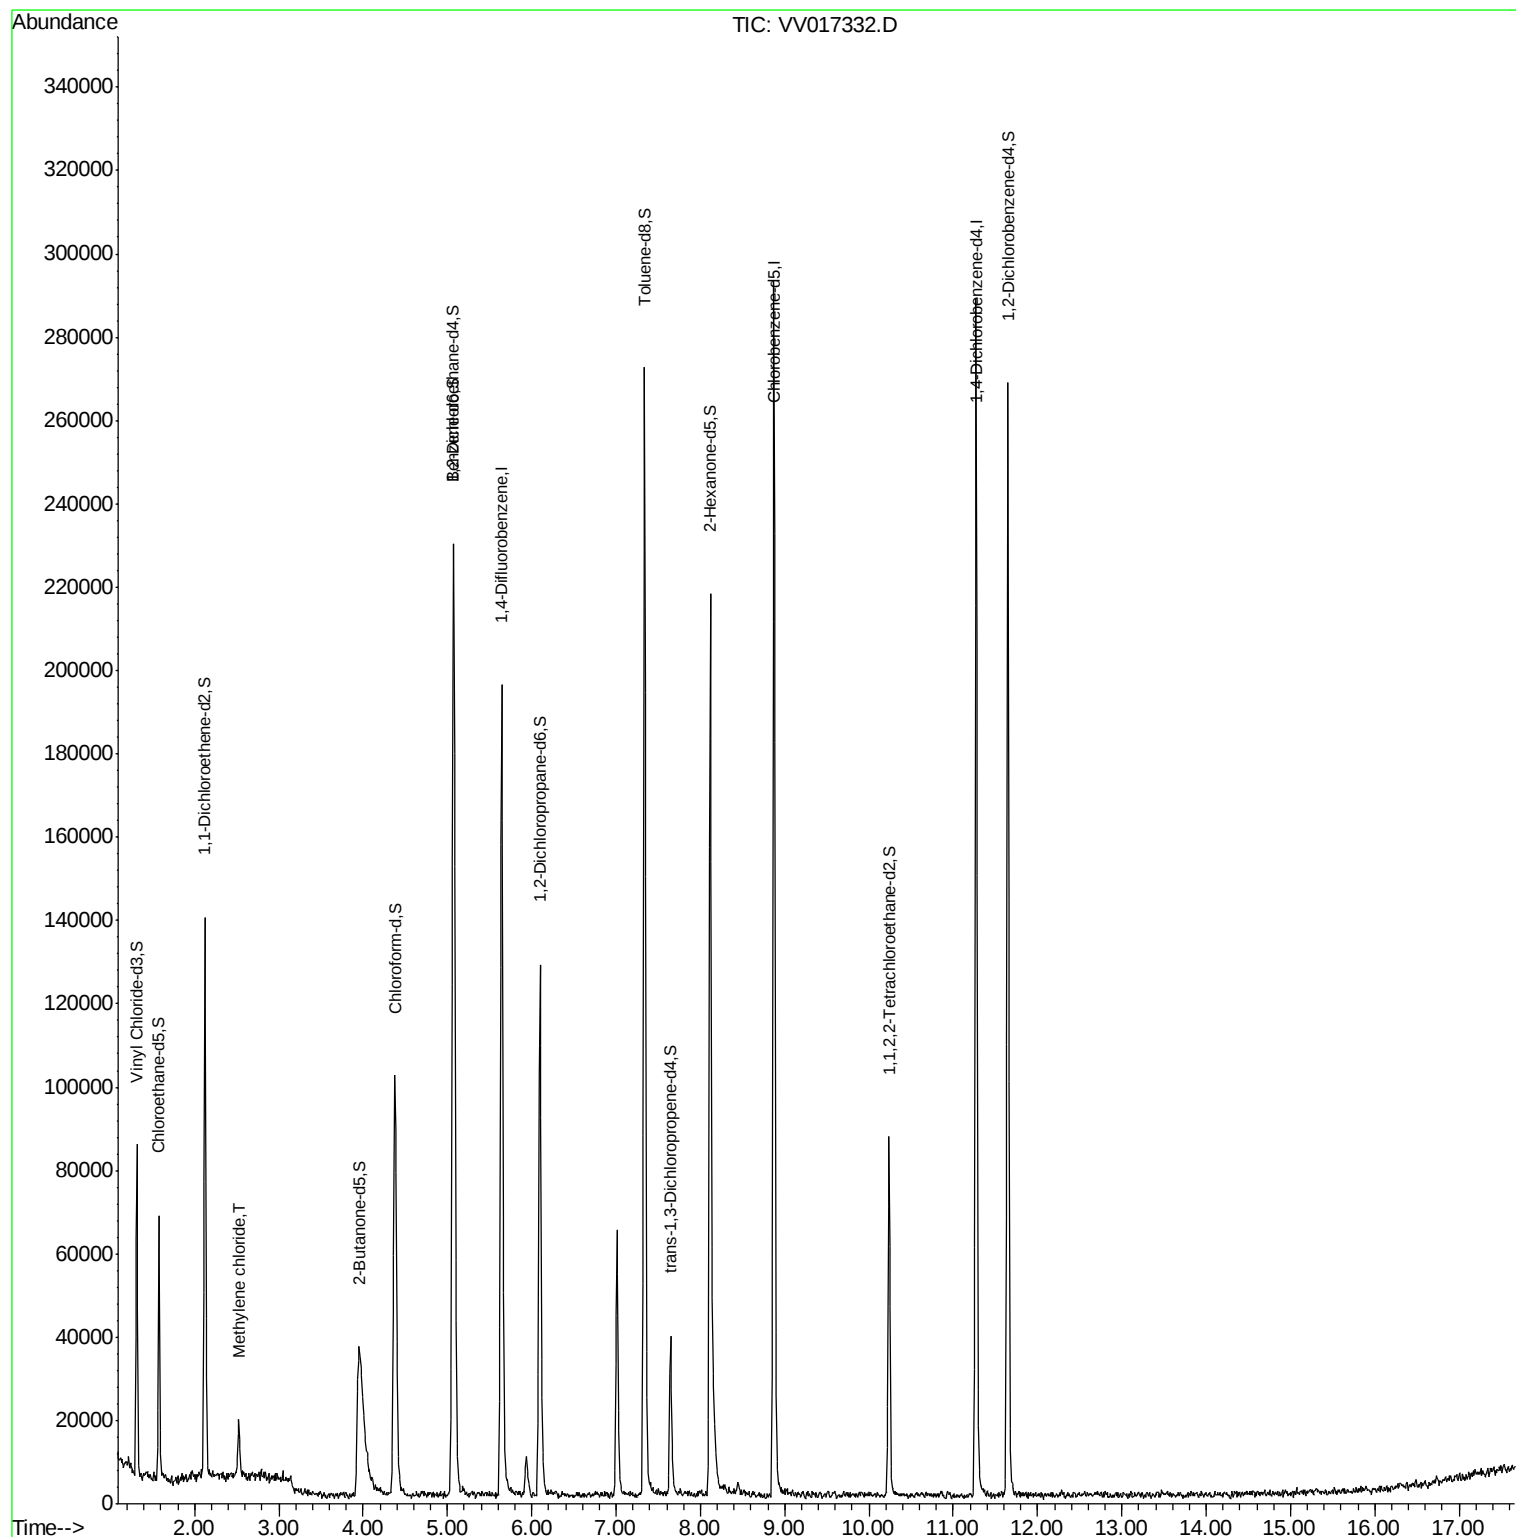

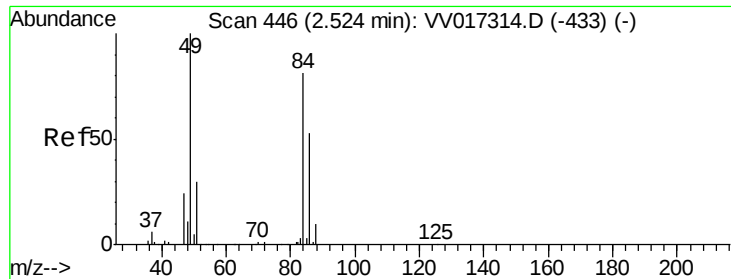

#16
 Methvlene chloride
 Concen: 0.662 ug/L
 RT: 2.53 min Scan# 447
 Delta R.T. 0.00 min
 Lab File: VV017332.D
 Acq: 03 Jul 2020 01:49

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 5335
 Ion Ratio Lower Upper
 84 100
 86 62.8 45.8 85.0
 49 131.7 89.6 166.4

