

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
 Data File : VV017335.D
 Acq On : 03 Jul 2020 03:01
 Operator : SY/MD
 Sample : L3154-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 03 08:12:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 03 06:15:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	158002	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	152736	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	73236	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	39687	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%
7) Chloroethane-d5	1.58	69	33348	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.12	63	65162	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	3.95	46	93180	38.55	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.10%
24) Chloroform-d	4.38	84	90830	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.06	65	52519	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
32) Benzene-d6	5.08	84	165800	4.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.80%
36) 1,2-Dichloropropane-d6	6.10	67	47930	4.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.80%
41) Toluene-d8	7.34	98	151029	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.20%
45) trans-1,3-Dichloropropene-	7.64	79	19788	4.01	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.20%
48) 2-Hexanone-d5	8.12	63	61087	32.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	64.90%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	32974	4.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	59997	4.43	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.60%


Target Compounds					Ovalue
16) Methylene chloride	2.52	84	3859	0.475 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
Data File : VV017335.D
Acq On : 03 Jul 2020 03:01
Operator : SY/MD
Sample : L3154-09
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 03 08:12:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 03 06:15:26 2020
Response via : Initial Calibration

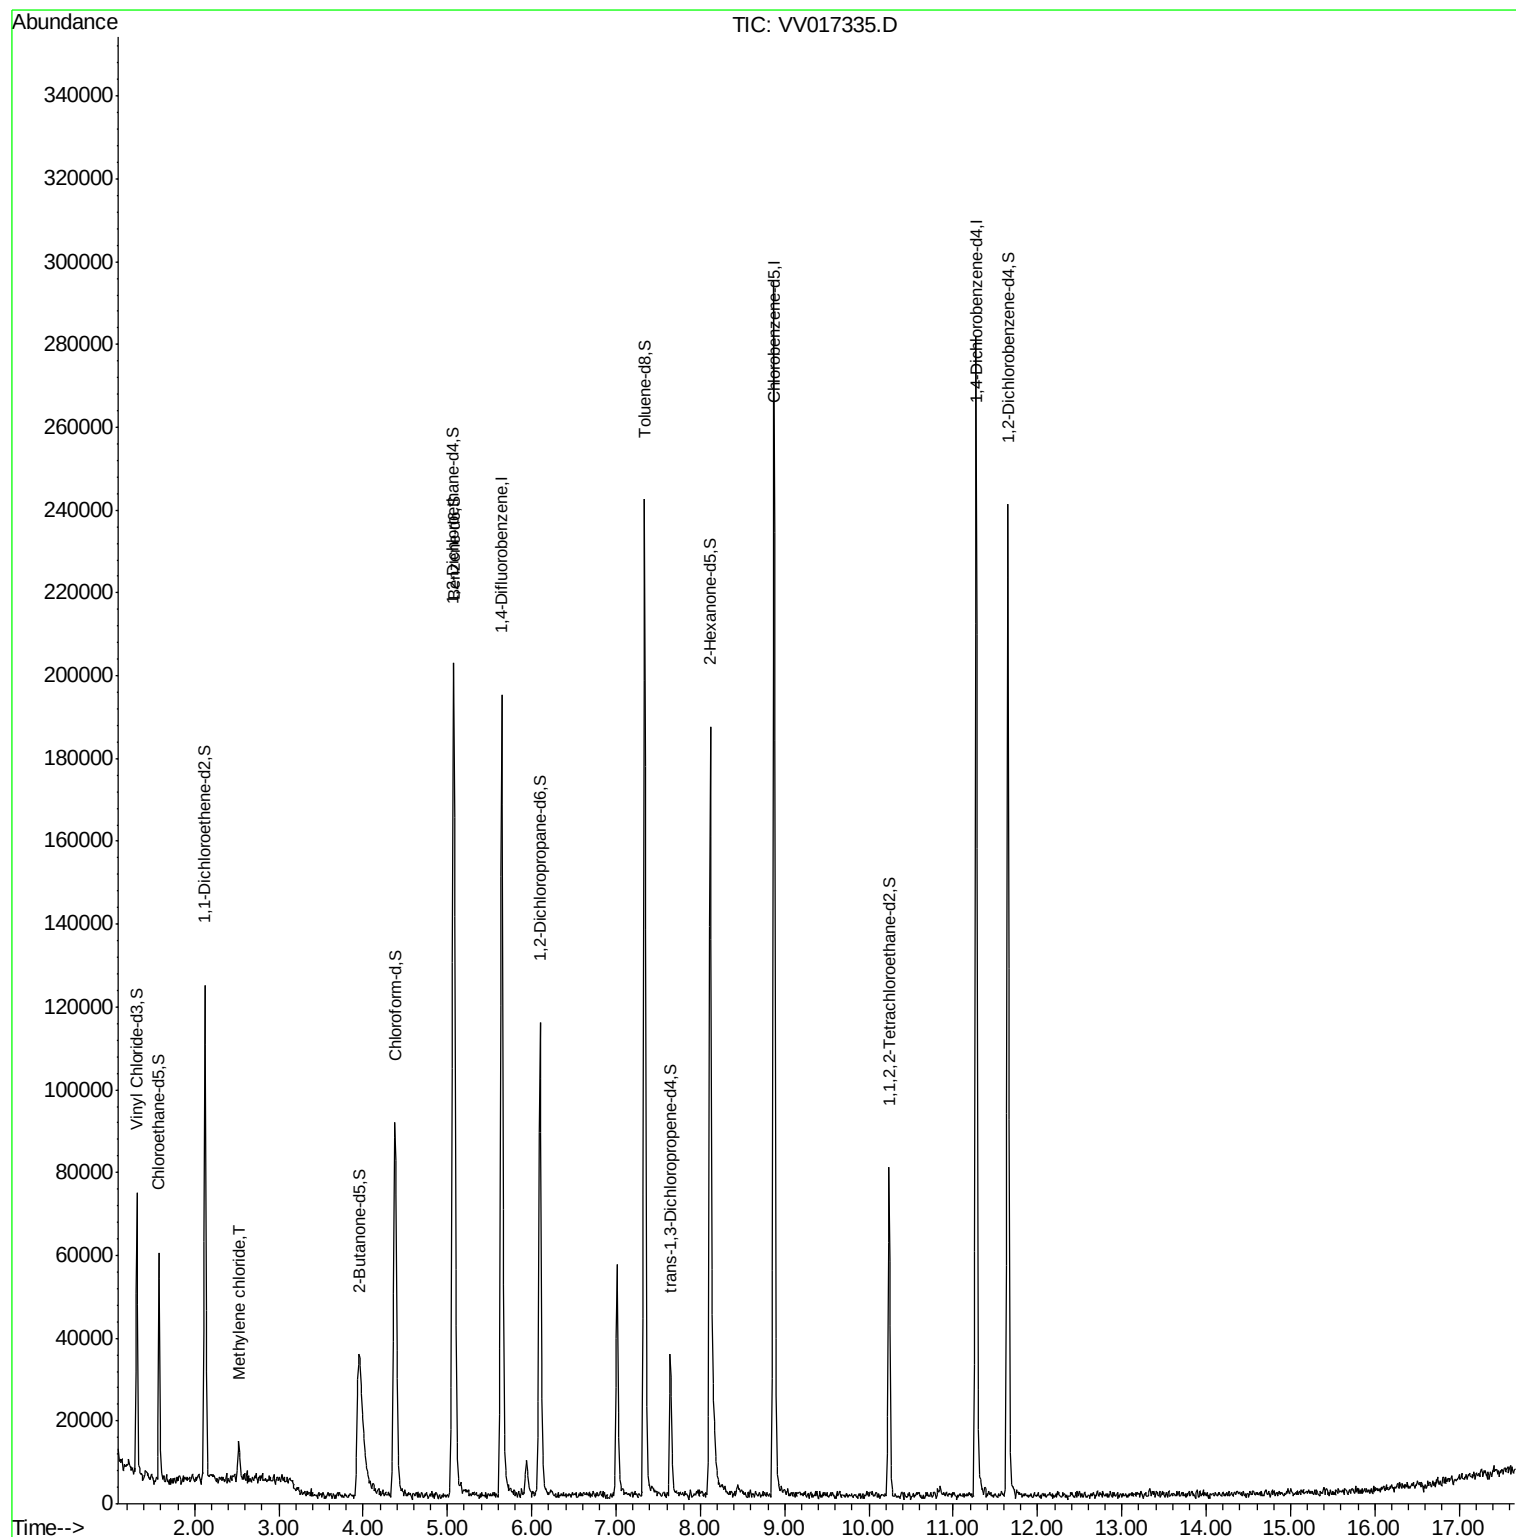

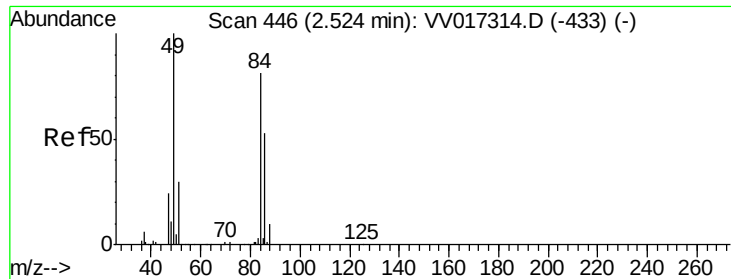

#16
 Methylene chloride
 Concen: 0.475 ug/L
 RT: 2.52 min Scan# 446
 Delta R.T. -0.00 min
 Lab File: VV017335.D
 Acq: 03 Jul 2020 03:01

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 3859
 Ion Ratio Lower Upper
 84 100
 86 51.1 45.8 85.0
 49 119.6 89.6 166.4

