


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV070220\
 Data File : VV017298.D
 Acq On : 02 Jul 2020 09:16
 Operator : SY/MD
 Sample : BFB46
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB46

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jul 06 00:46:50 2020

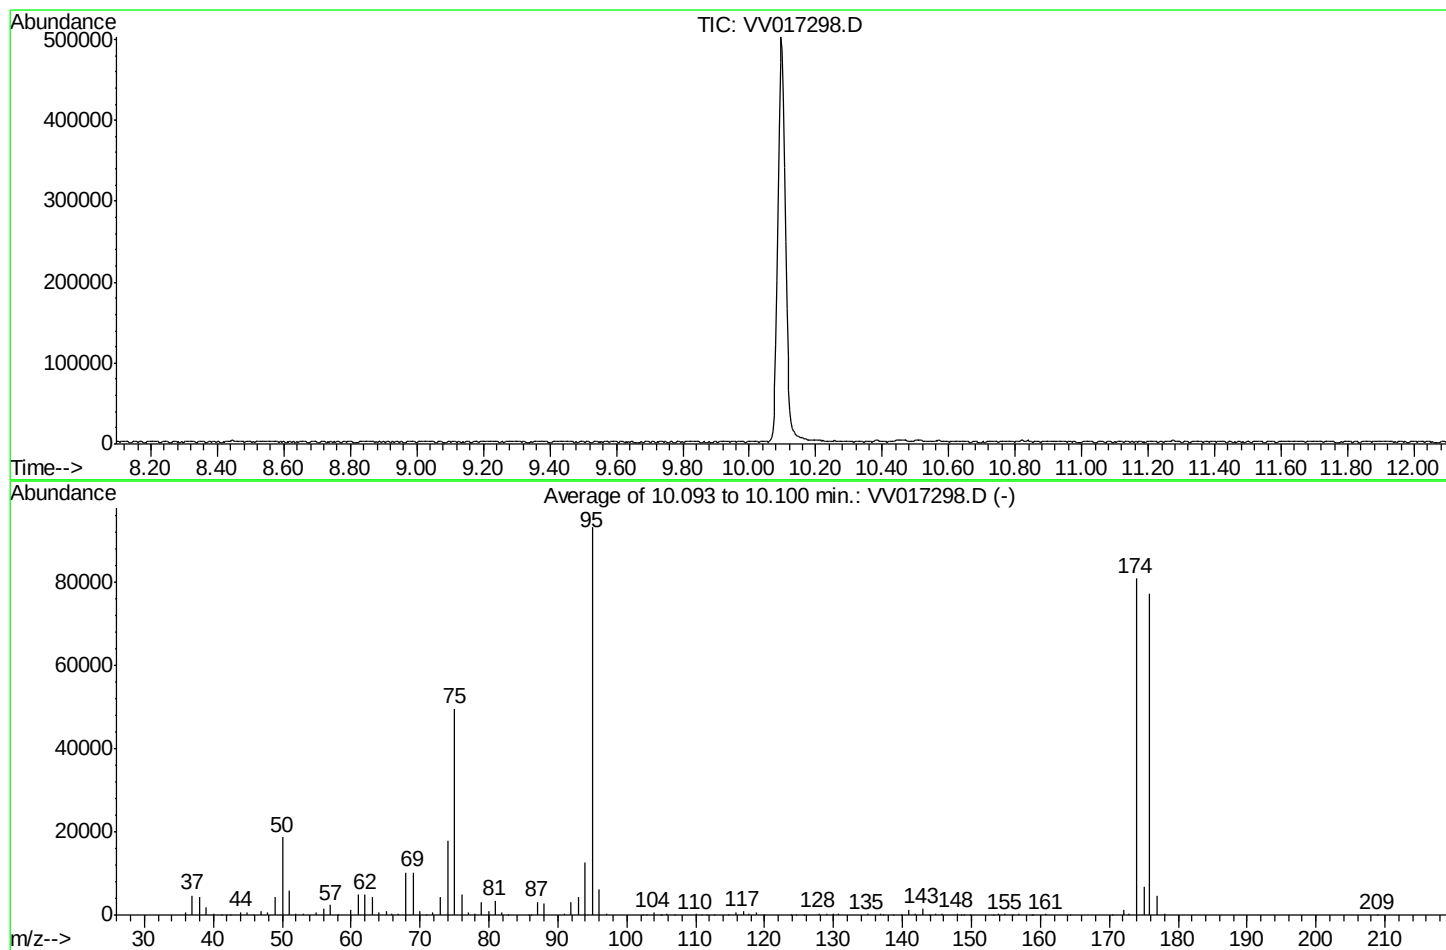

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	18789	PASS
75	95	30	80	53.2	49618	PASS
95	95	100	100	100.0	93322	PASS
96	95	5	9	6.5	6057	PASS
173	174	0.00	2	0.5	419	PASS
174	95	50	120	86.8	81034	PASS
175	174	5	9	8.2	6655	PASS
176	174	95	101	95.3	77250	PASS
177	176	5	9	6.2	4764	PASS

m/z	Abundance
35.00	135.0
35.80	169.0
36.20	105.0
36.90	160.0
37.40	116.0
38.40	126.0
39.00	159.0
40.00	174.0
42.30	112.0
43.00	182.0
44.00	255.0
44.80	146.0
46.30	150.0
48.20	143.0
51.40	126.0
57.00	171.0
96.60	106.0
107.80	105.0
213.50	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
35.20	177.0
36.00	1042.0
37.00	5040.0
38.00	4177.0
39.00	1983.0
40.10	380.0
41.10	107.0
41.90	144.0
42.50	114.0
43.00	160.0
44.00	943.0
45.00	648.0
45.90	153.0
47.00	1128.0
47.90	687.0
49.00	4018.0
50.00	17920.0
51.00	5845.0
51.90	291.0
53.00	265.0
54.90	556.0
56.00	1697.0
57.00	2719.0
58.00	107.0
60.00	1151.0
61.00	4508.0
62.00	4644.0
63.00	4103.0
64.00	692.0
65.00	929.0
65.80	261.0
66.80	319.0
68.00	9929.0
69.00	10182.0
70.00	733.0
70.90	145.0
71.90	580.0
73.00	4247.0
74.00	17560.0
75.00	48032.0
76.00	4693.0
77.00	665.0
77.80	458.0
78.90	3188.0
79.90	1204.0
80.90	3261.0
81.90	679.0
82.80	100.0
86.10	153.0
86.90	3216.0
87.90	2742.0
91.00	379.0
92.00	3050.0
93.00	4395.0
94.00	12295.0
95.00	90464.0
96.00	5898.0
97.00	268.0
102.90	148.0
103.90	480.0
104.90	169.0
105.80	446.0
106.90	131.0
110.00	171.0
110.90	112.0
111.50	107.0
112.70	126.0
115.90	516.0
116.90	747.0
117.80	475.0
118.80	689.0
124.60	126.0
127.90	416.0
129.00	180.0
129.90	314.0
130.70	187.0
134.90	248.0
136.70	183.0
137.20	170.0
139.80	125.0
140.90	1369.0
141.70	164.0
142.90	1517.0
143.90	215.0
144.80	464.0
145.70	175.0
147.90	297.0
148.60	136.0
149.80	143.0
153.20	153.0
154.00	137.0
155.00	293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

156.70	174.0
159.00	129.0
160.90	141.0
164.30	116.0
172.10	1210.0
172.90	1257.0
173.90	76728.0
175.00	6579.0
175.90	72864.0
177.00	4609.0
178.10	277.0
208.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	1025.0
37.00	4988.0
38.00	4377.0
39.00	2036.0
40.10	396.0
41.80	118.0
42.60	102.0
43.10	168.0
44.00	1108.0
45.00	702.0
47.00	1082.0
47.90	782.0
49.00	4360.0
50.00	19600.0
51.00	5962.0
51.90	327.0
53.00	264.0
54.90	586.0
56.00	1733.0
57.00	2665.0
58.00	157.0
60.00	1175.0
61.00	4981.0
62.00	5034.0
63.00	4541.0
64.00	690.0
65.00	864.0
65.90	234.0
66.90	318.0
68.00	10577.0
69.00	10565.0
70.00	861.0
70.80	131.0
71.90	666.0
73.00	4422.0
74.00	18392.0
75.00	51224.0
76.00	5006.0
77.00	733.0
77.80	459.0
78.90	3309.0
79.90	1051.0
80.90	3548.0
81.90	804.0
85.70	104.0
86.20	169.0
86.90	3253.0
87.90	3029.0
90.90	400.0
92.00	3168.0
93.00	4589.0
94.00	13251.0
95.00	96568.0
96.00	6298.0
97.00	287.0
102.30	121.0
102.90	146.0
103.80	551.0
105.10	187.0
105.80	390.0
106.90	162.0
110.00	212.0
110.80	154.0
114.70	122.0
115.80	486.0
116.90	798.0
117.70	452.0
118.80	763.0
127.90	419.0
129.00	176.0
129.90	365.0
130.70	199.0
134.90	254.0
136.70	198.0
137.30	177.0
138.70	107.0
139.80	133.0
140.90	1380.0
141.80	172.0
142.90	1562.0
143.90	164.0
144.90	386.0
145.80	194.0
147.90	370.0
148.80	138.0
149.80	153.0
153.20	143.0
153.90	179.0
154.90	329.0
156.80	223.0
158.60	108.0
158.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

160.80	193.0
164.30	157.0
170.50	119.0
172.10	1247.0
173.90	83552.0
175.00	6912.0
175.90	80248.0
177.00	4871.0
178.10	254.0
208.90	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	946.0
37.00	4484.0
38.00	4132.0
39.00	2024.0
40.10	445.0
43.10	212.0
44.00	1049.0
45.00	752.0
46.30	177.0
46.90	965.0
48.00	745.0
49.00	4360.0
50.00	18848.0
51.00	5636.0
51.90	317.0
53.10	235.0
54.90	533.0
56.00	1646.0
57.00	2425.0
58.00	172.0
59.90	1048.0
61.00	5062.0
62.00	4892.0
63.00	4433.0
64.00	665.0
65.10	870.0
66.00	190.0
66.80	363.0
68.00	10080.0
69.00	9958.0
69.90	836.0
71.90	621.0
73.00	4452.0
74.00	17448.0
75.00	49600.0
76.00	4881.0
76.90	690.0
77.90	369.0
78.90	3199.0
80.00	974.0
80.90	3542.0
81.90	844.0
82.90	123.0
85.60	154.0
86.10	132.0
87.00	3064.0
87.90	3004.0
90.90	419.0
91.90	3068.0
93.00	4327.0
94.00	12433.0
95.00	92936.0
96.00	5977.0
97.10	285.0
102.30	111.0
102.80	126.0
103.80	544.0
105.10	199.0
105.80	340.0
106.90	138.0
110.00	224.0
110.70	181.0
114.80	189.0
115.80	444.0
116.90	849.0
117.70	468.0
118.80	699.0
120.00	122.0
123.90	137.0
125.70	108.0
127.90	411.0
129.00	183.0
129.90	372.0
130.80	175.0
134.90	239.0
136.80	226.0
138.70	119.0
139.80	155.0
140.90	1170.0
141.90	224.0
142.90	1415.0
143.90	112.0
144.90	284.0
145.80	237.0
147.90	380.0
148.90	177.0
149.70	143.0
153.80	191.0
154.80	306.0
156.00	107.0
156.90	287.0
158.70	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

160.80	234.0
164.30	128.0
172.10	1204.0
173.90	82824.0
175.00	6476.0
175.90	78640.0
177.00	4813.0
177.90	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46