

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
 Data File : VV021592.D
 Acq On : 02 Jul 2021 12:12
 Operator : SY/MD
 Sample : M2914-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBK50

Quant Time: Jul 03 00:07:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 03 00:01:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	482237	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	447375	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	216573	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	22527	7.383	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	14.760%#	
7) Chloroethane-d5	1.564	69	23116	9.270	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	18.540%#	
11) 1,1-Dichloroethene-d2	2.105	63	36692	6.573	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	13.140%#	
21) 2-Butanone-d5	3.883	46	320750	123.091	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	123.090%	
24) Chloroform-d	4.349	84	67063	10.508	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	21.020%#	
26) 1,2-Dichloroethane-d4	5.031	65	42702	11.355	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	22.720%#	
32) Benzene-d6	5.050	84	134857	10.736	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	21.480%#	
36) 1,2-Dichloropropane-d6	6.069	67	45450	11.472	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	22.940%#	
41) Toluene-d8	7.317	98	123535	10.634	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	21.260%#	
43) trans-1,3-Dichloroprop...	7.625	79	18573	9.424	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	18.840%#	
47) 2-Hexanone-d5	8.085	63	190788	103.817	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	103.820%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	55871	10.467	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	20.940%#	
66) 1,2-Dichlorobenzene-d4	11.625	152	51153	11.847	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	23.700%#	
Target Compounds						
					Qvalue	
48) 2-Hexanone	8.143	43	30777	7.495	ug/L #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
Data File : VV021592.D
Acq On : 02 Jul 2021 12:12
Operator : SY/MD
Sample : M2914-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBK50


Quant Time: Jul 03 00:07:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 03 00:01:46 2021
Response via : Initial Calibration

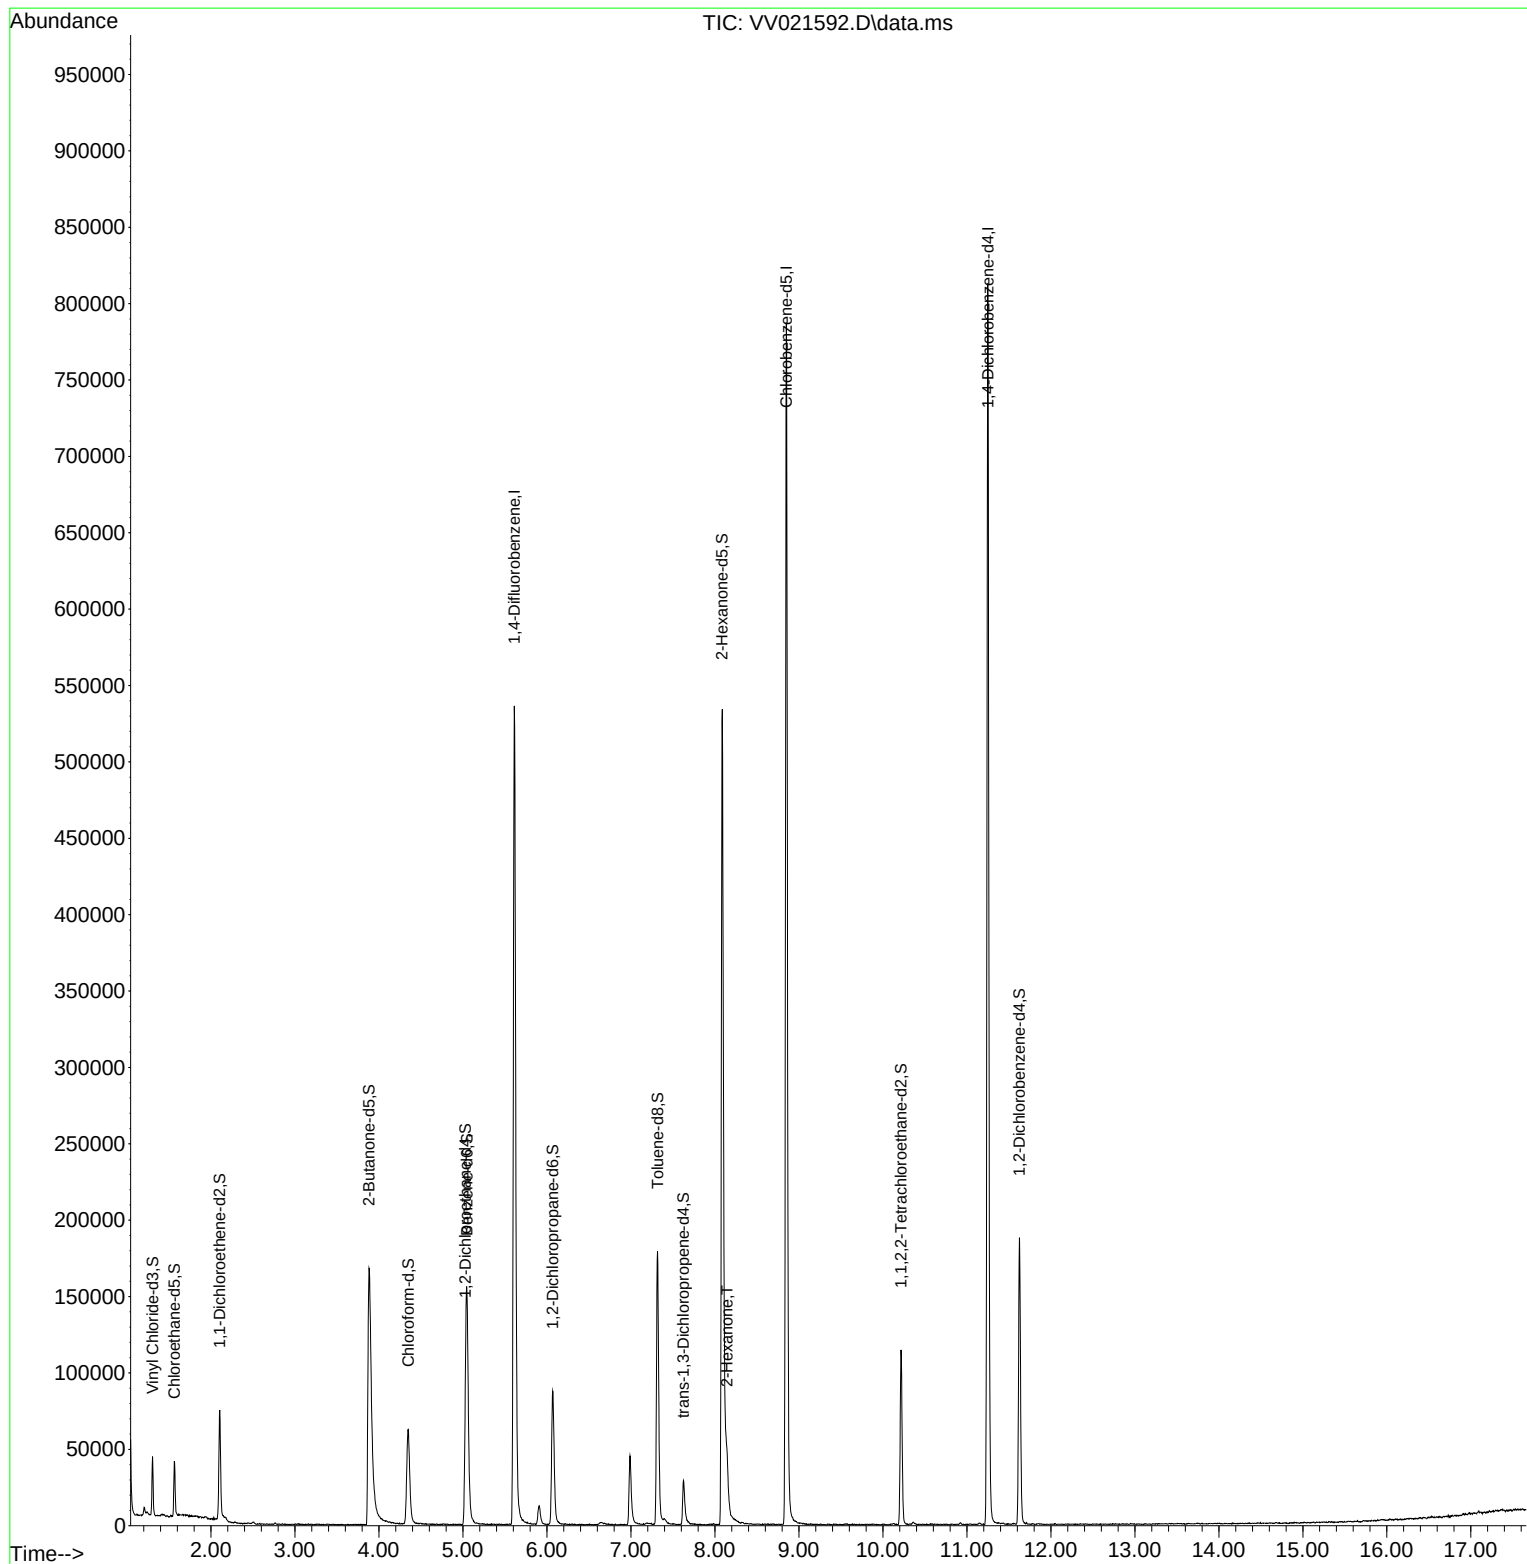

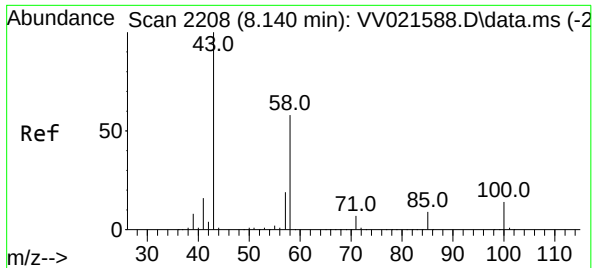

#48
2-Hexanone
Concen: 7.495 ug/L
RT: 8.143 min Scan# 2209
Delta R.T. 0.003 min
Lab File: VV021592.D
Acq: 02 Jul 2021 12:12

Instrument :
MSVOA_V
ClientSampleId :
DBK50

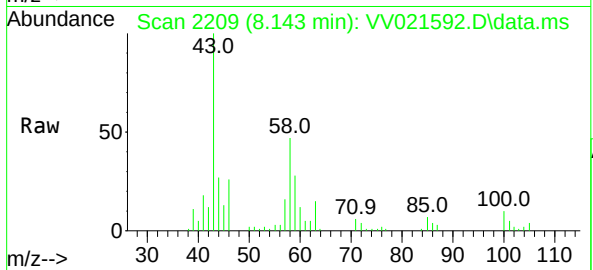

Tgt Ion: 43 Resp: 30777
Ion Ratio Lower Upper
43 100
58 42.3 46.7 70.1#
57 13.2 15.5 23.3#
100 7.8 11.0 16.4#

