

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
 Data File : VV021592.D
 Acq On : 02 Jul 2021 12:12
 Operator : SY/MD
 Sample : M2914-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBK50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	94	rVB	38872	39869	3.11%	0.558%
2	1.564	158	163	176	rVB	35542	40647	3.17%	0.568%
3	2.105	323	331	343	rBV	69232	96517	7.53%	1.350%
4	2.552	468	470	473	rBB2	380	172	0.01%	0.002%
5	2.635	494	496	499	rBV	366	264	0.02%	0.004%
6	2.699	513	516	519	rBV3	291	201	0.02%	0.003%
7	2.764	530	536	543	rVB4	1131	1431	0.11%	0.020%
8	2.902	576	579	584	rBV3	303	302	0.02%	0.004%
9	3.002	607	610	615	rBV2	545	479	0.04%	0.007%
10	3.127	647	649	654	rVV4	354	298	0.02%	0.004%
11	3.320	706	709	712	rBV2	373	238	0.02%	0.003%
12	3.375	722	726	728	rBV3	392	296	0.02%	0.004%
13	3.539	774	777	781	rVB2	246	185	0.01%	0.003%
14	3.568	784	786	792	rVB3	297	246	0.02%	0.003%
15	3.632	804	806	808	rVB	337	148	0.01%	0.002%
16	3.706	826	829	832	rBV2	317	247	0.02%	0.003%
17	3.738	837	839	842	rBV3	293	160	0.01%	0.002%
18	3.783	850	853	856	rBV2	221	172	0.01%	0.002%
19	3.883	873	884	928	rBV	167794	519954	40.55%	7.271%
20	4.349	1013	1029	1058	rBV	61763	158158	12.33%	2.212%
21	4.561	1092	1095	1097	rVB2	649	342	0.03%	0.005%
22	4.658	1123	1125	1128	rVB2	613	336	0.03%	0.005%
23	4.690	1128	1135	1138	rBV3	669	761	0.06%	0.011%
24	4.760	1155	1157	1162	rBV2	506	463	0.04%	0.006%
25	4.851	1183	1185	1188	rBV3	306	192	0.01%	0.003%
26	4.876	1191	1193	1196	rVV2	375	267	0.02%	0.004%
27	4.908	1198	1203	1205	rBV	395	323	0.03%	0.005%
28	5.043	1227	1245	1278	rBV2	156074	404334	31.53%	5.655%
29	5.310	1326	1328	1330	rBV2	351	168	0.01%	0.002%
30	5.342	1336	1338	1341	rBV3	532	267	0.02%	0.004%
31	5.426	1360	1364	1365	rBV2	348	207	0.02%	0.003%
32	5.490	1380	1384	1386	rBV	226	200	0.02%	0.003%
33	5.513	1388	1391	1393	rBV2	366	150	0.01%	0.002%
34	5.526	1393	1395	1400	rVB4	471	305	0.02%	0.004%
35	5.551	1400	1403	1405	rBV	547	390	0.03%	0.005%
36	5.613	1409	1422	1447	rBV	535892	1080090	84.23%	15.105%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
 Data File : VV021592.D
 Acq On : 02 Jul 2021 12:12
 Operator : SY/MD
 Sample : M2914-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBK50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.908	1502	1514	1529	rBV2	12303	27018	2.11%	0.378%
38	6.011	1543	1546	1548	rVB2	372	167	0.01%	0.002%
39	6.069	1552	1564	1583	rVV	86868	182787	14.25%	2.556%
40	6.214	1607	1609	1612	rBV3	503	320	0.02%	0.004%
41	6.288	1630	1632	1636	rVV2	342	245	0.02%	0.003%
42	6.381	1658	1661	1663	rBV2	297	180	0.01%	0.003%
43	6.394	1663	1665	1668	rVB	472	220	0.02%	0.003%
44	6.416	1668	1672	1677	rVB2	470	361	0.03%	0.005%
45	6.506	1697	1700	1707	rVB4	515	398	0.03%	0.006%
46	6.564	1715	1718	1721	rBV	208	143	0.01%	0.002%
47	6.735	1769	1771	1773	rVB	481	164	0.01%	0.002%
48	6.818	1791	1797	1798	rBV2	410	334	0.03%	0.005%
49	6.883	1812	1817	1820	rBV2	350	361	0.03%	0.005%
50	6.989	1839	1850	1872	rBV	45123	87129	6.79%	1.218%
51	7.149	1898	1900	1903	rBV3	605	287	0.02%	0.004%
52	7.182	1903	1910	1912	rBV4	862	920	0.07%	0.013%
53	7.268	1934	1937	1939	rBV2	424	209	0.02%	0.003%
54	7.317	1939	1952	1972	rBV	178795	320610	25.00%	4.484%
55	7.590	2035	2037	2039	rBV	279	150	0.01%	0.002%
56	7.625	2039	2048	2065	rBV	28762	54667	4.26%	0.765%
57	7.915	2133	2138	2140	rVB3	287	185	0.01%	0.003%
58	7.934	2140	2144	2147	rBV3	524	472	0.04%	0.007%
59	7.979	2155	2158	2165	rBV5	663	742	0.06%	0.010%
60	8.088	2181	2192	2233	rBV2	533594	1090586	85.05%	15.252%
61	8.567	2339	2341	2343	rVB2	476	187	0.01%	0.003%
62	8.667	2369	2372	2375	rVB3	559	424	0.03%	0.006%
63	8.693	2375	2380	2384	rBV5	706	758	0.06%	0.011%
64	8.709	2384	2385	2390	rVB	353	144	0.01%	0.002%
65	8.735	2390	2393	2396	rBV	255	169	0.01%	0.002%
66	8.760	2399	2401	2406	rVB3	662	404	0.03%	0.006%
67	8.786	2406	2409	2411	rBV3	413	261	0.02%	0.004%
68	8.850	2417	2429	2456	rBV	786565	1282313	100.00%	17.933%
69	9.182	2530	2532	2535	rBV2	311	163	0.01%	0.002%
70	9.259	2553	2556	2562	rVB3	460	345	0.03%	0.005%
71	9.342	2579	2582	2585	rBV3	465	373	0.03%	0.005%
72	9.365	2588	2589	2591	rVB3	373	143	0.01%	0.002%
73	9.416	2603	2605	2608	rVB	432	206	0.02%	0.003%
74	9.500	2629	2631	2634	rVB	349	153	0.01%	0.002%
75	9.545	2636	2645	2647	rBV4	580	619	0.05%	0.009%
76	9.558	2647	2649	2653	rVB2	370	227	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
 Data File : VV021592.D
 Acq On : 02 Jul 2021 12:12
 Operator : SY/MD
 Sample : M2914-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.641	2671	2675	2678	rVV2	513	277	0.02%	0.004%
78	9.661	2678	2681	2685	rVB2	374	320	0.02%	0.004%
79	9.744	2702	2707	2709	rBV2	433	280	0.02%	0.004%
80	9.789	2716	2721	2724	rBV3	450	361	0.03%	0.005%
81	9.841	2734	2737	2738	rBV	254	162	0.01%	0.002%
82	10.095	2815	2816	2818	rBV	375	188	0.01%	0.003%
83	10.217	2843	2854	2872	rBV	114358	183826	14.34%	2.571%
84	10.429	2918	2920	2924	rBV2	316	256	0.02%	0.004%
85	10.616	2976	2978	2982	rBV3	269	157	0.01%	0.002%
86	10.805	3035	3037	3041	rBV	321	246	0.02%	0.003%
87	10.886	3059	3062	3064	rBV2	302	177	0.01%	0.002%
88	10.921	3067	3073	3079	rBV6	1139	1477	0.12%	0.021%
89	11.127	3134	3137	3138	rBV	359	169	0.01%	0.002%
90	11.198	3157	3159	3161	rVB	581	212	0.02%	0.003%
91	11.249	3163	3175	3201	rBV	812450	1252655	97.69%	17.518%
92	11.497	3249	3252	3256	rBV2	483	303	0.02%	0.004%
93	11.545	3264	3267	3269	rBV2	582	365	0.03%	0.005%
94	11.625	3280	3292	3310	rBV	187522	302523	23.59%	4.231%
95	11.776	3336	3339	3343	rBV3	675	523	0.04%	0.007%
96	11.831	3354	3356	3359	rBV3	387	307	0.02%	0.004%
97	12.050	3422	3424	3429	rVB2	693	457	0.04%	0.006%
98	12.590	3590	3592	3593	rBV2	429	178	0.01%	0.002%
99	12.734	3636	3637	3644	rVB3	438	339	0.03%	0.005%
100	14.159	4078	4080	4083	rBV3	780	509	0.04%	0.007%




Sum of corrected areas: 7150590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
Data File : VV021592.D
Acq On : 02 Jul 2021 12:12
Operator : SY/MD
Sample : M2914-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBK50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

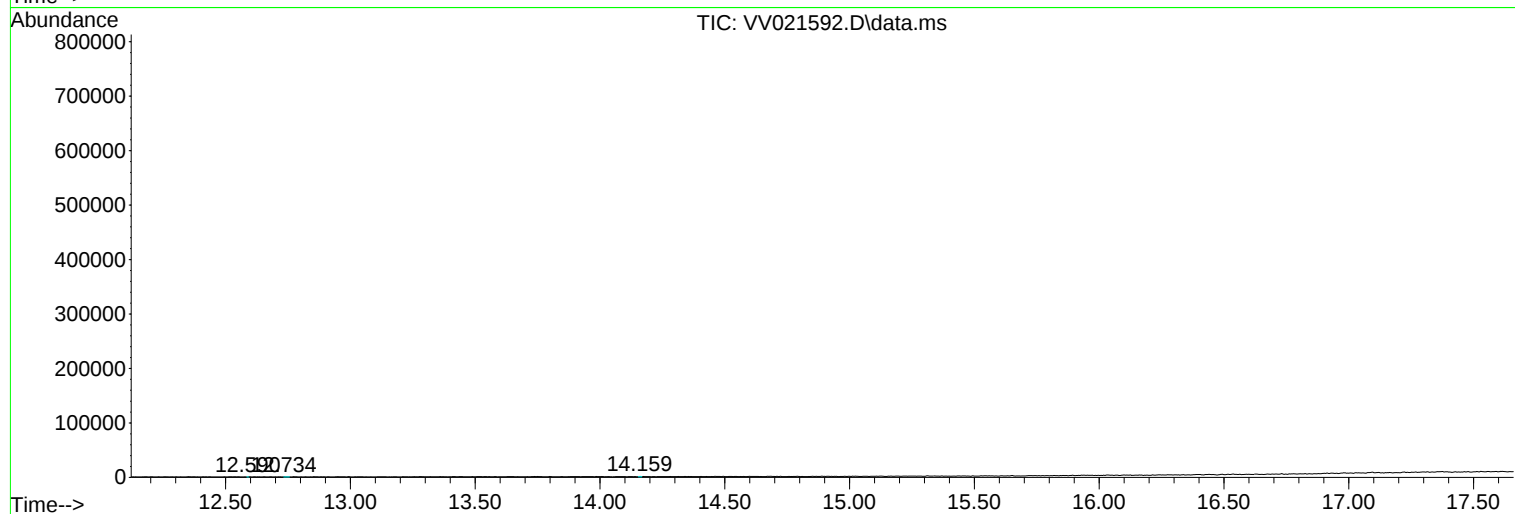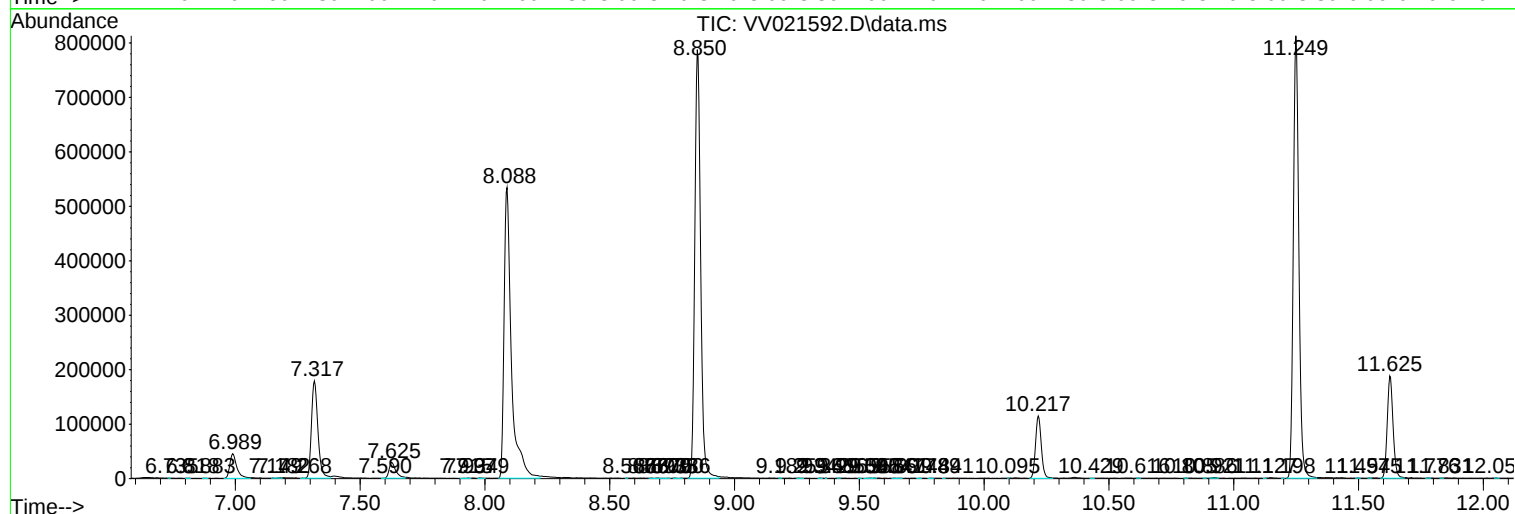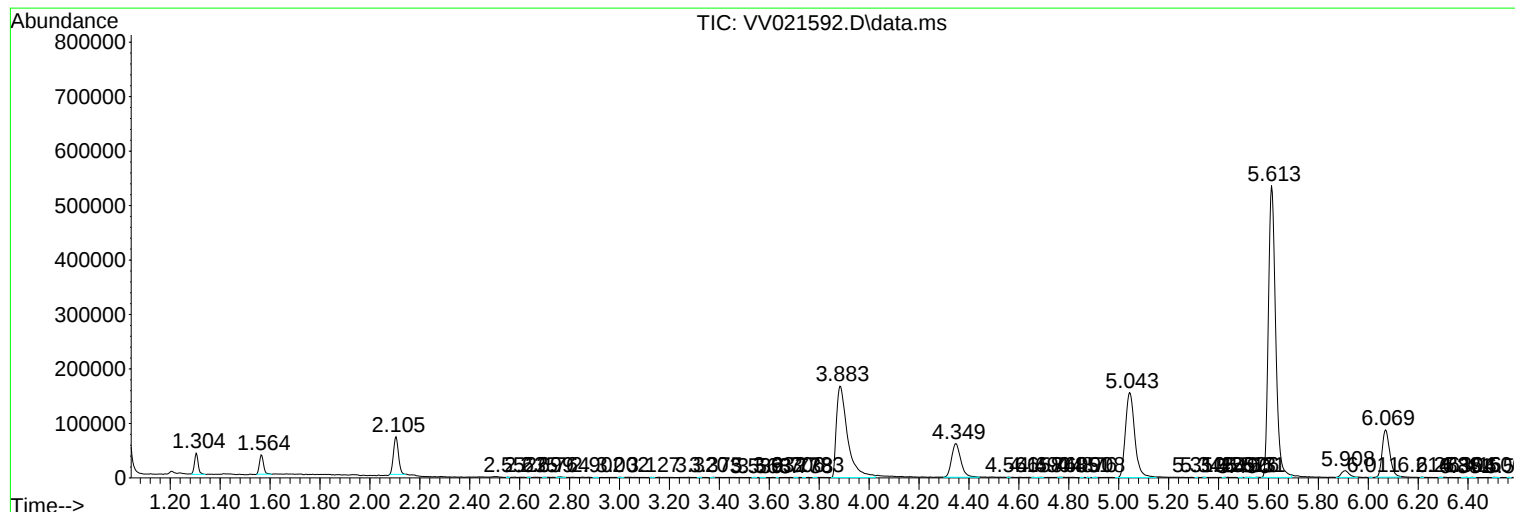

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
Data File : VV021592.D
Acq On : 02 Jul 2021 12:12
Operator : SY/MD
Sample : M2914-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBK50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
Data File : VV021592.D
Acq On : 02 Jul 2021 12:12
Operator : SY/MD
Sample : M2914-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBK50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
