

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
 Data File : VV021600.D
 Acq On : 02 Jul 2021 16:06
 Operator : SY/MD
 Sample : VIBLK161
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	191467	187868	11.86%	1.467%
2	1.558	155	161	181	rVB	154261	181279	11.45%	1.416%
3	2.105	322	331	345	rVB	325159	471585	29.78%	3.683%
4	2.506	449	456	467	rVB3	6188	10654	0.67%	0.083%
5	2.551	467	470	473	rBV3	637	492	0.03%	0.004%
6	2.748	528	531	536	rVB3	420	273	0.02%	0.002%
7	2.828	551	556	557	rBV2	302	195	0.01%	0.002%
8	3.024	615	617	619	rBV2	340	166	0.01%	0.001%
9	3.121	645	647	650	rBV2	455	315	0.02%	0.002%
10	3.217	672	677	682	rBV4	359	453	0.03%	0.004%
11	3.259	685	690	691	rBV	244	170	0.01%	0.001%
12	3.288	697	699	701	rBV	397	179	0.01%	0.001%
13	3.407	733	736	738	rBV	286	215	0.01%	0.002%
14	3.449	745	749	753	rBV2	285	212	0.01%	0.002%
15	3.513	766	769	771	rVB3	345	202	0.01%	0.002%
16	3.648	808	811	813	rBV	339	156	0.01%	0.001%
17	3.677	816	820	823	rVB2	201	174	0.01%	0.001%
18	3.715	828	832	836	rBV2	353	363	0.02%	0.003%
19	3.873	871	881	922	rBV	153133	420811	26.58%	3.287%
20	4.349	1013	1029	1065	rBV	253917	626613	39.57%	4.894%
21	4.677	1127	1131	1135	rBV3	411	396	0.03%	0.003%
22	4.783	1163	1164	1168	rVB3	334	163	0.01%	0.001%
23	4.857	1183	1187	1189	rBV	334	286	0.02%	0.002%
24	4.876	1189	1193	1197	rVB2	261	245	0.02%	0.002%
25	4.918	1204	1206	1208	rBV3	348	166	0.01%	0.001%
26	5.047	1229	1246	1277	rBV2	619215	1583401	100.00%	12.366%
27	5.374	1344	1348	1351	rBV3	460	356	0.02%	0.003%
28	5.452	1368	1372	1377	rBV3	458	471	0.03%	0.004%
29	5.474	1377	1379	1382	rBV4	428	270	0.02%	0.002%
30	5.493	1382	1385	1386	rBV	514	282	0.02%	0.002%
31	5.555	1402	1404	1407	rBV	258	163	0.01%	0.001%
32	5.616	1410	1423	1450	rBV	542565	1083585	68.43%	8.463%
33	5.908	1504	1514	1525	rBV5	9133	18349	1.16%	0.143%
34	6.072	1551	1565	1593	rBV	349982	721760	45.58%	5.637%
35	6.284	1629	1631	1636	rVB3	656	328	0.02%	0.003%
36	6.307	1636	1638	1641	rBV	352	187	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V070221\
 Data File : V021600.D
 Acq On : 02 Jul 2021 16:06
 Operator : SY/MD
 Sample : VIBLK161
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.355	1651	1653	1656	rVB2	659	304	0.02%	0.002%
38	6.452	1680	1683	1687	rBV2	521	354	0.02%	0.003%
39	6.481	1689	1692	1695	rBV	350	216	0.01%	0.002%
40	6.506	1695	1700	1702	rBV2	295	192	0.01%	0.001%
41	6.516	1702	1703	1705	rBV2	387	175	0.01%	0.001%
42	6.558	1711	1716	1719	rBV2	238	208	0.01%	0.002%
43	6.577	1719	1722	1725	rBV2	372	265	0.02%	0.002%
44	6.628	1728	1738	1748	rBV6	4516	10599	0.67%	0.083%
45	6.854	1807	1808	1812	rVB2	626	275	0.02%	0.002%
46	6.889	1812	1819	1821	rBV3	379	306	0.02%	0.002%
47	6.989	1838	1850	1878	rBV	203202	372975	23.56%	2.913%
48	7.317	1941	1952	1973	rBV	756213	1305387	82.44%	10.195%
49	7.622	2037	2047	2068	rBV	140234	240050	15.16%	1.875%
50	7.812	2102	2106	2110	rBV4	668	551	0.03%	0.004%
51	7.879	2123	2127	2131	rVB2	501	356	0.02%	0.003%
52	7.915	2135	2138	2142	rVB3	387	326	0.02%	0.003%
53	7.944	2142	2147	2149	rBV3	612	600	0.04%	0.005%
54	8.037	2173	2176	2178	rBV3	415	255	0.02%	0.002%
55	8.088	2181	2192	2232	rBV	487517	868467	54.85%	6.783%
56	8.522	2323	2327	2328	rBV2	371	226	0.01%	0.002%
57	8.542	2331	2333	2335	rVB2	644	256	0.02%	0.002%
58	8.609	2348	2354	2357	rBV3	629	519	0.03%	0.004%
59	8.641	2360	2364	2366	rBV4	726	549	0.03%	0.004%
60	8.677	2372	2375	2377	rBV2	373	181	0.01%	0.001%
61	8.689	2377	2379	2380	rVV	309	169	0.01%	0.001%
62	8.715	2384	2387	2390	rVV3	269	169	0.01%	0.001%
63	8.773	2400	2405	2406	rBV	364	307	0.02%	0.002%
64	8.853	2416	2430	2471	rBV	797969	1298756	82.02%	10.143%
65	9.130	2513	2516	2517	rBV2	740	422	0.03%	0.003%
66	9.207	2538	2540	2542	rBV	364	197	0.01%	0.002%
67	9.255	2552	2555	2556	rBV	425	201	0.01%	0.002%
68	9.345	2580	2583	2586	rBV2	300	251	0.02%	0.002%
69	9.551	2643	2647	2652	rBV3	574	666	0.04%	0.005%
70	9.638	2668	2674	2678	rBV3	349	436	0.03%	0.003%
71	9.763	2711	2713	2716	rVB2	339	202	0.01%	0.002%
72	9.805	2724	2726	2728	rBV2	283	183	0.01%	0.001%
73	9.953	2768	2772	2777	rBV3	495	534	0.03%	0.004%
74	9.982	2777	2781	2783	rBV2	295	248	0.02%	0.002%
75	10.021	2788	2793	2796	rBV2	715	550	0.03%	0.004%
76	10.066	2805	2807	2811	rBV2	297	199	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
 Data File : VV021600.D
 Acq On : 02 Jul 2021 16:06
 Operator : SY/MD
 Sample : VIBLK161
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	10.123	2819	2825	2826	rBV2	1879	1415	0.09%	0.011%
78	10.217	2841	2854	2877	rBV	531565	826985	52.23%	6.459%
79	10.361	2897	2899	2905	rVB5	838	603	0.04%	0.005%
80	10.458	2921	2929	2936	rBV6	1763	3052	0.19%	0.024%
81	10.545	2950	2956	2960	rBV4	1678	1960	0.12%	0.015%
82	10.699	2999	3004	3011	rBV4	1015	1098	0.07%	0.009%
83	10.741	3014	3017	3030	rVB5	1053	1323	0.08%	0.010%
84	10.812	3036	3039	3041	rBV2	320	220	0.01%	0.002%
85	10.921	3064	3073	3083	rBV2	5432	8671	0.55%	0.068%
86	10.982	3089	3092	3095	rBV	332	293	0.02%	0.002%
87	11.027	3101	3106	3108	rBV2	1224	934	0.06%	0.007%
88	11.072	3118	3120	3122	rBV	434	240	0.02%	0.002%
89	11.252	3164	3176	3202	rBV	840675	1312015	82.86%	10.247%
90	11.422	3226	3229	3230	rBV3	1334	804	0.05%	0.006%
91	11.625	3280	3292	3313	rBV	760615	1211127	76.49%	9.459%
92	11.889	3371	3374	3375	rBV	437	265	0.02%	0.002%
93	11.924	3379	3385	3395	rVB6	2266	3583	0.23%	0.028%
94	12.001	3400	3409	3422	rBV8	2735	5286	0.33%	0.041%
95	12.287	3495	3498	3499	rBV2	466	276	0.02%	0.002%
96	12.590	3590	3592	3593	rBV2	583	292	0.02%	0.002%
97	12.757	3641	3644	3645	rBV2	445	211	0.01%	0.002%
98	12.889	3680	3685	3692	rVB5	2129	2509	0.16%	0.020%
99	13.107	3750	3753	3756	rBV3	778	607	0.04%	0.005%
100	13.342	3824	3826	3831	rVB2	644	321	0.02%	0.003%




Sum of corrected areas: 12803955

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
Data File : VV021600.D
Acq On : 02 Jul 2021 16:06
Operator : SY/MD
Sample : VIBLK161
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

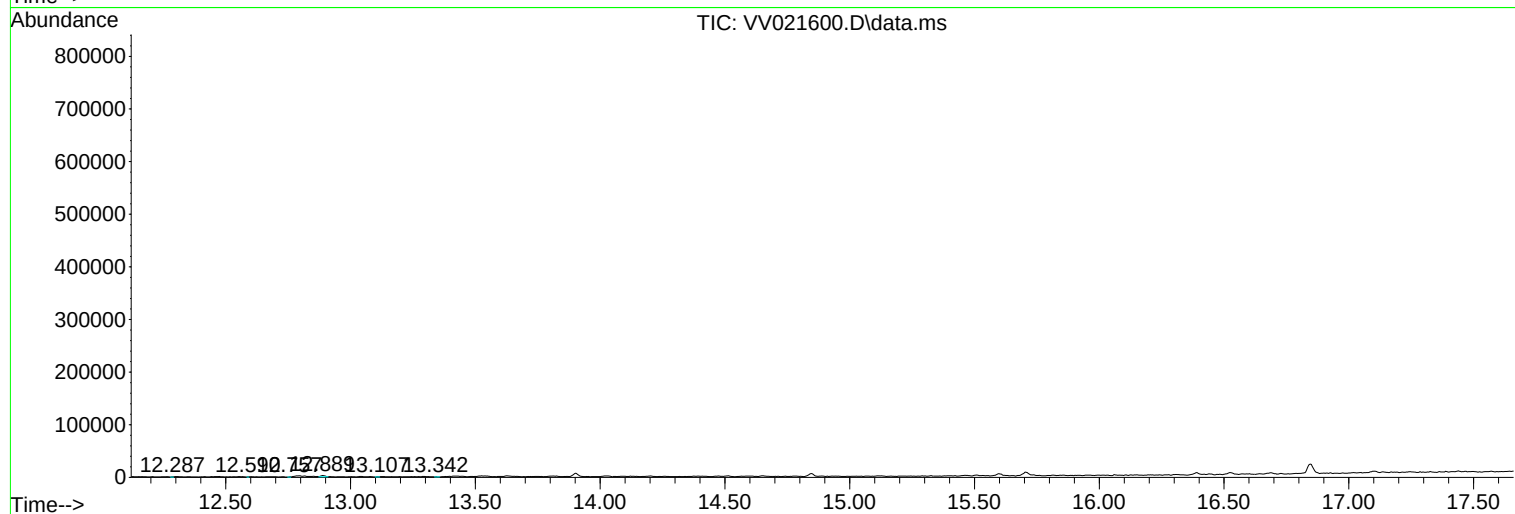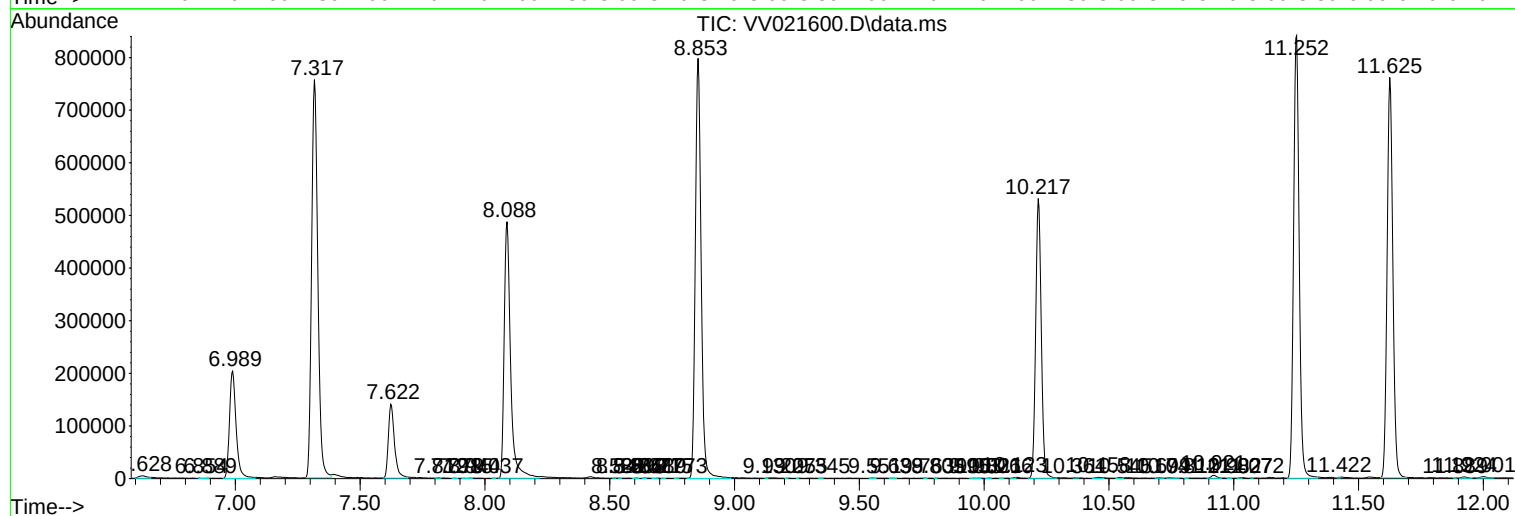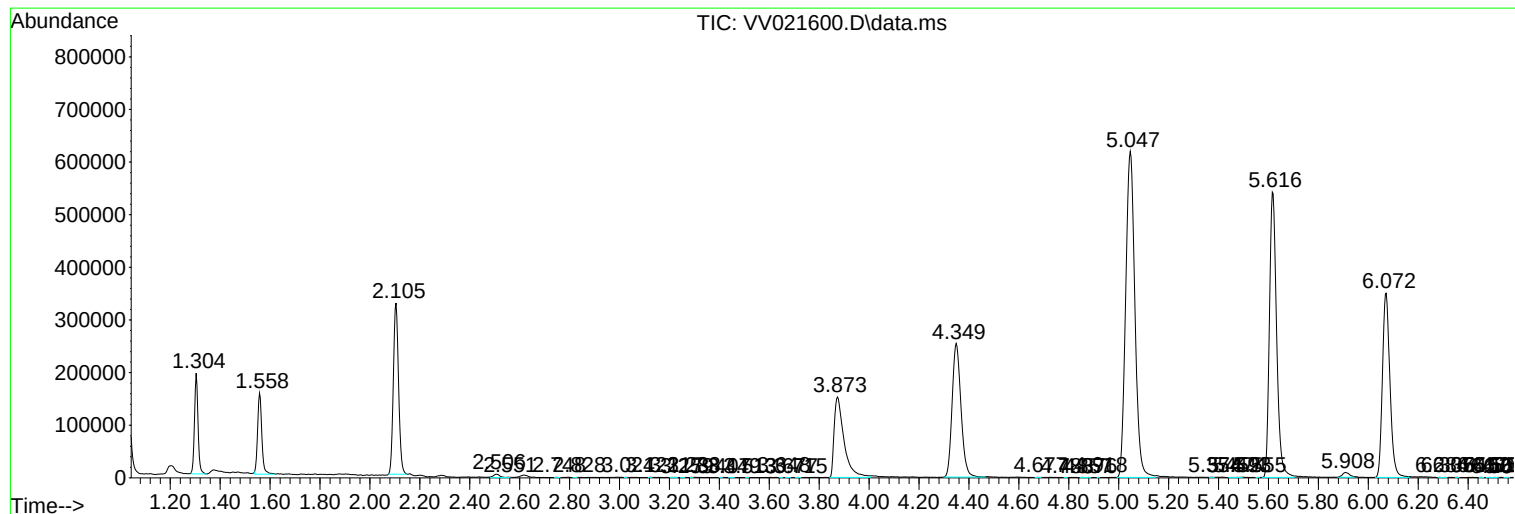

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
Data File : VV021600.D
Acq On : 02 Jul 2021 16:06
Operator : SY/MD
Sample : VIBLK161
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
Data File : VV021600.D
Acq On : 02 Jul 2021 16:06
Operator : SY/MD
Sample : VIBLK161
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
