
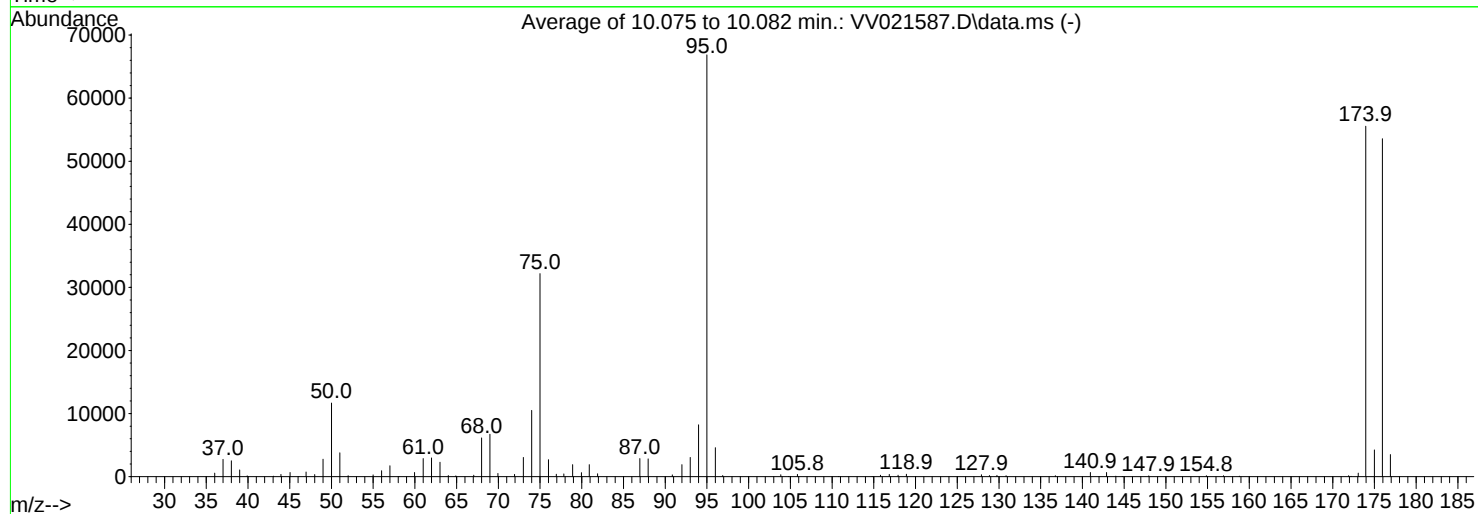


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070221\
 Data File : VV021587.D
 Acq On : 02 Jul 2021 08:59
 Operator : SY/MD
 Sample : BFB76
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB176

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis
 Last Update : Wed Jul 07 01:00:10 2021

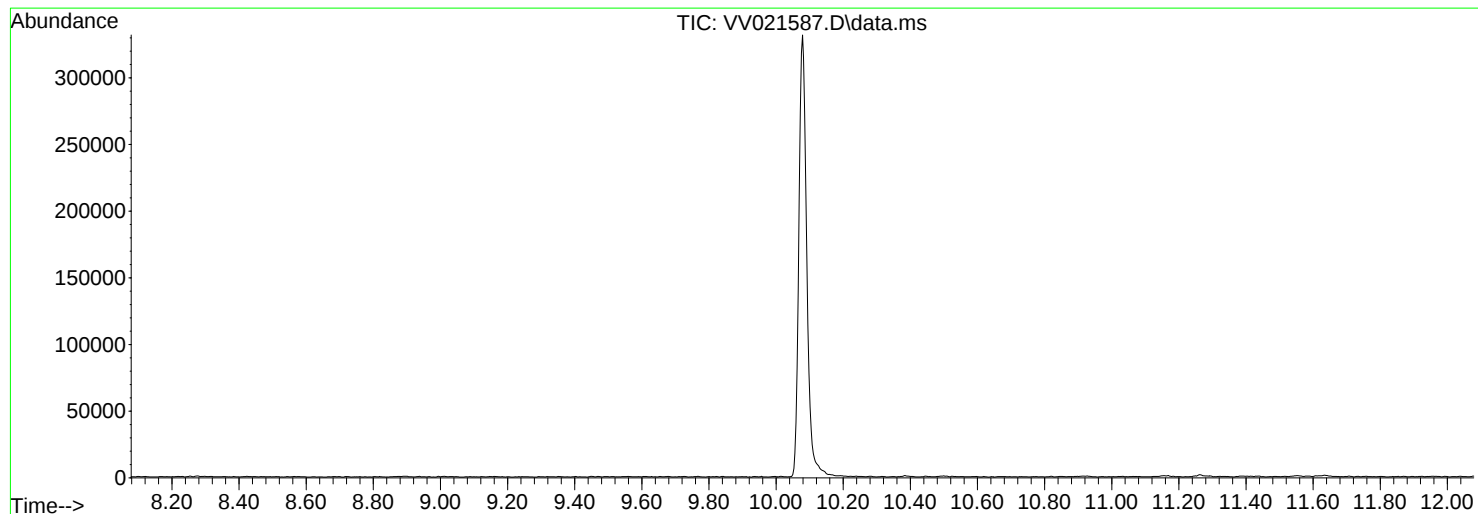

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	11667	PASS
75	95	30	80	48.1	32181	PASS
95	95	100	100	100.0	66867	PASS
96	95	5	9	6.9	4591	PASS
173	174	0.00	2	1.0	565	PASS
174	95	50	120	83.1	55547	PASS
175	174	5	9	7.6	4227	PASS
176	174	95	105	96.4	53568	PASS
177	176	5	10	6.5	3495	PASS

m/z	Abundance
39.90	260.0
41.00	133.0
43.90	457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB176

m/z	Abundance
36.00	550.0
37.00	2779.0
38.00	2674.0
39.00	1067.0
39.90	320.0
41.00	135.0
43.00	118.0
44.00	817.0
45.00	646.0
46.90	682.0
47.90	386.0
49.00	2800.0
50.00	11620.0
51.00	3638.0
52.00	201.0
55.00	243.0
56.00	929.0
57.00	1738.0
60.00	681.0
61.00	2892.0
62.00	3014.0
63.00	2291.0
63.90	200.0
64.90	134.0
67.20	178.0
68.00	6147.0
69.00	6932.0
69.90	532.0
72.00	335.0
73.00	3103.0
74.00	10663.0
75.00	32648.0
76.00	2613.0
77.00	435.0
77.80	392.0
78.90	1841.0
79.90	617.0
80.90	1894.0
81.90	474.0
87.00	2834.0
87.90	2587.0
90.90	257.0
92.00	1844.0
93.00	3066.0
94.00	8167.0
95.00	66960.0
96.00	4722.0
96.90	227.0
103.80	303.0
105.80	355.0
115.70	252.0
116.80	333.0
117.90	242.0
118.90	384.0
127.90	270.0
128.80	194.0
129.80	234.0
130.90	165.0
136.70	146.0
141.00	611.0
142.00	116.0
142.90	625.0
144.00	131.0
144.80	114.0
148.00	117.0
154.90	179.0
157.00	146.0
158.80	112.0
171.90	225.0
173.10	635.0
173.90	53384.0
175.00	4177.0
175.90	51544.0
176.90	3500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB176

m/z	Abundance
36.00	592.0
37.00	2844.0
38.00	2582.0
39.00	1100.0
40.00	419.0
41.10	134.0
43.10	100.0
44.00	835.0
45.10	667.0
47.00	741.0
48.00	312.0
49.00	2849.0
50.00	12133.0
51.00	3983.0
52.00	165.0
55.00	294.0
56.00	963.0
57.00	1769.0
59.90	698.0
61.00	2967.0
62.00	3025.0
63.00	2320.0
64.00	171.0
64.90	120.0
67.00	232.0
68.00	6323.0
69.00	7030.0
69.90	513.0
72.00	356.0
73.00	3114.0
74.00	10793.0
75.00	33088.0
76.00	2822.0
76.90	385.0
77.80	462.0
78.90	1970.0
79.90	641.0
80.90	1961.0
81.90	467.0
87.00	2902.0
87.90	2917.0
90.80	298.0
92.00	1952.0
93.00	3213.0
94.00	8525.0
95.00	68792.0
96.00	4755.0
96.90	195.0
103.80	315.0
105.80	351.0
114.80	109.0
115.80	254.0
116.80	359.0
117.90	256.0
118.90	402.0
127.90	322.0
128.90	179.0
129.80	218.0
130.90	165.0
136.70	154.0
141.00	681.0
142.90	663.0
144.00	107.0
147.90	123.0
154.90	163.0
156.90	150.0
158.80	111.0
171.90	210.0
173.10	563.0
173.90	57224.0
175.00	4419.0
175.90	55472.0
176.90	3644.0

Instrument :
MSVOA_V
ClientSampleId :
BFB176

m/z	Abundance
36.00	569.0
37.00	2584.0
38.00	2264.0
39.00	1015.0
40.00	467.0
41.00	112.0
44.00	802.0
45.00	630.0
46.10	116.0
47.00	763.0
48.10	292.0
49.00	2639.0
50.00	11249.0
51.00	3747.0
52.00	131.0
55.00	274.0
56.00	912.0
57.00	1653.0
58.10	112.0
59.90	639.0
61.00	2769.0
62.00	2839.0
63.00	2215.0
64.10	167.0
64.90	142.0
67.00	264.0
68.00	5930.0
69.00	6188.0
70.00	443.0
71.90	347.0
73.00	2933.0
74.00	10021.0
75.00	30808.0
76.00	2608.0
76.90	339.0
77.90	483.0
78.90	1886.0
80.00	619.0
80.90	1847.0
81.90	426.0
86.90	2836.0
88.00	2956.0
90.80	276.0
92.00	1911.0
93.00	2872.0
94.00	7945.0
95.00	64848.0
96.00	4295.0
96.90	146.0
103.90	336.0
104.80	112.0
105.90	328.0
110.80	105.0
115.90	214.0
116.90	373.0
117.90	225.0
118.90	345.0
127.90	346.0
128.90	148.0
129.70	204.0
130.80	148.0
136.80	160.0
140.90	676.0
142.90	670.0
147.90	127.0
154.80	136.0
156.80	156.0
172.20	187.0
173.00	496.0
174.00	56032.0
175.00	4085.0
176.00	53688.0
176.90	3341.0

Instrument :
MSVOA_V
ClientSampleId :
BFB176