
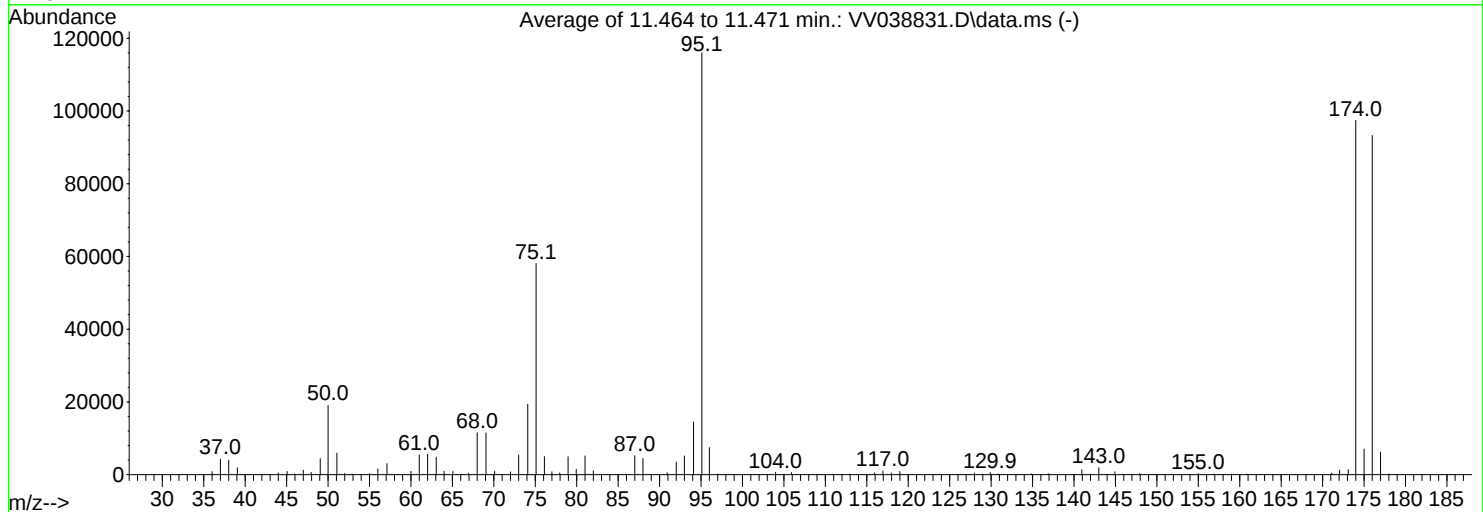


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV070225\
Data File : VV038831.D
Acq On : 02 Jul 2025 08:46
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V070225W.M
Title : SW846 8260
Last Update : Thu Jul 03 02:44:44 2025

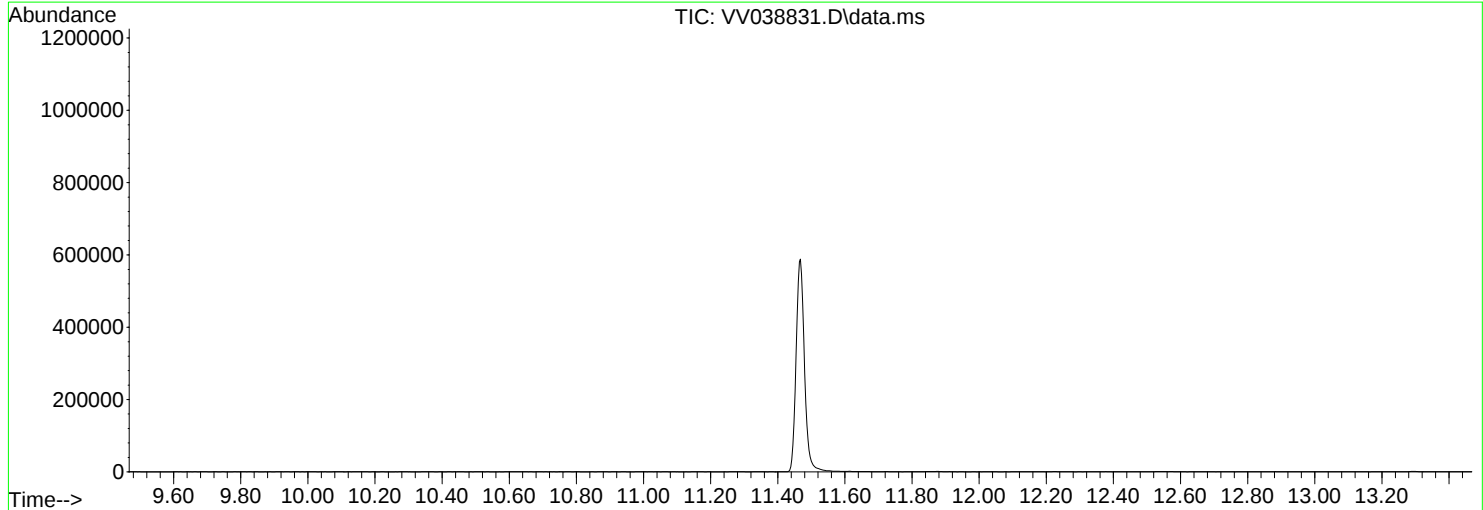

AutoFind: Scans 3242, 3243, 3244; Background Corrected with Scan 3229

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	19064	PASS
75	95	30	60	50.1	58083	PASS
95	95	100	100	100.0	116000	PASS
96	95	5	9	6.4	7452	PASS
173	174	0.00	2	1.4	1354	PASS
174	95	50	100	84.0	97408	PASS
175	174	5	9	7.2	7048	PASS
176	174	95	101	95.8	93307	PASS
177	176	5	9	6.6	6203	PASS