

Data File : VV011829.D
Acq On : 03 Jul 2019 14:31
Operator : SY/MD
Sample : K3598-02DL 20X
Misc : 26ML/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAM80DL

Quant Time: Jul 04 00:28:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 23:52:56 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	192575	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	184359	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	80226	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	50647	3.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.20%
7) Chloroethane-d5	1.58	69	41636	4.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.60%
11) 1,1-Dichloroethene-d2	2.13	63	74264	2.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.60%#
20) 2-Butanone-d5	3.95	46	140420	43.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.74%
24) Chloroform-d	4.40	84	100114	3.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.00%
26) 1,2-Dichloroethane-d4	5.08	65	56075	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.00%
32) Benzene-d6	5.10	84	201936	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.40%
36) 1,2-Dichloropropane-d6	6.12	67	63661	4.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.40%
41) Toluene-d8	7.36	98	171306	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
43) trans-1,3-Dichloropropene-	7.67	79	19985	3.79	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.80%
46) 2-Hexanone-d5	8.14	63	103687	42.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.28%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	41119	3.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	76.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	63334	4.47	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.40%


Target Compounds					Qvalue
47) Tetrachloroethene	8.02	164	128485	11.434 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV011829.D
Acq On : 03 Jul 2019 14:31
Operator : SY/MD
Sample : K3598-02DL 20X
Misc : 26ML/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAM80DL

Quant Time: Jul 04 00:28:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 23:52:56 2019
Response via : Initial Calibration

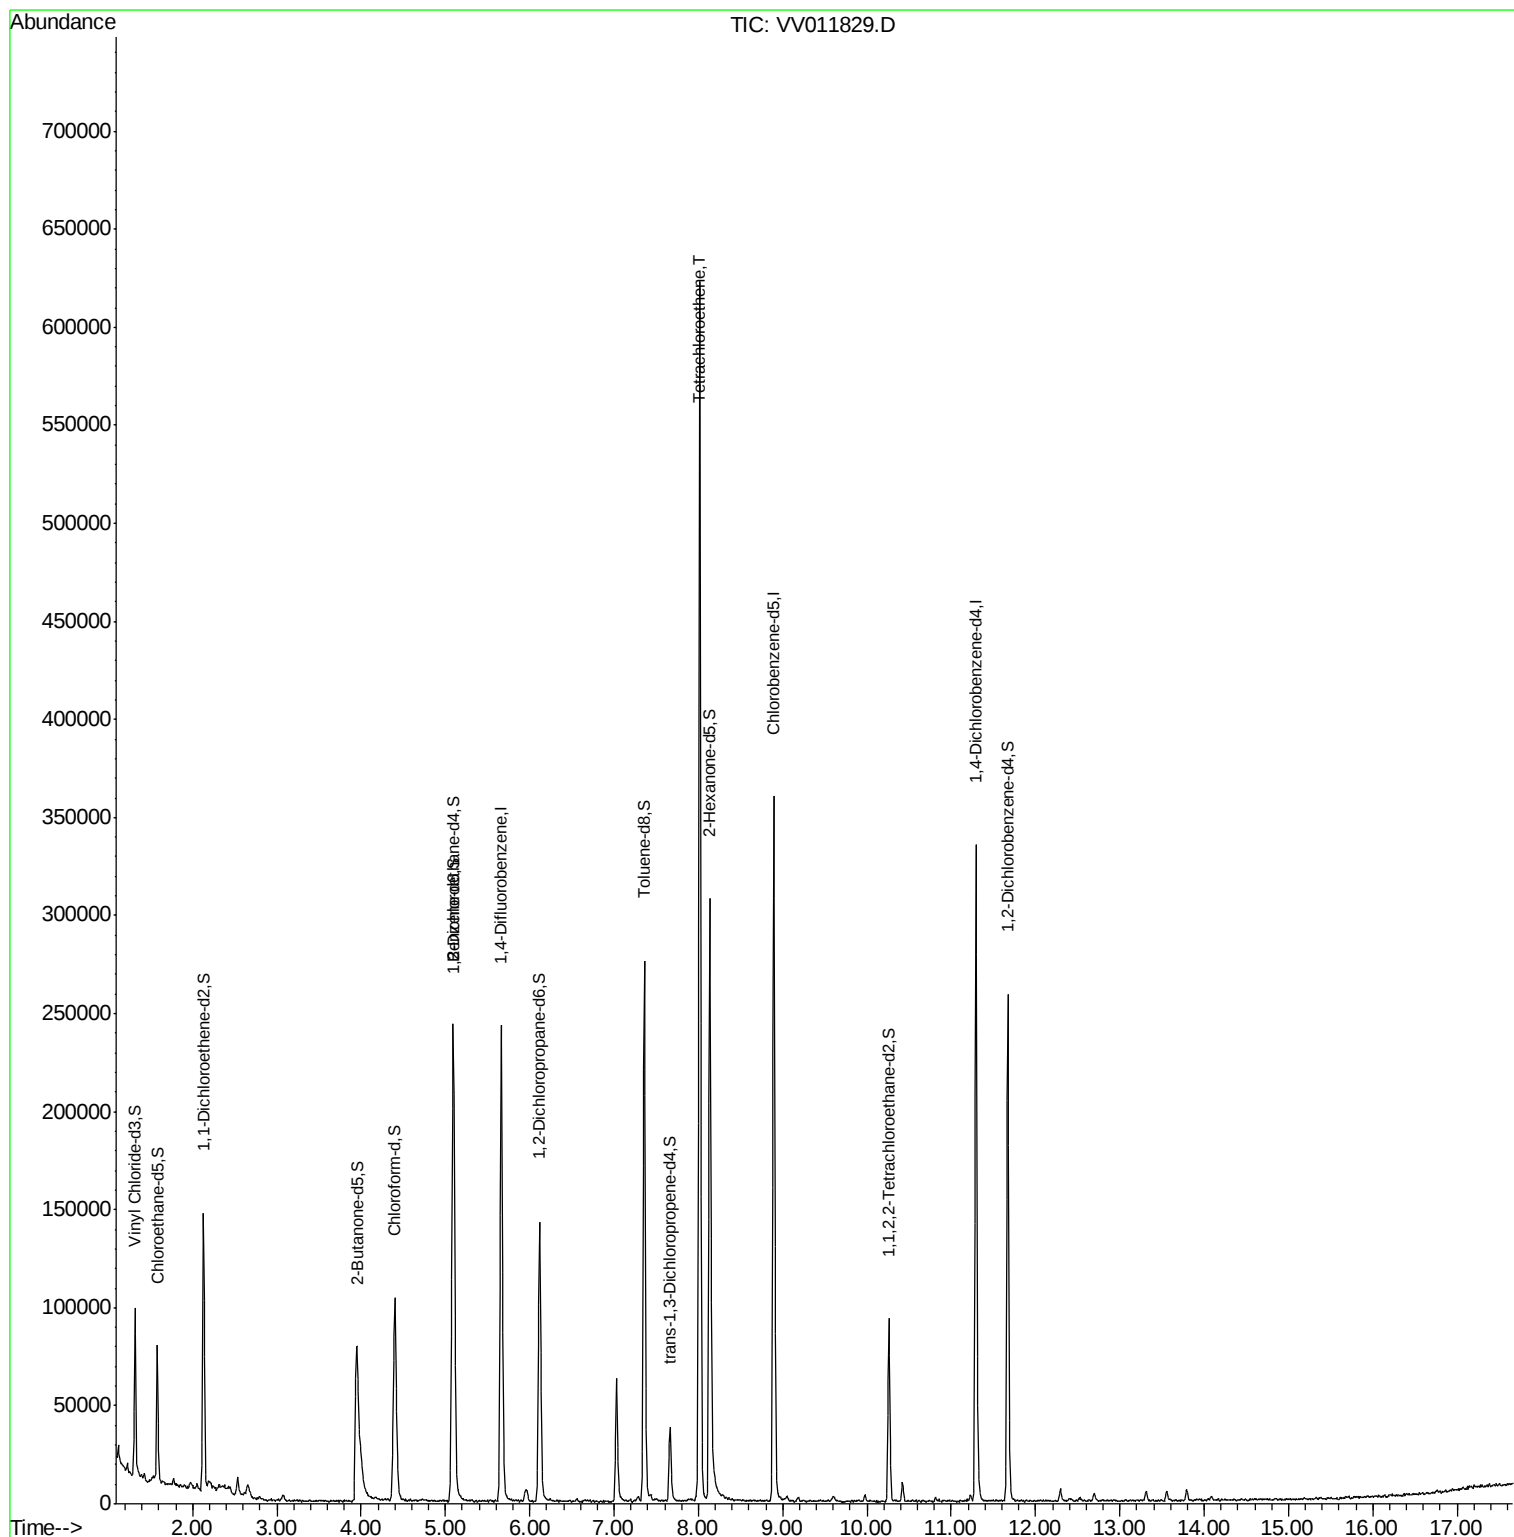

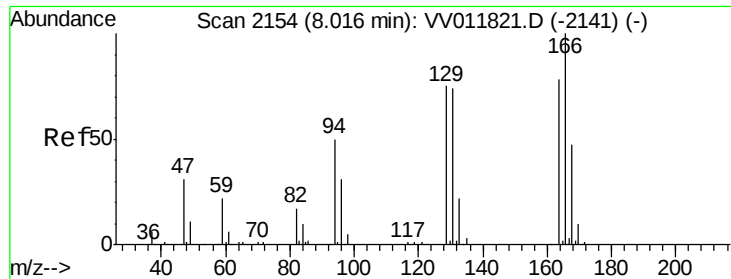

#47

Tetrachloroethene

Concen: 11.434 ug/L


RT: 8.02 min Scan# 2154

Delta R.T. -0.00 min

Lab File: VV011829.D

Acq: 03 Jul 2019 14:31

Instrument :
MSVOA_V
ClientSampleId :
GAM80DL

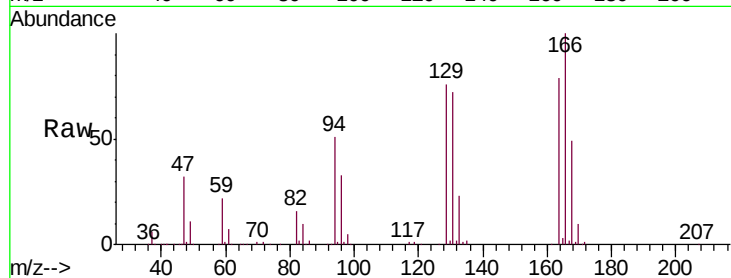

Tgt Ion:	164	Resp:	128485
Ion	Ratio	Lower	Upper
164	100		
129	95.8	65.7	121.9
131	91.2	63.2	117.4
166	125.9	85.8	159.3

