


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV070319\
Data File : VV011820.D
Acq On : 03 Jul 2019 09:16
Operator : SY/MD
Sample : BFB60
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB60

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jul 05 00:59:17 2019

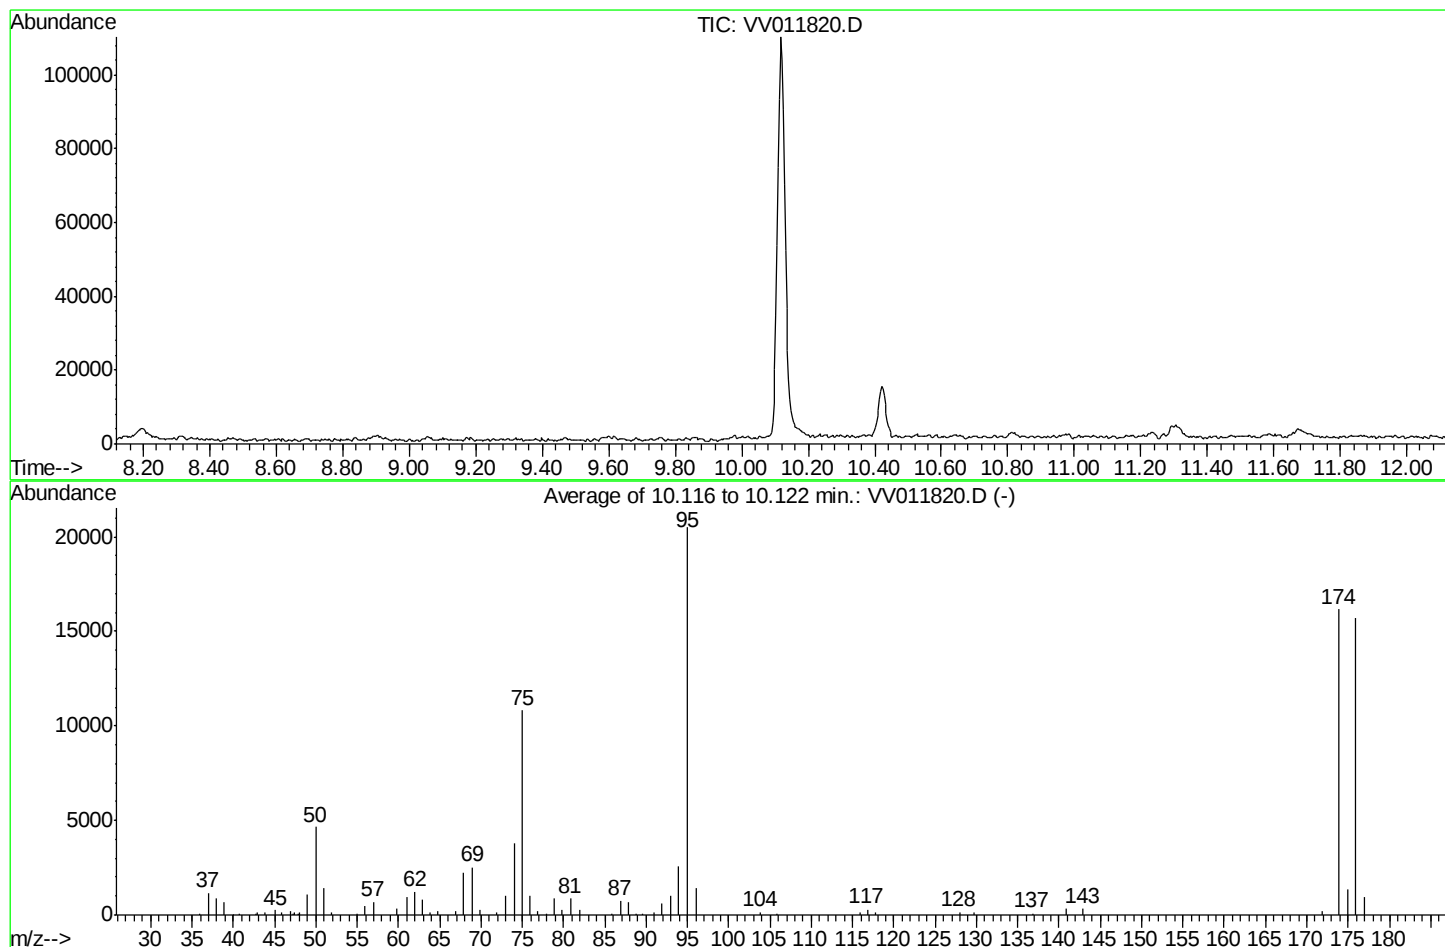

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	4663	PASS
75	95	30	80	52.8	10830	PASS
95	95	100	100	100.0	20501	PASS
96	95	5	9	6.8	1391	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.8	16162	PASS
175	174	5	9	8.4	1354	PASS
176	174	95	101	97.4	15737	PASS
177	176	5	9	6.1	964	PASS

m/z	Abundance
36.00	603.0
36.80	155.0
37.80	232.0
40.00	215.0
40.70	103.0
44.00	429.0
55.30	114.0
62.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	677.0
37.00	1277.0
37.90	1189.0
38.90	672.0
40.00	237.0
40.90	158.0
43.00	134.0
43.80	608.0
45.10	247.0
45.90	101.0
46.90	214.0
47.20	188.0
48.10	207.0
48.90	1088.0
50.00	4733.0
51.00	1505.0
52.00	140.0
54.90	140.0
56.00	463.0
57.00	735.0
59.80	352.0
61.00	1013.0
62.00	1285.0
62.90	915.0
63.80	197.0
64.70	208.0
66.90	159.0
67.90	2184.0
69.00	2494.0
69.80	260.0
71.90	124.0
73.00	1026.0
74.00	3894.0
75.00	10883.0
76.00	1082.0
77.00	180.0
78.00	173.0
78.90	908.0
79.90	278.0
80.80	822.0
81.90	239.0
86.90	741.0
88.00	741.0
88.80	106.0
89.50	119.0
90.90	129.0
91.90	672.0
92.90	1036.0
94.00	2600.0
95.00	20000.0
96.00	1415.0
103.90	150.0
105.80	141.0
115.80	127.0
116.80	266.0
117.80	105.0
127.90	162.0
129.80	118.0
136.80	101.0
140.80	309.0
142.90	365.0
171.90	149.0
173.90	15965.0
174.90	1407.0
175.90	15041.0
176.90	952.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	684.0
37.00	1406.0
37.90	1147.0
38.90	667.0
40.00	214.0
40.90	175.0
42.70	111.0
42.90	115.0
43.90	584.0
45.10	276.0
45.90	125.0
46.90	231.0
47.40	211.0
48.00	201.0
48.90	1110.0
50.00	4739.0
51.00	1451.0
52.00	158.0
55.00	130.0
56.00	457.0
57.00	682.0
59.80	354.0
61.00	998.0
62.00	1286.0
62.90	941.0
63.80	139.0
64.80	183.0
66.90	190.0
67.90	2319.0
69.00	2620.0
69.90	277.0
72.00	128.0
73.00	1008.0
74.00	3902.0
75.00	11175.0
76.00	1021.0
76.90	206.0
78.00	131.0
78.90	941.0
79.80	259.0
80.80	861.0
81.90	259.0
85.80	113.0
86.90	759.0
87.80	672.0
88.80	101.0
90.90	149.0
91.90	636.0
92.90	1078.0
93.90	2625.0
95.00	21272.0
96.00	1442.0
103.90	170.0
105.90	118.0
115.80	131.0
116.80	305.0
117.70	113.0
128.00	174.0
129.70	160.0
140.80	334.0
142.90	346.0
171.80	171.0
173.90	16656.0
174.90	1417.0
175.90	16275.0
176.90	991.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	746.0
37.00	1294.0
38.00	1034.0
38.90	607.0
39.90	202.0
40.90	170.0
42.70	130.0
43.00	124.0
43.90	519.0
45.10	272.0
45.90	119.0
46.90	252.0
47.30	219.0
47.80	233.0
48.90	1036.0
50.00	4517.0
51.00	1348.0
51.90	133.0
55.90	409.0
57.00	636.0
59.90	297.0
61.00	924.0
62.00	1114.0
62.90	834.0
64.80	141.0
66.90	174.0
67.90	2256.0
69.00	2412.0
69.90	289.0
72.00	136.0
73.00	1001.0
74.00	3646.0
75.00	10433.0
75.90	941.0
76.80	218.0
78.90	831.0
79.80	243.0
80.90	867.0
81.90	257.0
86.90	788.0
87.80	574.0
90.90	143.0
91.90	573.0
92.90	1029.0
93.90	2463.0
95.00	20232.0
96.00	1318.0
103.80	162.0
115.90	124.0
116.80	289.0
117.70	111.0
128.00	157.0
129.70	165.0
136.80	106.0
140.80	322.0
142.90	289.0
171.70	232.0
173.90	15866.0
175.00	1238.0
175.90	15897.0
176.90	951.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60