

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
 Data File : VV031638.D
 Acq On : 03 Jul 2023 15:39
 Operator : SY/MD
 Sample : 03472-21ME
 Misc : 4.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46R2ME

Quant Time: Jul 04 07:09:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 04 07:06:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	222129	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	224017	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	122026	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	53229	36.006	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.020%
7) Chloroethane-d5	1.503	69	27072	20.988	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	41.980%#
11) 1,1-Dichloroethene-d2	2.040	65	28346	37.204	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.400%
21) 2-Butanone-d5	3.806	46	118590	99.068	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.070%
24) Chloroform-d	4.253	84	142024	38.360	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.720%
26) 1,2-Dichloroethane-d4	4.944	65	97407	42.050	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.100%
32) Benzene-d6	4.963	84	230942	36.625	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.260%
36) 1,2-Dichloropropane-d6	5.992	67	90171	40.347	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.700%
41) Toluene-d8	7.249	98	185503	32.059	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	64.120%#
43) trans-1,3-Dichloroprop...	7.561	79	40949	37.585	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.180%
47) 2-Hexanone-d5	8.043	63	82474	93.464	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.460%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	149234	44.239	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.480%
66) 1,2-Dichlorobenzene-d4	11.571	152	93260	40.094	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.180%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.388	43	13098	6.586	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV070323\
Data File : VV031638.D
Acq On : 03 Jul 2023 15:39
Operator : SY/MD
Sample : 03472-21ME
Misc : 4.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46R2ME

Quant Time: Jul 04 07:09:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 04 07:06:08 2023
Response via : Initial Calibration

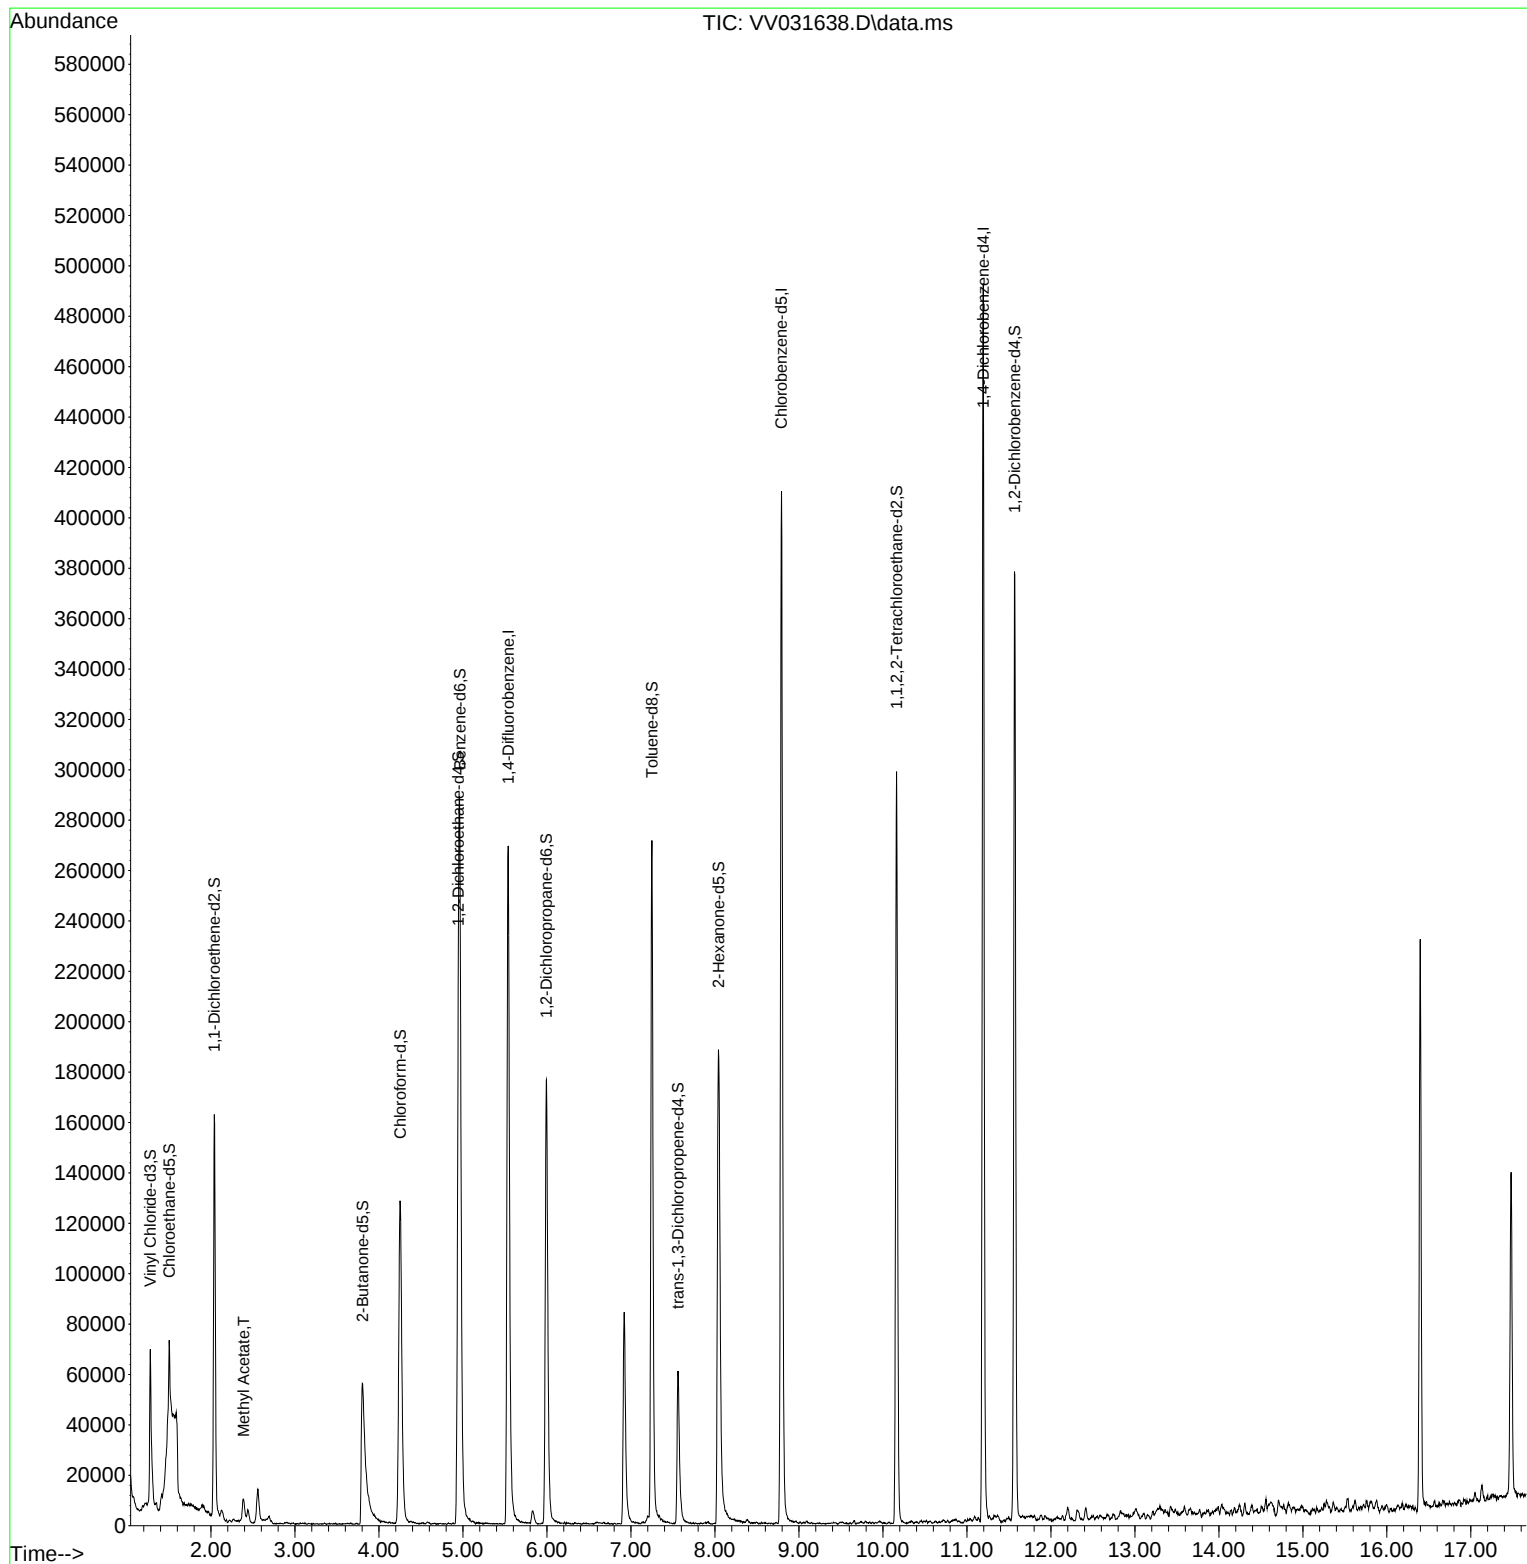

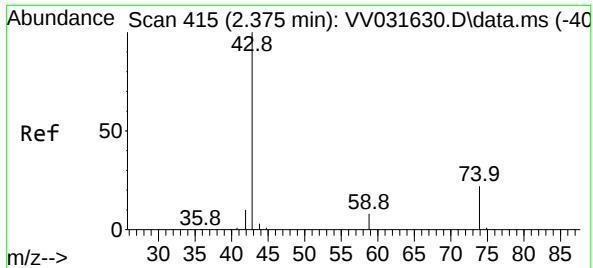

#15
Methyl Acetate
Concen: 6.586 ug/L
RT: 2.388 min Scan# 41
Delta R.T. 0.013 min
Lab File: VV031638.D
Acq: 03 Jul 2023 15:39

Instrument :
MSVOA_V
ClientSampleId :
A46R2ME

Tgt Ion: 43 Resp: 13098
Ion Ratio Lower Upper
43 100
74 21.2 17.8 26.6

